

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061220\
 Data File : BN010854.D
 Acq On : 12 Jun 2020 22:31
 Operator : CG/JU
 Sample : L2988-05DL 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE132D4-20200608DL

Quant Time: Jun 13 01:33:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 12 11:11:17 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	2679	0.40	ng	0.00
7) Naphthalene-d8	10.30	136	9505	0.40	ng	0.00
13) Acenaphthene-d10	14.17	164	5232	0.40	ng	-0.01
19) Phenanthrene-d10	16.92	188	11180	0.40	ng	0.00
27) Chrysene-d12	21.13	240	10667	0.40	ng	0.00
34) Perylene-d12	23.28	264	11662	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.21	112	386	0.07	ng	0.00
5) Phenol-d6	6.75	99	250	0.04	ng	0.00
8) Nitrobenzene-d5	8.69	82	1230	0.17	ng	0.00
11) 2-Methylnaphthalene-d10	11.90	152	2307	0.16	ng	0.00
14) 2,4,6-Tribromophenol	15.68	330	303	0.16	ng	0.00
15) 2-Fluorobiphenyl	12.80	172	3718	0.18	ng	0.00
25) Fluoranthene-d10	18.96	212	5109	0.17	ng	0.00
29) Terphenyl-d14	19.57	244	5303	0.21	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.22	88	3299	1.257	ng	99
32) Bis(2-ethylhexyl)phthalate	21.07	149	520	0.050	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061220\
Data File : BN010854.D
Acq On : 12 Jun 2020 22:31
Operator : CG/JU
Sample : L2988-05DL 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE132D4-20200608DL

Quant Time: Jun 13 01:33:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 12 11:11:17 2020
Response via : Initial Calibration

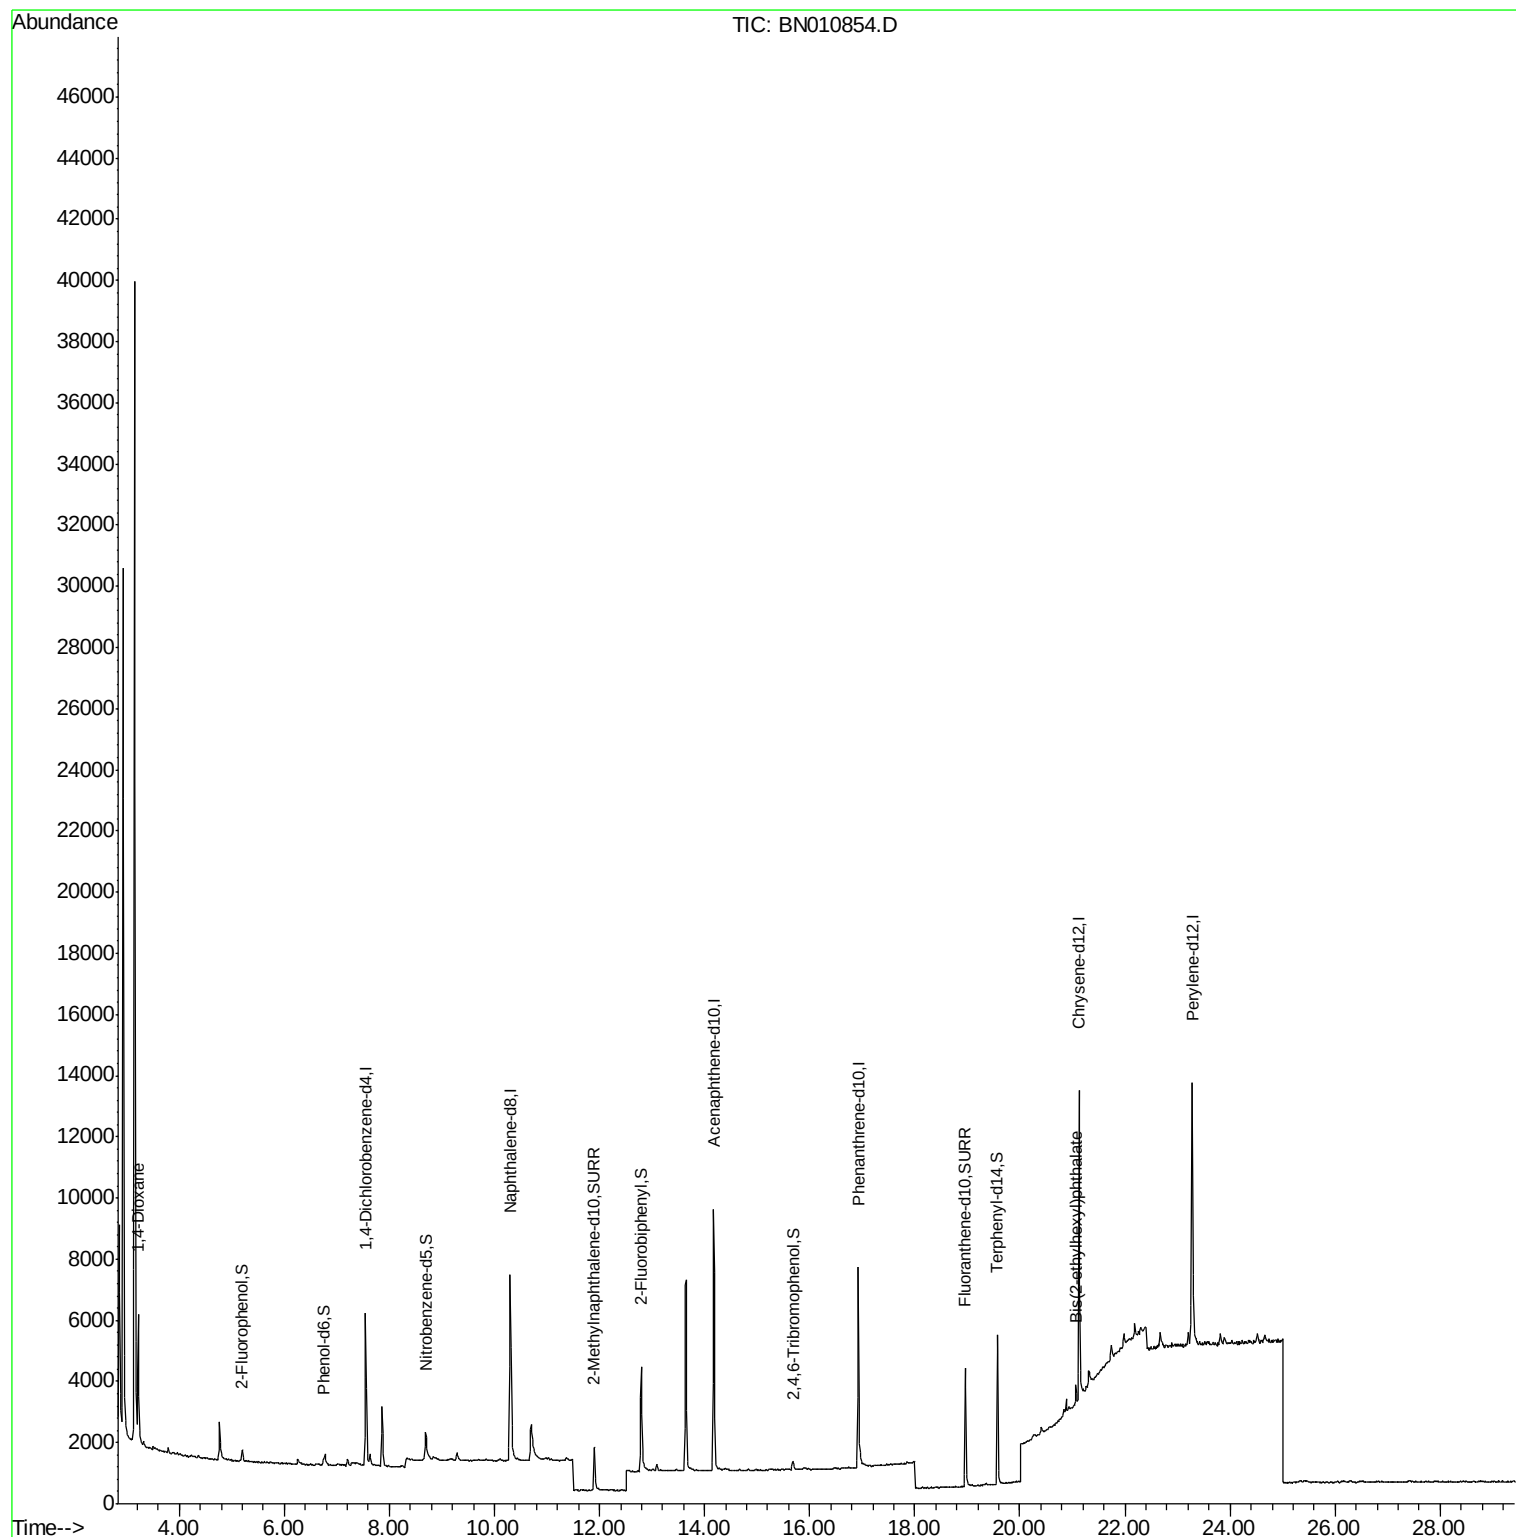

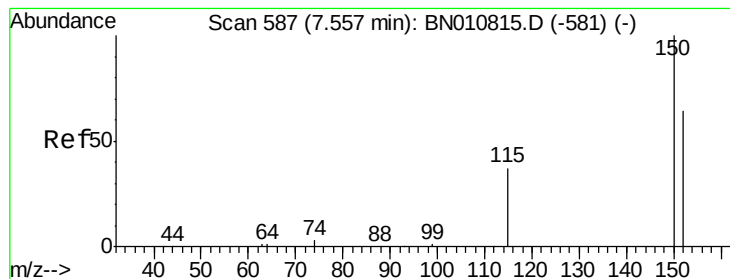


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.55 min Scan# 586
Delta R.T. -0.01 min
Lab File: BN010854.D
Acq: 12 Jun 2020 22:31

Instrument :
BNA_N
ClientSampleId :
RE132D4-20200608DL

Tot Ion:152 Resp: 2679
Ion Ratio Lower Upper
152 100
150 158.7 123.8 185.6
115 64.5 49.2 73.8

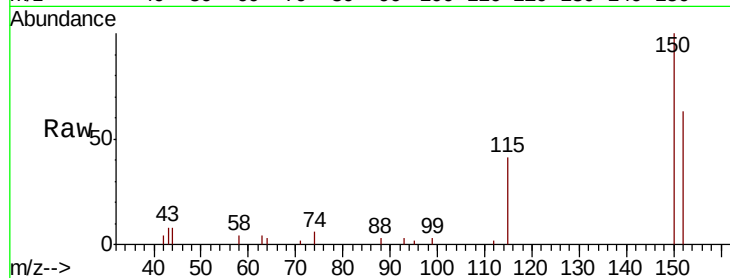


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

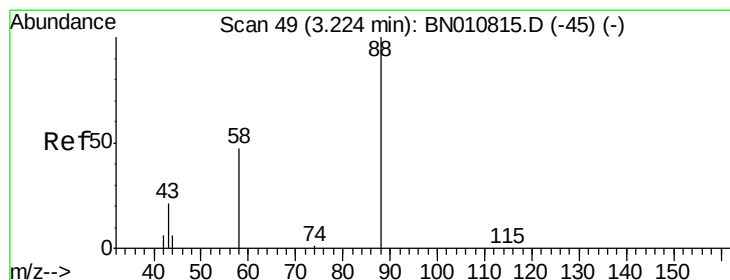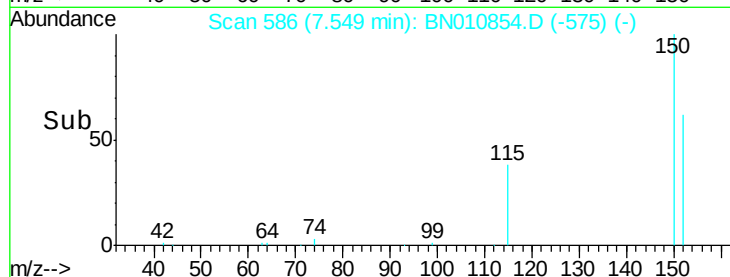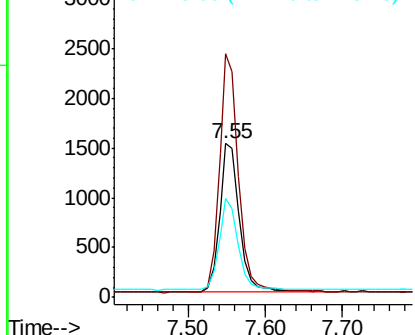



#2


1,4-Dioxane
Concen: 1.257 ng
RT: 3.22 min Scan# 48
Delta R.T. -0.01 min
Lab File: BN010854.D
Acq: 12 Jun 2020 22:31

Tgt Ion: 88 Resp: 3299
Ion Ratio Lower Upper
88 100
58 46.7 38.2 57.4
43 18.8 15.1 22.7

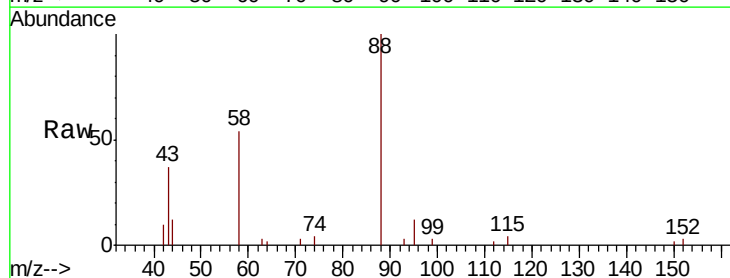

Abundance Ion 88.00 (87.70 to 88.70): BNC
Ion 58.00 (57.70 to 58.70): BNC
Ion 43.00 (42.70 to 43.70): BNC

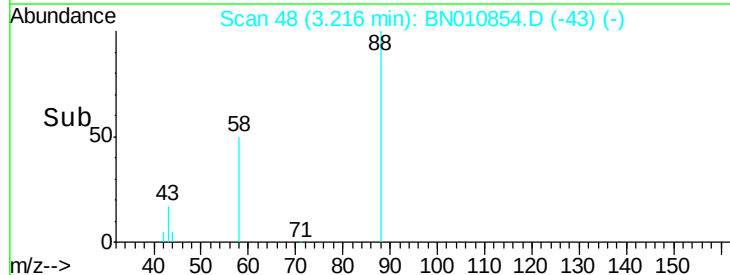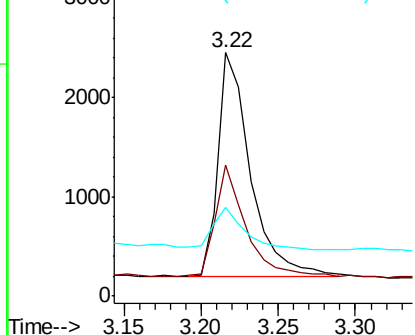

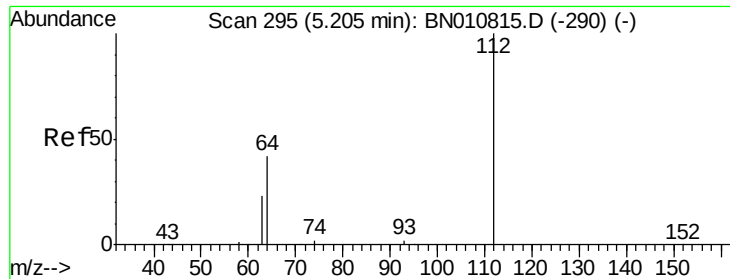

#4

2-Fluorophenol

Concen: 0.075 ng

RT: 5.21 min Scan# 295

Delta R.T. -0.00 min

Lab File: BN010854.D

Acq: 12 Jun 2020 22:31

Instrument :

BNA_N

ClientSampleId :

RE132D4-20200608DL


Tot Ion: 112 Resp: 386

Ion Ratio Lower Upper

112 100

64 46.6 37.4 56.0

63 26.9 22.2 33.4

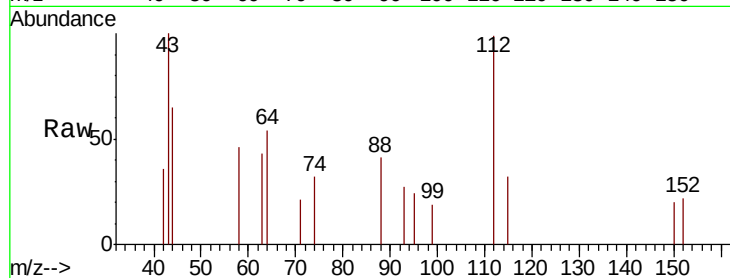

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BN0

Ion 63.00 (62.70 to 63.70): BN0

5.21

300

200

100



0

5.10

5.20

5.30

Time-->

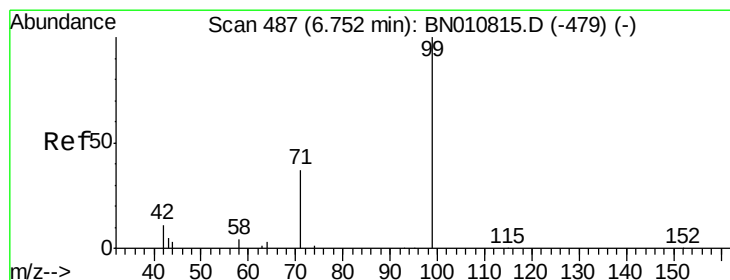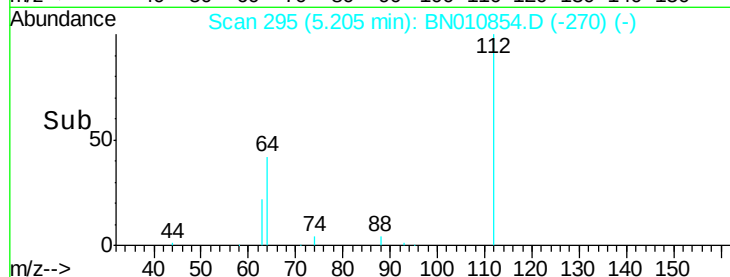

#5

Phenol-d6

Concen: 0.041 ng

RT: 6.75 min Scan# 487

Delta R.T. -0.00 min

Lab File: BN010854.D

Acq: 12 Jun 2020 22:31


Tgt Ion: 99 Resp: 250

Ion Ratio Lower Upper

99 100

42 19.6 11.1 16.7#

71 43.6 31.4 47.2

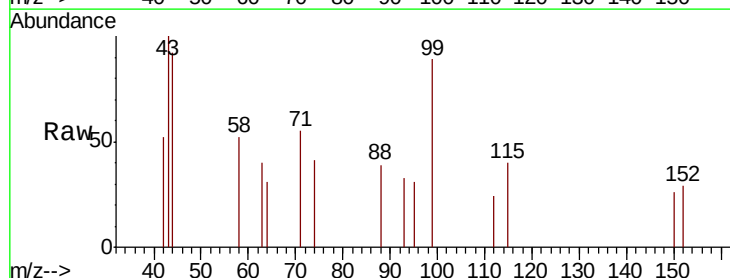

Abundance Ion 99.00 (98.70 to 99.70): BN0

Ion 42.00 (41.70 to 42.70): BN0

Ion 71.00 (70.70 to 71.70): BN0

6.75

200

150

100


50


0

6.70

6.80

Time-->

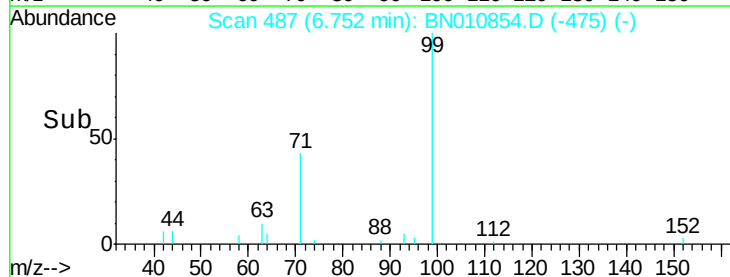

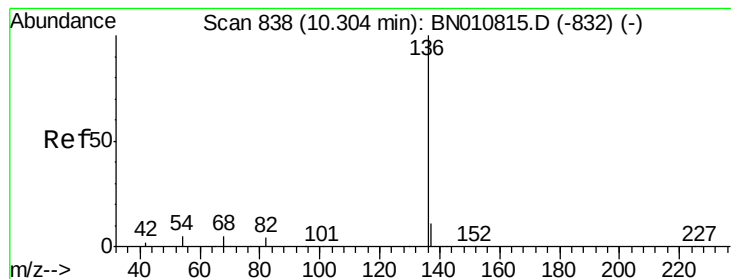

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.30 min Scan# 838

Delta R.T. -0.00 min

Lab File: BN010854.D

Acq: 12 Jun 2020 22:31

Instrument :

BNA_N

ClientSampleId :

RE132D4-20200608DL

Tot Ion:136 Resp: 9505


Ion Ratio Lower Upper

136 100

137 12.0 9.7 14.5

54 4.7 4.9 7.3#

68 5.5 4.7 7.1






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

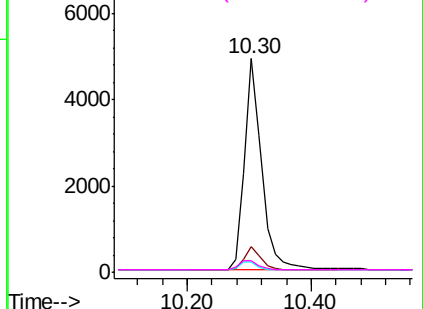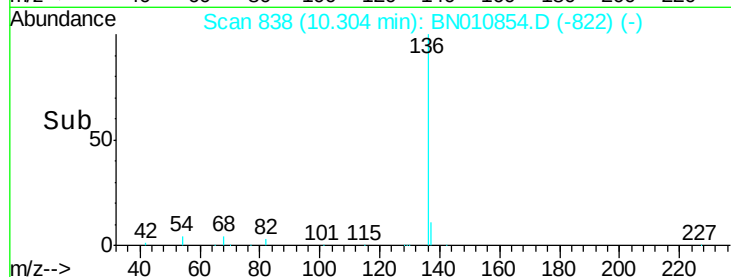

#8

Nitrobenzene-d5

Concen: 0.175 ng

RT: 8.69 min Scan# 711

Delta R.T. -0.00 min

Lab File: BN010854.D

Acq: 12 Jun 2020 22:31


Tgt Ion: 82 Resp: 1230

Ion Ratio Lower Upper

82 100

128 48.3 35.4 53.0



54 39.0 28.2 42.4




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC

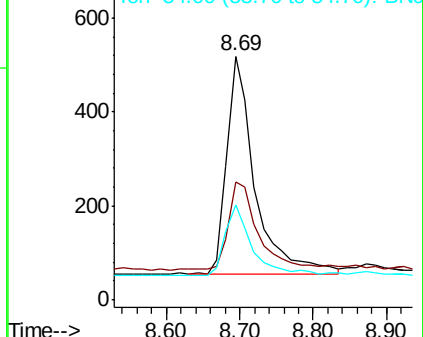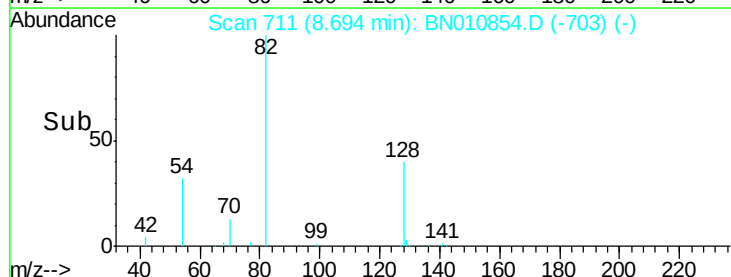

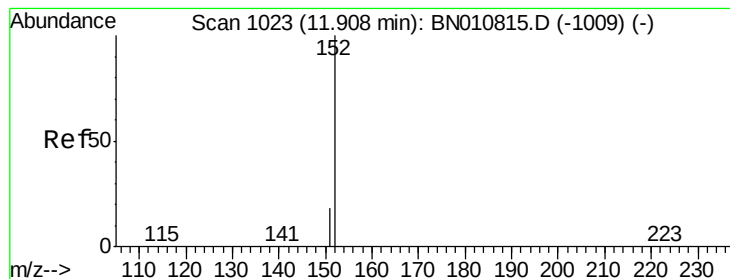

#11

2-Methylnaphthalene-d10

Concen: 0.156 ng

RT: 11.90 min Scan# 1021

Delta R.T. -0.00 min

Lab File: BN010854.D

Acq: 12 Jun 2020 22:31

Instrument :

BNA_N

ClientSampleId :


RE132D4-20200608DL

Tot Ion:152 Resp: 2307

Ion Ratio Lower Upper

152 100

151 19.5 15.3 22.9

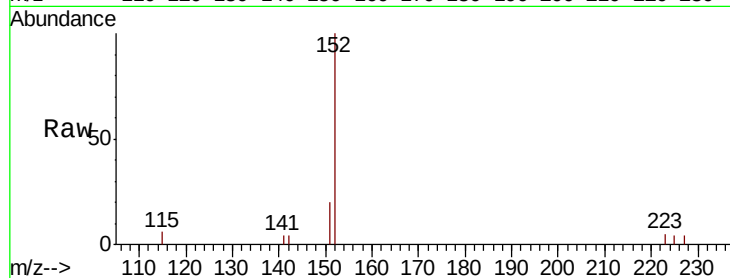

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E



11.90

1000

500

0

Time--> 11.80 11.90 12.00 12.10

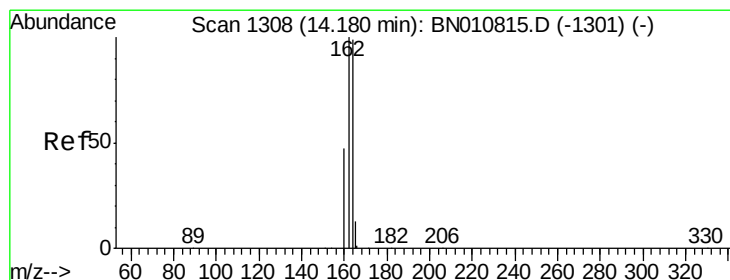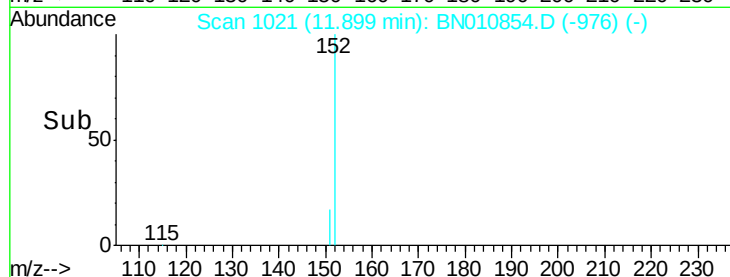

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.17 min Scan# 1307

Delta R.T. -0.01 min

Lab File: BN010854.D

Acq: 12 Jun 2020 22:31


Tgt Ion:164 Resp: 5232

Ion Ratio Lower Upper

164 100

162 106.4 81.0 121.6

160 51.2 38.9 58.3

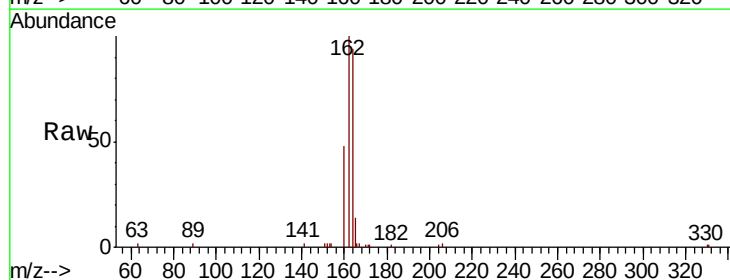

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

14.17

4000


3000


2000

1000

0

Time--> 14.10 14.20 14.30




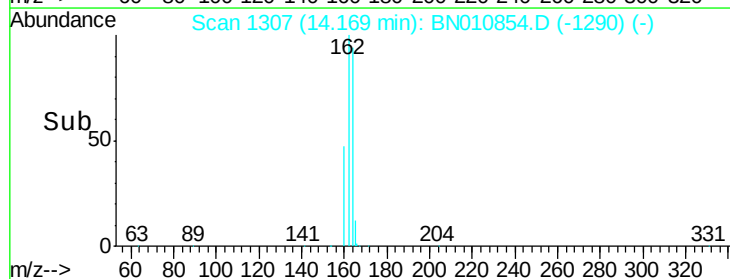


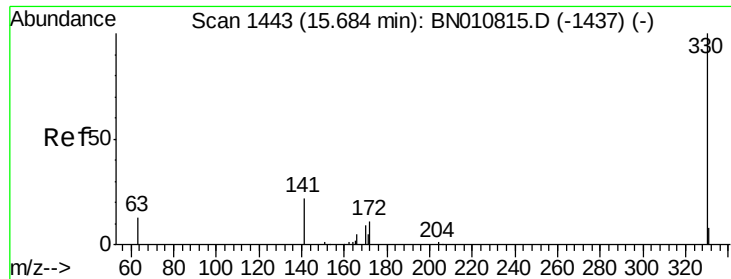

#14
 2,4,6-Tribromophenol
 Concen: 0.162 ng
 RT: 15.68 min Scan# 1443
 Delta R.T. -0.00 min
 Lab File: BN010854.D
 Acq: 12 Jun 2020 22:31




Instrument :
 BNA_N
 ClientSampleId :
 RE132D4-20200608DL


Tot Ion:330 Resp: 303
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 40.3 33.2 49.8

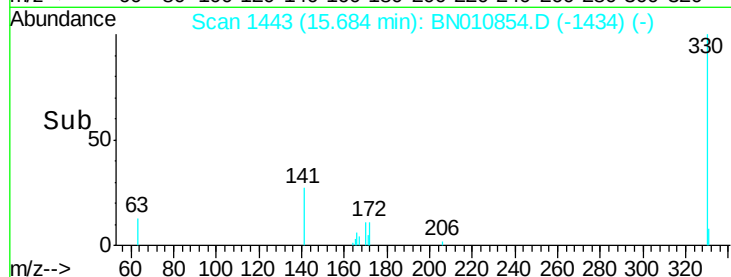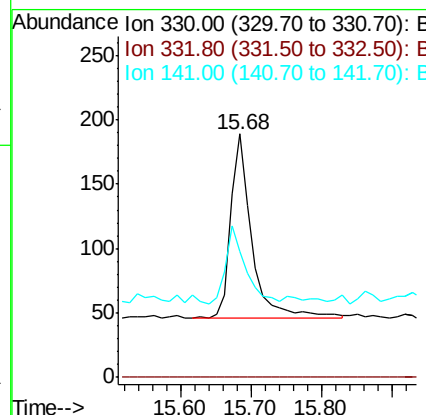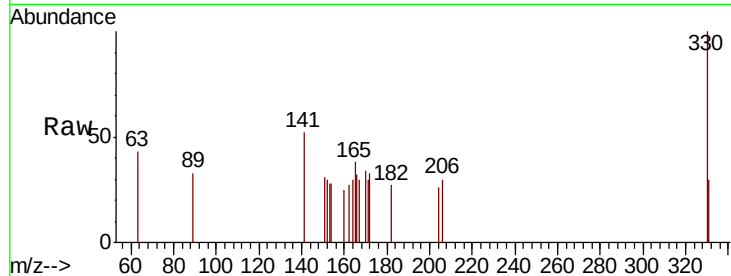

#15
 2-Fluorobiphenyl
 Concen: 0.180 ng
 RT: 12.80 min Scan# 1184
 Delta R.T. -0.00 min
 Lab File: BN010854.D
 Acq: 12 Jun 2020 22:31

Tgt Ion:172 Resp: 3718
 Ion Ratio Lower Upper
 172 100
 171 35.5 28.5 42.7
 170 24.2 19.7 29.5

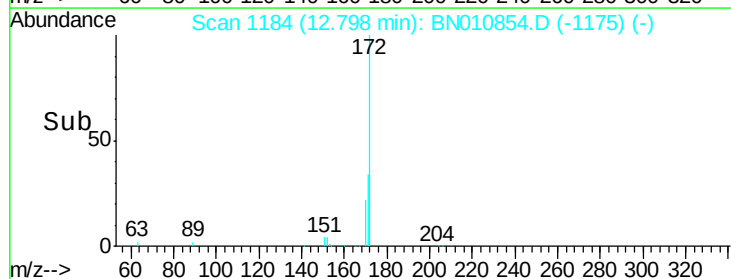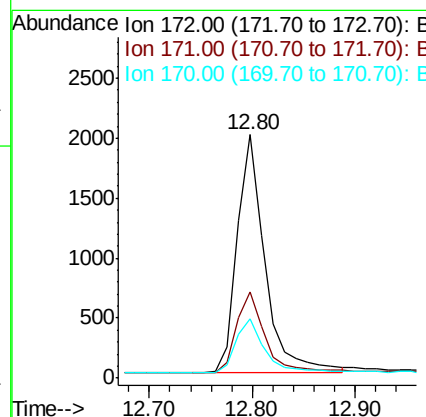

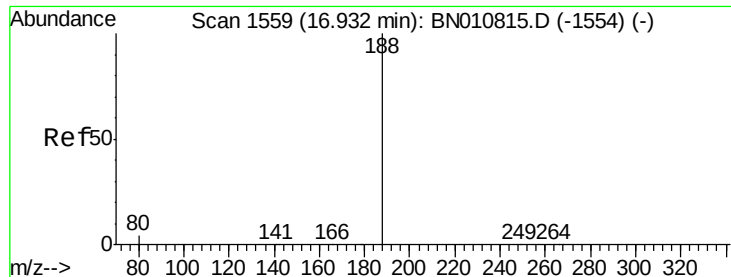

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.92 min Scan# 1558

Delta R.T. -0.00 min

Lab File: BN010854.D

Acq: 12 Jun 2020 22:31

Instrument :

BNA_N

ClientSampleId :

RE132D4-20200608DL


Tot Ion:188 Resp: 11180

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 9.7 4.5 6.7#

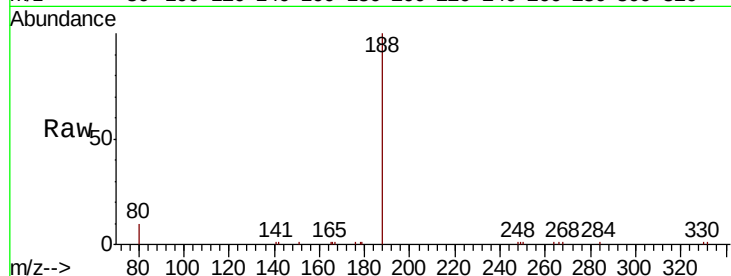

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNO

Ion 80.00 (79.70 to 80.70): BNO

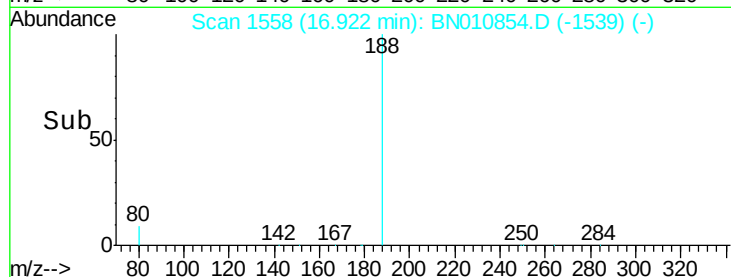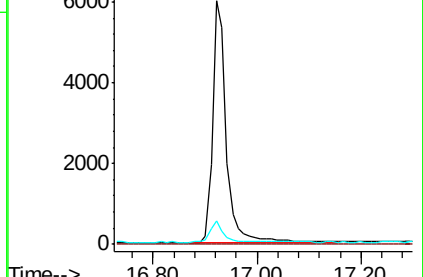

#25

Fluoranthene-d10

Concen: 0.166 ng

RT: 18.96 min Scan# 1853

Delta R.T. -0.00 min

Lab File: BN010854.D

Acq: 12 Jun 2020 22:31


Tgt Ion:212 Resp: 5109

Ion Ratio Lower Upper

212 100

106 10.3 6.6 10.0#



104 6.0 4.0 6.0#




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E



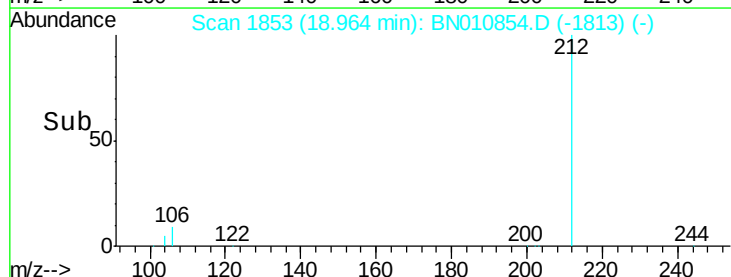
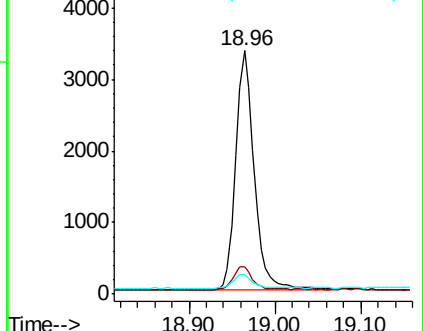


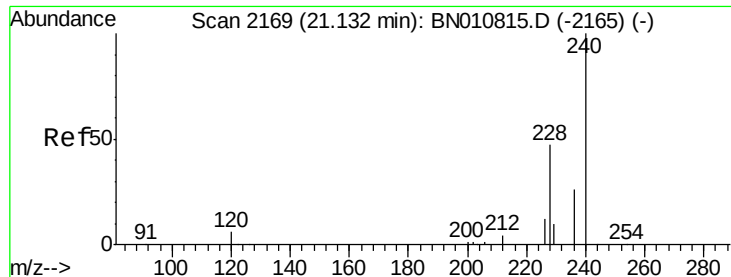

#27
Chrysene-d12
Concen: 0.400 ng
RT: 21.13 min Scan# 2169
Delta R.T. -0.00 min
Lab File: BN010854.D
Acq: 12 Jun 2020 22:31




Instrument :
BNA_N
ClientSampleId :
RE132D4-20200608DL


Tot Ion:240 Resp: 10667
Ion Ratio Lower Upper
240 100
120 8.0 7.5 11.3
236 28.1 22.3 33.5

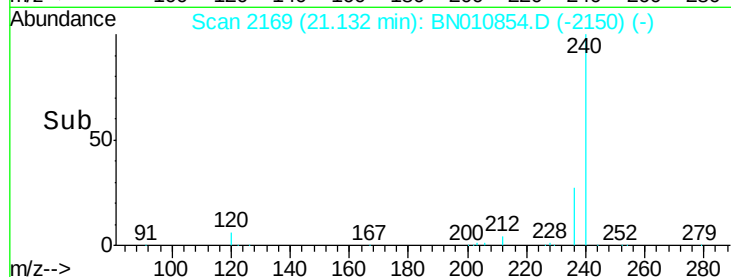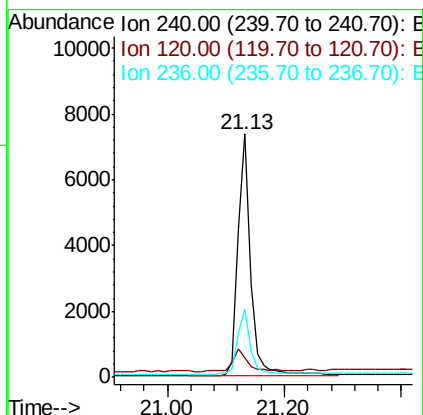

#29
Terphenyl-d14
Concen: 0.212 ng
RT: 19.57 min Scan# 1976
Delta R.T. -0.00 min
Lab File: BN010854.D
Acq: 12 Jun 2020 22:31

Tgt Ion:244 Resp: 5303
Ion Ratio Lower Upper
244 100
212 8.9 7.4 11.2
122 10.5 7.5 11.3

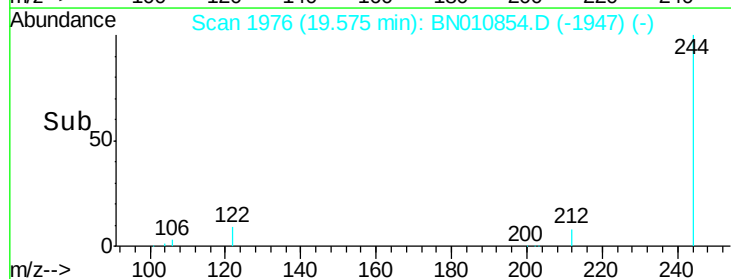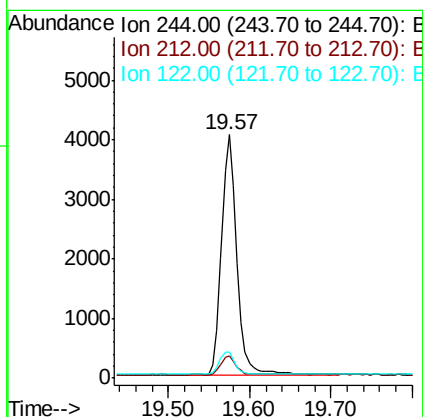

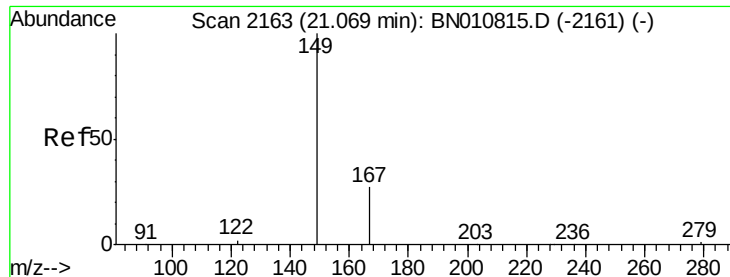

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.050 ng

RT: 21.07 min Scan# 2163

Delta R.T. -0.00 min

Lab File: BN010854.D

Acq: 12 Jun 2020 22:31

Instrument :

BNA_N

ClientSampleId :

RE132D4-20200608DL


Tot Ion:149 Resp: 520

Ion Ratio Lower Upper

149 100

167 29.6 24.1 36.1




279 7.7 4.6 7.0#

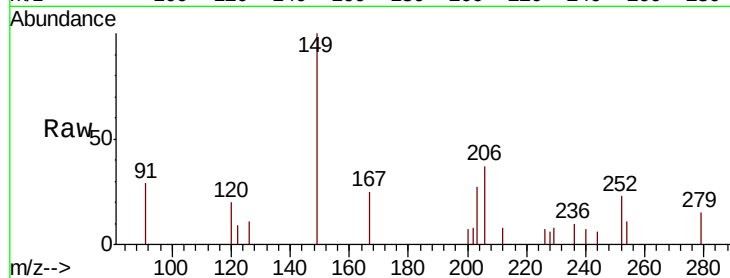

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

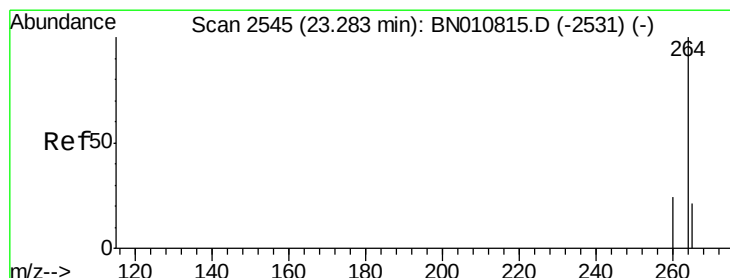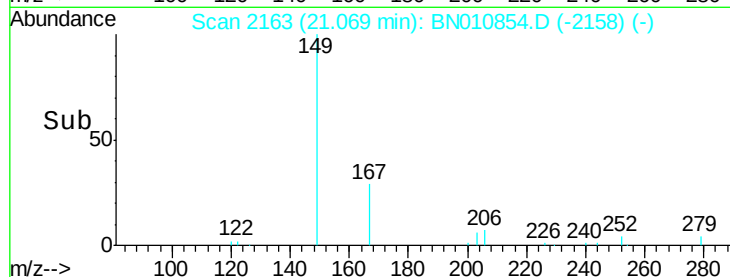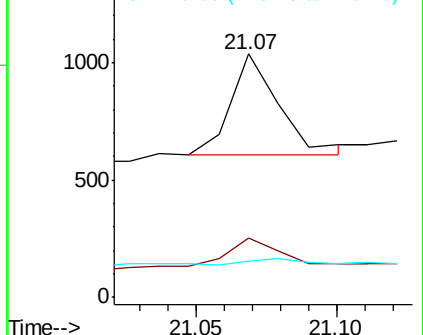

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.28 min Scan# 2544

Delta R.T. -0.00 min

Lab File: BN010854.D

Acq: 12 Jun 2020 22:31


Tgt Ion:264 Resp: 11662

Ion Ratio Lower Upper

264 100

260 24.4 20.4 30.6

265 77.3 75.0 112.4

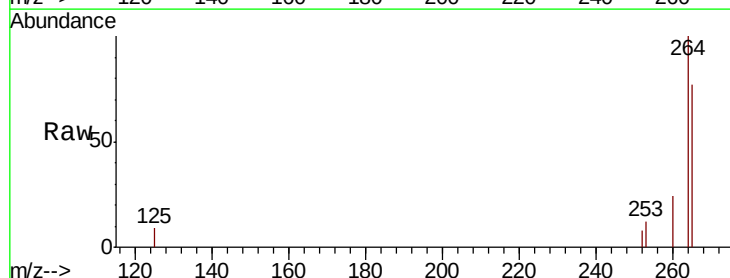

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

