

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061220\
 Data File : BN010860.D
 Acq On : 13 Jun 2020 02:07
 Operator : CG/JU
 Sample : L2988-19
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE135D3-20200609

Quant Time: Jun 13 03:23:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 12 11:11:17 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	2532	0.40	ng	0.00
7) Naphthalene-d8	10.30	136	8908	0.40	ng	0.00
13) Acenaphthene-d10	14.18	164	4964	0.40	ng	0.00
19) Phenanthrene-d10	16.93	188	10175	0.40	ng	0.00
27) Chrysene-d12	21.12	240	9845	0.40	ng	0.00
34) Perylene-d12	23.27	264	10526	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.21	112	821	0.17	ng	0.00
5) Phenol-d6	6.75	99	537	0.09	ng	0.00
8) Nitrobenzene-d5	8.69	82	2576	0.39	ng	0.00
11) 2-Methylnaphthalene-d10	11.90	152	4622	0.33	ng	0.00
14) 2,4,6-Tribromophenol	15.68	330	612	0.34	ng	0.00
15) 2-Fluorobiphenyl	12.79	172	7702	0.39	ng	0.00
25) Fluoranthene-d10	18.96	212	10969	0.39	ng	0.00
29) Terphenyl-d14	19.57	244	10350	0.45	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.22	88	425	0.171	ng	# 66
32) Bis(2-ethylhexyl)phthalate	21.07	149	1322	0.137	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061220\
Data File : BN010860.D
Acq On : 13 Jun 2020 02:07
Operator : CG/JU
Sample : L2988-19
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE135D3-20200609

Quant Time: Jun 13 03:23:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 12 11:11:17 2020
Response via : Initial Calibration

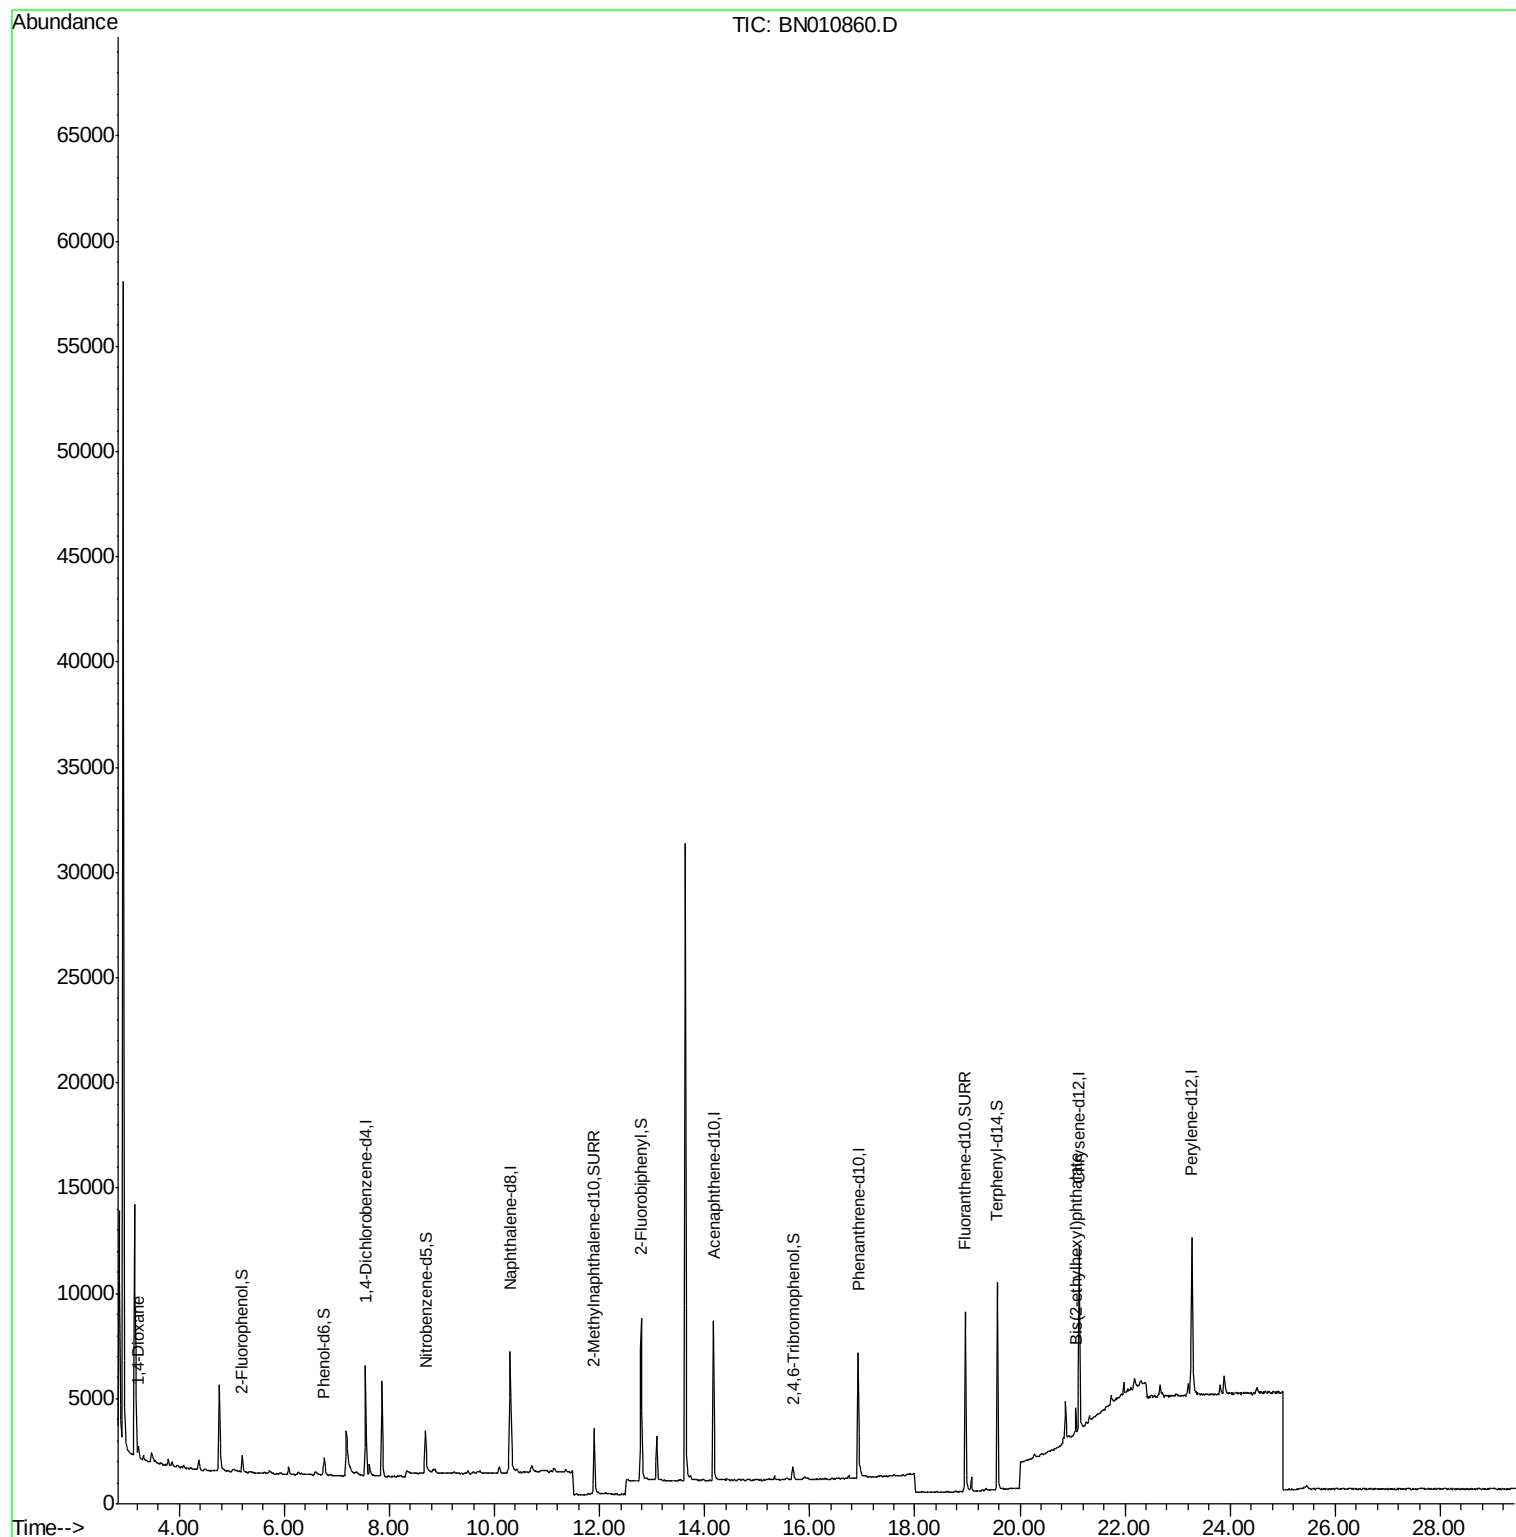

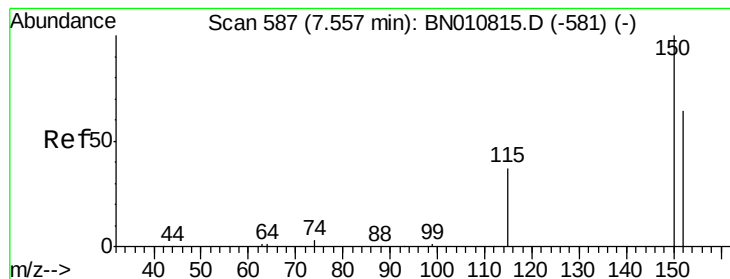


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.55 min Scan# 586
Delta R.T. -0.01 min
Lab File: BN010860.D
Acq: 13 Jun 2020 02:07

Instrument :
BNA_N
ClientSampleId :
RE135D3-20200609

Tot Ion:152 Resp: 2532
Ion Ratio Lower Upper
152 100
150 152.7 123.8 185.6
115 62.7 49.2 73.8

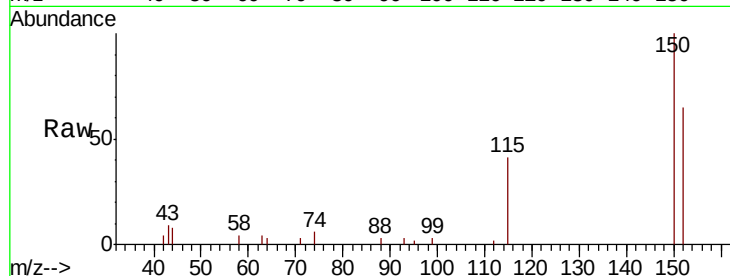


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

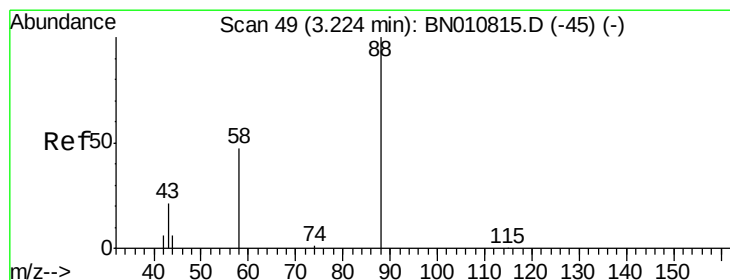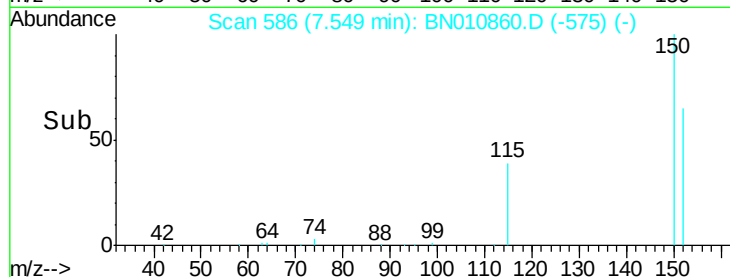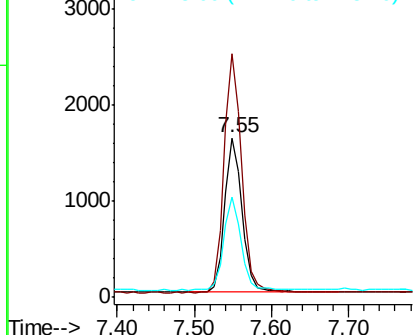



#2


1,4-Dioxane
Concen: 0.171 ng
RT: 3.22 min Scan# 49
Delta R.T. 0.00 min
Lab File: BN010860.D
Acq: 13 Jun 2020 02:07

Tgt Ion: 88 Resp: 425
Ion Ratio Lower Upper
88 100
58 56.0 38.2 57.4
43 59.5 15.1 22.7#

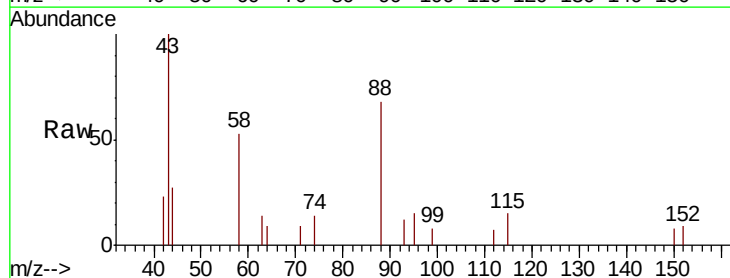

Abundance Ion 88.00 (87.70 to 88.70): BN0
Ion 58.00 (57.70 to 58.70): BN0
Ion 43.00 (42.70 to 43.70): BN0

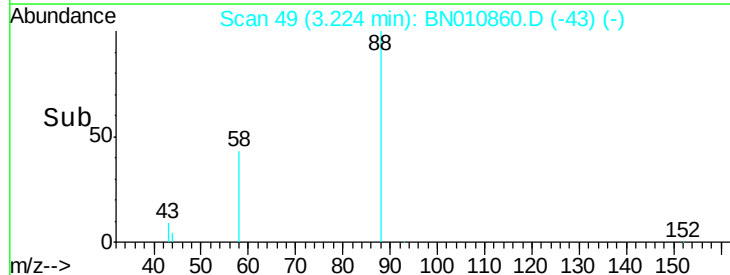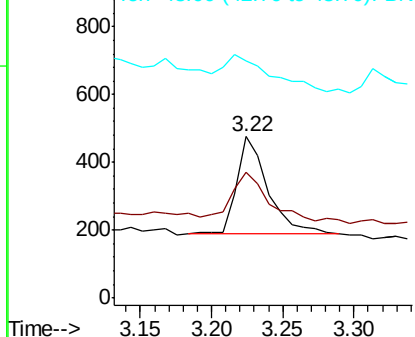

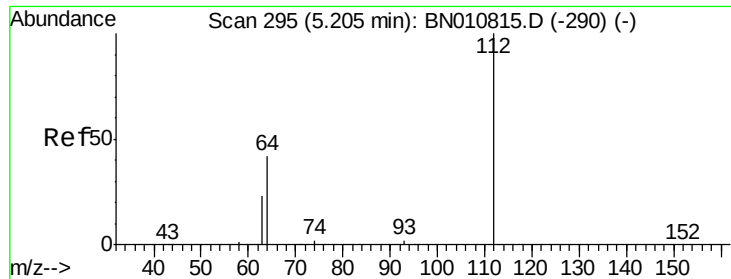

#4

2-Fluorophenol

Concen: 0.168 ng

RT: 5.21 min Scan# 295

Delta R.T. 0.00 min

Lab File: BN010860.D

Acq: 13 Jun 2020 02:07

Instrument :

BNA_N

ClientSampleId :

RE135D3-20200609


Tot Ion: 112 Resp: 821

Ion Ratio Lower Upper

112 100

64 46.0 37.4 56.0

63 24.2 22.2 33.4



Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): BNO

Ion 63.00 (62.70 to 63.70): BNO

5.21



400

200

0

5.10 5.20 5.30

Time-->



#5

Phenol-d6

Concen: 0.093 ng

RT: 6.75 min Scan# 487

Delta R.T. 0.00 min

Lab File: BN010860.D

Acq: 13 Jun 2020 02:07


Tgt Ion: 99 Resp: 537

Ion Ratio Lower Upper

99 100

42 24.2 11.1 16.7#

71 42.5 31.4 47.2



Abundance Ion 99.00 (98.70 to 99.70): BNO

Ion 42.00 (41.70 to 42.70): BNO

Ion 71.00 (70.70 to 71.70): BNO

6.75

400

300


200


100

0

6.70 6.80

Time-->



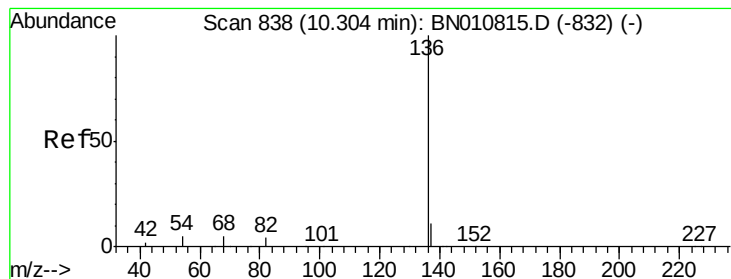

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.30 min Scan# 838

Delta R.T. 0.00 min

Lab File: BN010860.D

Acq: 13 Jun 2020 02:07

Instrument :

BNA_N

ClientSampleId :

RE135D3-20200609

Tot Ion:136 Resp: 8908


Ion Ratio Lower Upper

136 100

137 12.0 9.7 14.5

54 4.4 4.9 7.3#

68 5.3 4.7 7.1






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

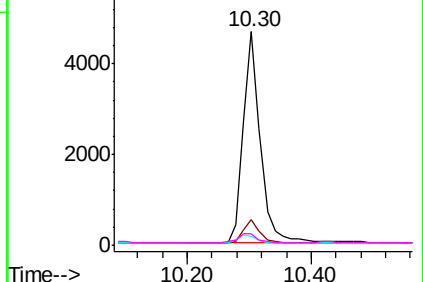

#8

Nitrobenzene-d5

Concen: 0.391 ng

RT: 8.69 min Scan# 711

Delta R.T. 0.00 min

Lab File: BN010860.D

Acq: 13 Jun 2020 02:07


Tgt Ion: 82 Resp: 2576

Ion Ratio Lower Upper

82 100

128 49.6 35.4 53.0



54 32.1 28.2 42.4




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC



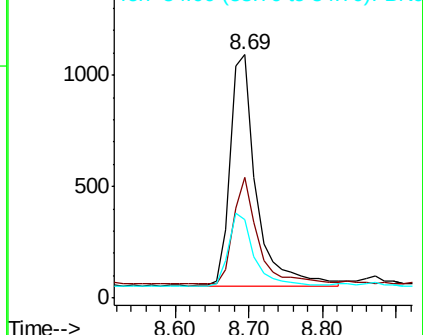



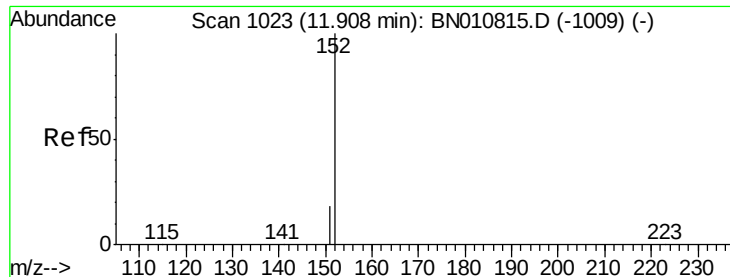

#11
2-Methylnaphthalene-d10
Concen: 0.335 ng
RT: 11.90 min Scan# 1021
Delta R.T. 0.00 min
Lab File: BN010860.D
Acq: 13 Jun 2020 02:07




Instrument :
BNA_N
ClientSampleId :
RE135D3-20200609


Tot Ion:152 Resp: 4622
Ion Ratio Lower Upper
152 100
151 20.0 15.3 22.9

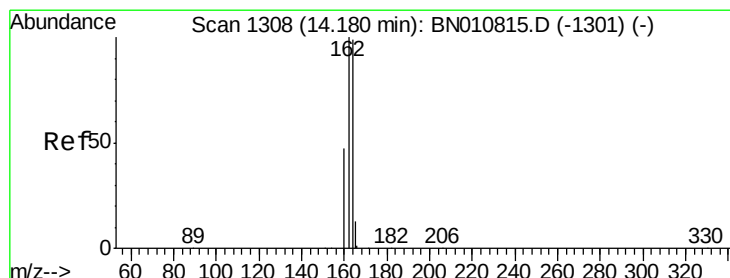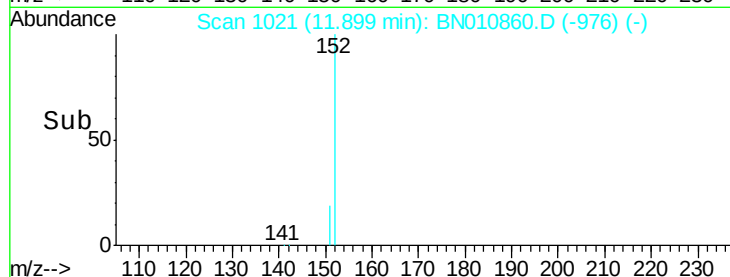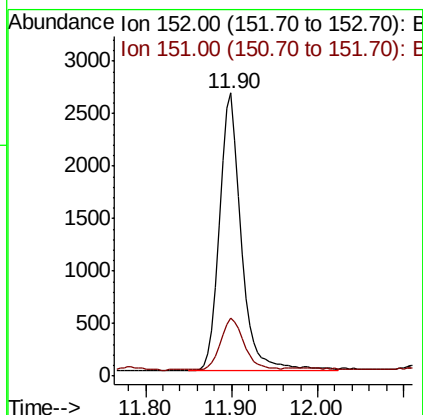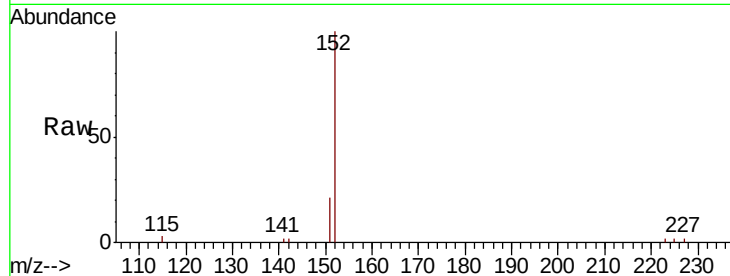

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.18 min Scan# 1307
Delta R.T. -0.00 min
Lab File: BN010860.D
Acq: 13 Jun 2020 02:07

Tgt Ion:164 Resp: 4964
Ion Ratio Lower Upper
164 100
162 99.4 81.0 121.6
160 45.3 38.9 58.3

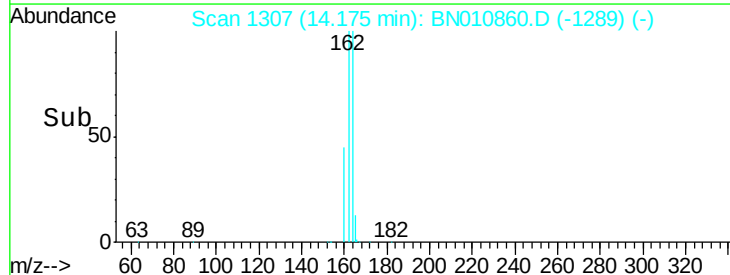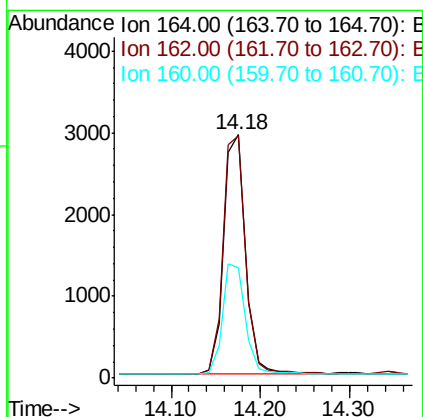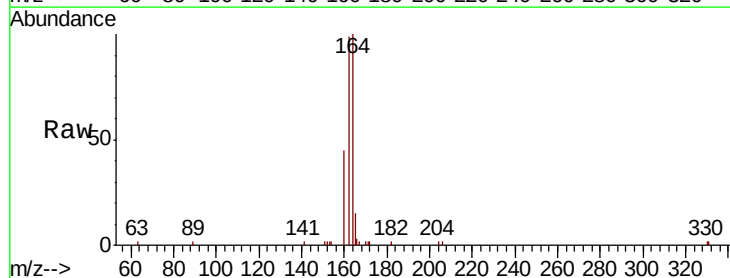


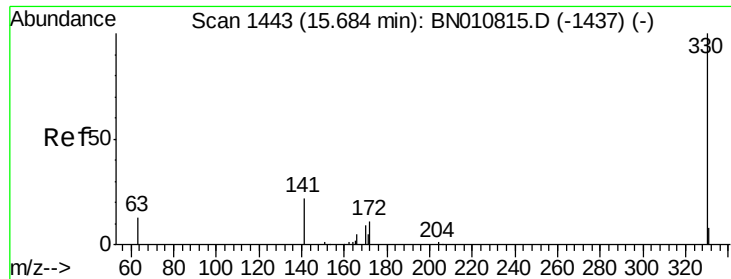




#14
 2,4,6-Tribromophenol
 Concen: 0.345 ng
 RT: 15.68 min Scan# 1442
 Delta R.T. -0.00 min
 Lab File: BN010860.D
 Acq: 13 Jun 2020 02:07

Instrument :
 BNA_N
 ClientSampleId :
 RE135D3-20200609

Tot Ion:330 Resp: 612
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 40.0 33.2 49.8

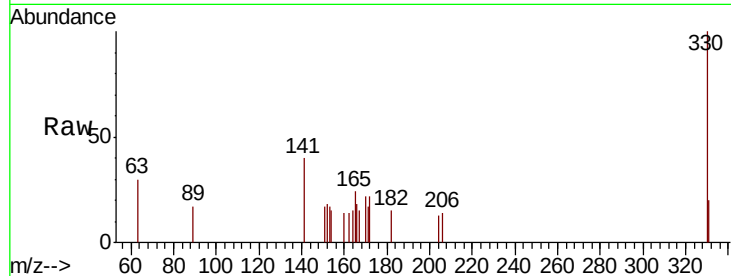


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


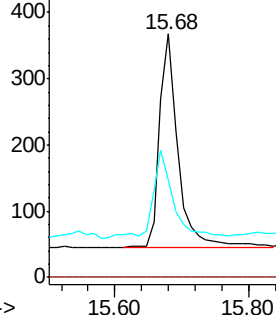



#15
 2-Fluorobiphenyl
 Concen: 0.393 ng
 RT: 12.79 min Scan# 1183
 Delta R.T. -0.00 min
 Lab File: BN010860.D
 Acq: 13 Jun 2020 02:07

Tgt Ion:172 Resp: 7702
 Ion Ratio Lower Upper
 172 100
 171 35.2 28.5 42.7
 170 23.0 19.7 29.5



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

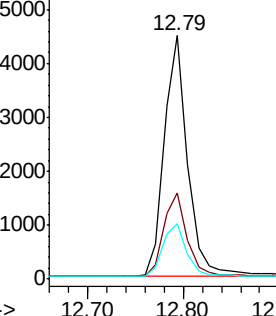

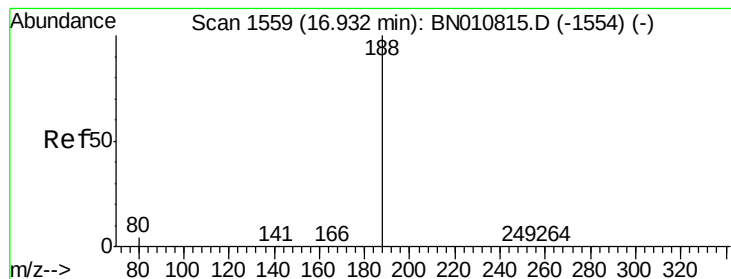

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.93 min Scan# 1558

Delta R.T. 0.01 min

Lab File: BN010860.D

Acq: 13 Jun 2020 02:07

Instrument :

BNA_N

ClientSampleId :

RE135D3-20200609


Tot Ion:188 Resp: 10175

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 6.6 4.5 6.7



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNO

Ion 80.00 (79.70 to 80.70): BNO

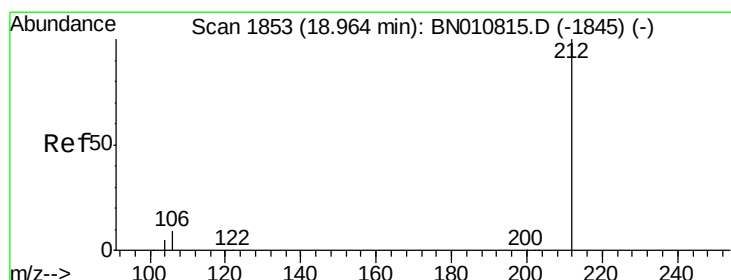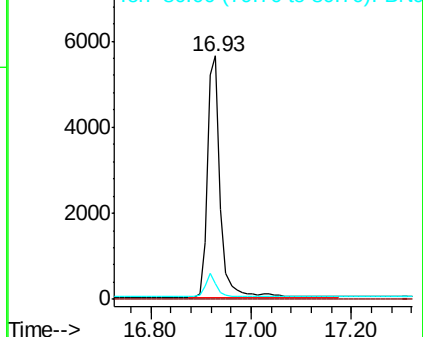

#25

Fluoranthene-d10

Concen: 0.391 ng

RT: 18.96 min Scan# 1851

Delta R.T. -0.00 min

Lab File: BN010860.D

Acq: 13 Jun 2020 02:07


Tgt Ion:212 Resp: 10969

Ion Ratio Lower Upper

212 100

106 10.2 6.6 10.0#



104 5.9 4.0 6.0




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

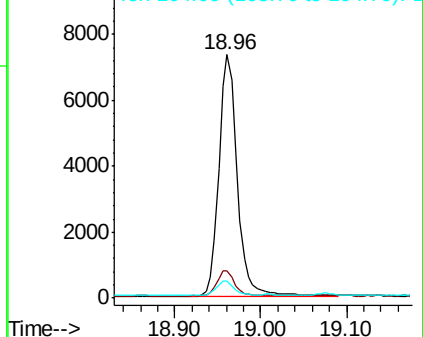

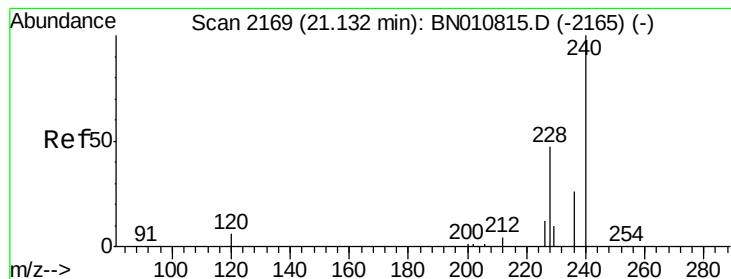

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.12 min Scan# 2167

Delta R.T. -0.01 min

Lab File: BN010860.D

Acq: 13 Jun 2020 02:07

Instrument :

BNA_N

ClientSampleId :

RE135D3-20200609


Tot Ion:240 Resp: 9845

Ion Ratio Lower Upper

240 100

120 12.6 7.5 11.3#




236 28.6 22.3 33.5



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

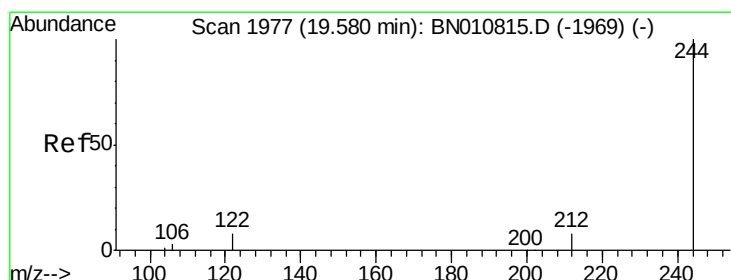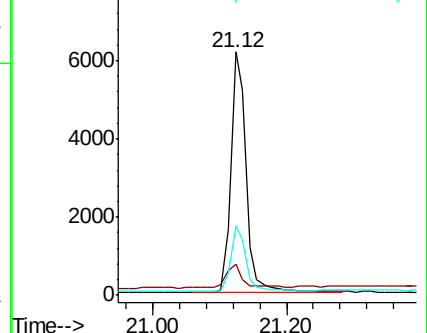

#29

Terphenyl-d14

Concen: 0.449 ng

RT: 19.57 min Scan# 1974

Delta R.T. -0.01 min

Lab File: BN010860.D

Acq: 13 Jun 2020 02:07


Tgt Ion:244 Resp: 10350

Ion Ratio Lower Upper

244 100

212 8.6 7.4 11.2



122 10.6 7.5 11.3




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

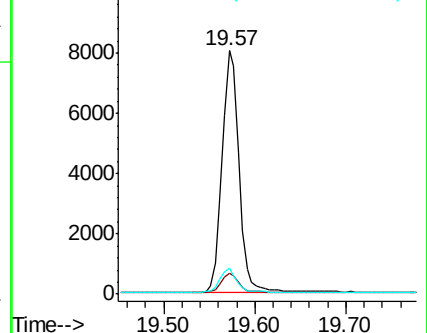



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.137 ng

RT: 21.07 min Scan# 2162

Delta R.T. 0.00 min

Lab File: BN010860.D

Acq: 13 Jun 2020 02:07

Instrument :

BNA_N

ClientSampleId :

RE135D3-20200609


Tot Ion:149 Resp: 1322

Ion Ratio Lower Upper

149 100

167 27.2 24.1 36.1




279 4.6 4.6 7.0#



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

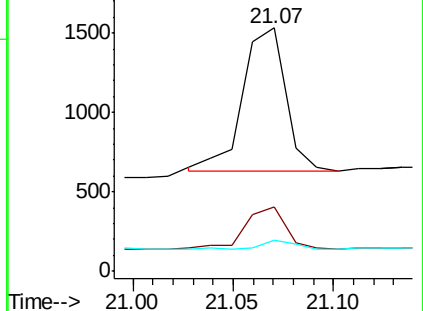

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.27 min Scan# 2540

Delta R.T. -0.01 min

Lab File: BN010860.D

Acq: 13 Jun 2020 02:07


Tgt Ion:264 Resp: 10526

Ion Ratio Lower Upper

264 100

260 24.3 20.4 30.6

265 82.7 75.0 112.4



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

