


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061220\
 Data File : BN010850.D
 Acq On : 12 Jun 2020 19:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 15 11:09:46 2020

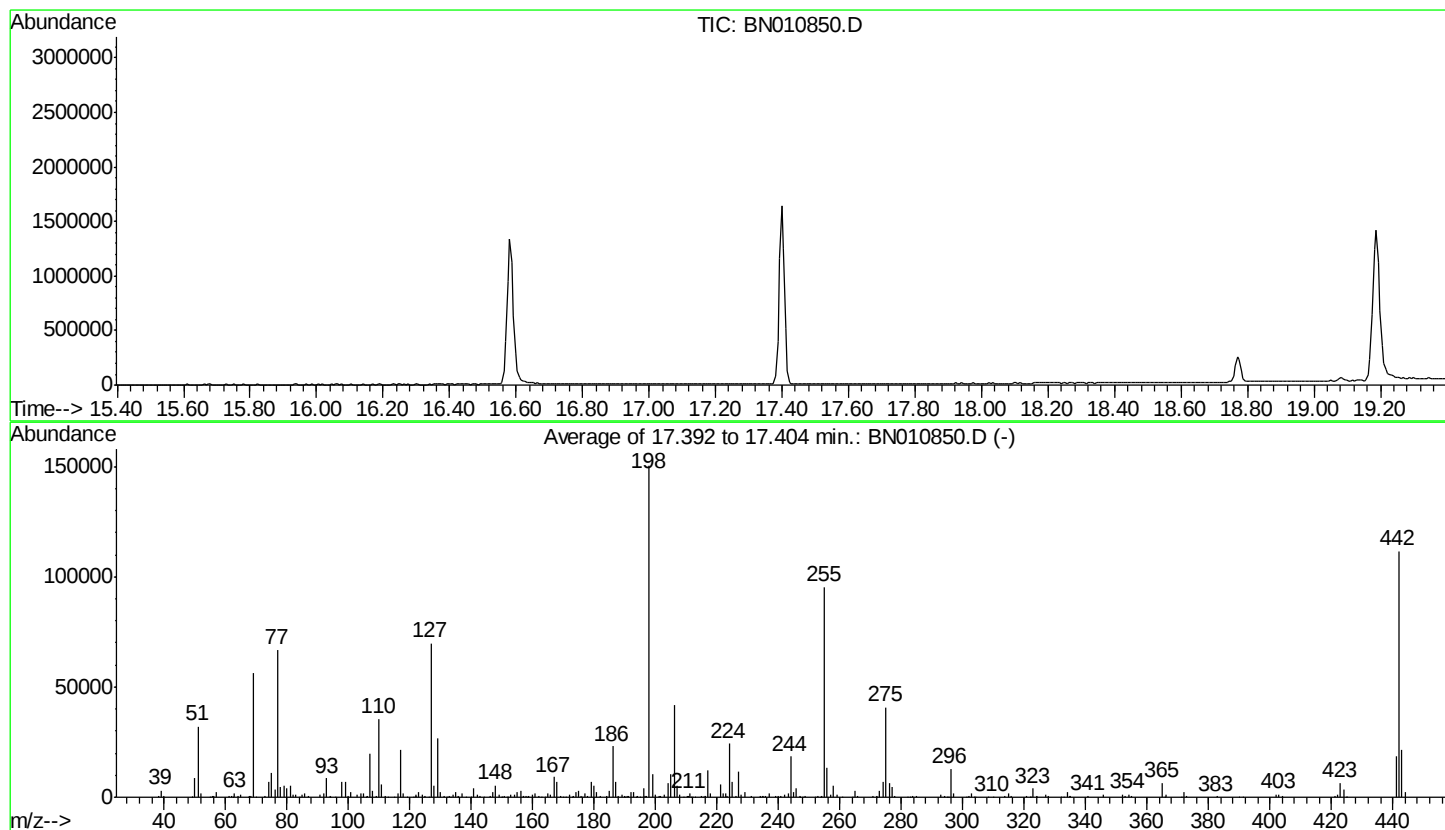

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.4	32130	PASS
68	69	0.00	2	1.4	767	PASS
69	198	0.00	100	37.3	56165	PASS
70	69	0.00	2	0.3	187	PASS
127	198	10	80	46.4	69762	PASS
197	198	0.00	2	0.2	376	PASS
198	198	100	100	100.0	150405	PASS
199	198	5	9	6.8	10185	PASS
275	198	10	60	27.2	40906	PASS
365	198	1	100	4.3	6431	PASS
441	198	0.01	100	12.5	18798	PASS
442	198	50	100	74.2	111661	PASS
443	442	15	24	19.2	21422	PASS