

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031917.D
 Acq On : 11 Jun 2024 19:40
 Operator : MA/JU
 Sample : PB161309BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK309

Quant Time: Jun 11 22:32:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 11 22:28:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.658	152	304666	20.000	ng/ul	0.00
20) Naphthalene-d8	10.440	136	1390076	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.304	164	973765	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.051	188	2066836	20.000	ng/ul	0.00
79) Chrysene-d12	21.292	240	1963816	20.000	ng/ul	0.00
88) Perylene-d12	24.221	264	2237038	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.176	96	39424	5.353	ng/uL	0.00
4) Pyridine-d5	3.581	84	490054	23.639	ng/ul	0.00
7) Phenol-d5	6.834	99	708327	27.120	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	433518	28.377	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132	575721	28.889	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	598126	28.094	ng/ul	0.00
21) Nitrobenzene-d5	8.816	128	307130	28.897	ng/ul	0.00
24) 2-Nitrophenol-d4	9.534	143	315784	28.762	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	550363	26.851	ng/ul	0.00
31) 4-Chloroaniline-d4	10.587	131	863495	28.374	ng/ul	0.00
46) Dimethylphthalate-d6	13.722	166	1969439	29.031	ng/ul	0.00
49) Acenaphthylene-d8	13.998	160	2154976	27.627	ng/ul	0.00
54) 4-Nitrophenol-d4	14.516	143	357151	26.294	ng/ul	0.00
60) Fluorene-d10	15.298	176	1623910	28.291	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.428	200	250791	24.140	ng/ul	0.00
73) Anthracene-d10	17.151	188	2577259	29.126	ng/ul	0.00
81) Pyrene-d10	19.451	212	2967960	28.243	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.021	264	2866387	26.834	ng/ul	0.00


Target Compounds					Qvalue	
5) Pyridine	3.605	79	21029	1.015	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031917.D
Acq On : 11 Jun 2024 19:40
Operator : MA/JU
Sample : PB161309BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK309

Quant Time: Jun 11 22:32:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 11 22:28:10 2024
Response via : Initial Calibration

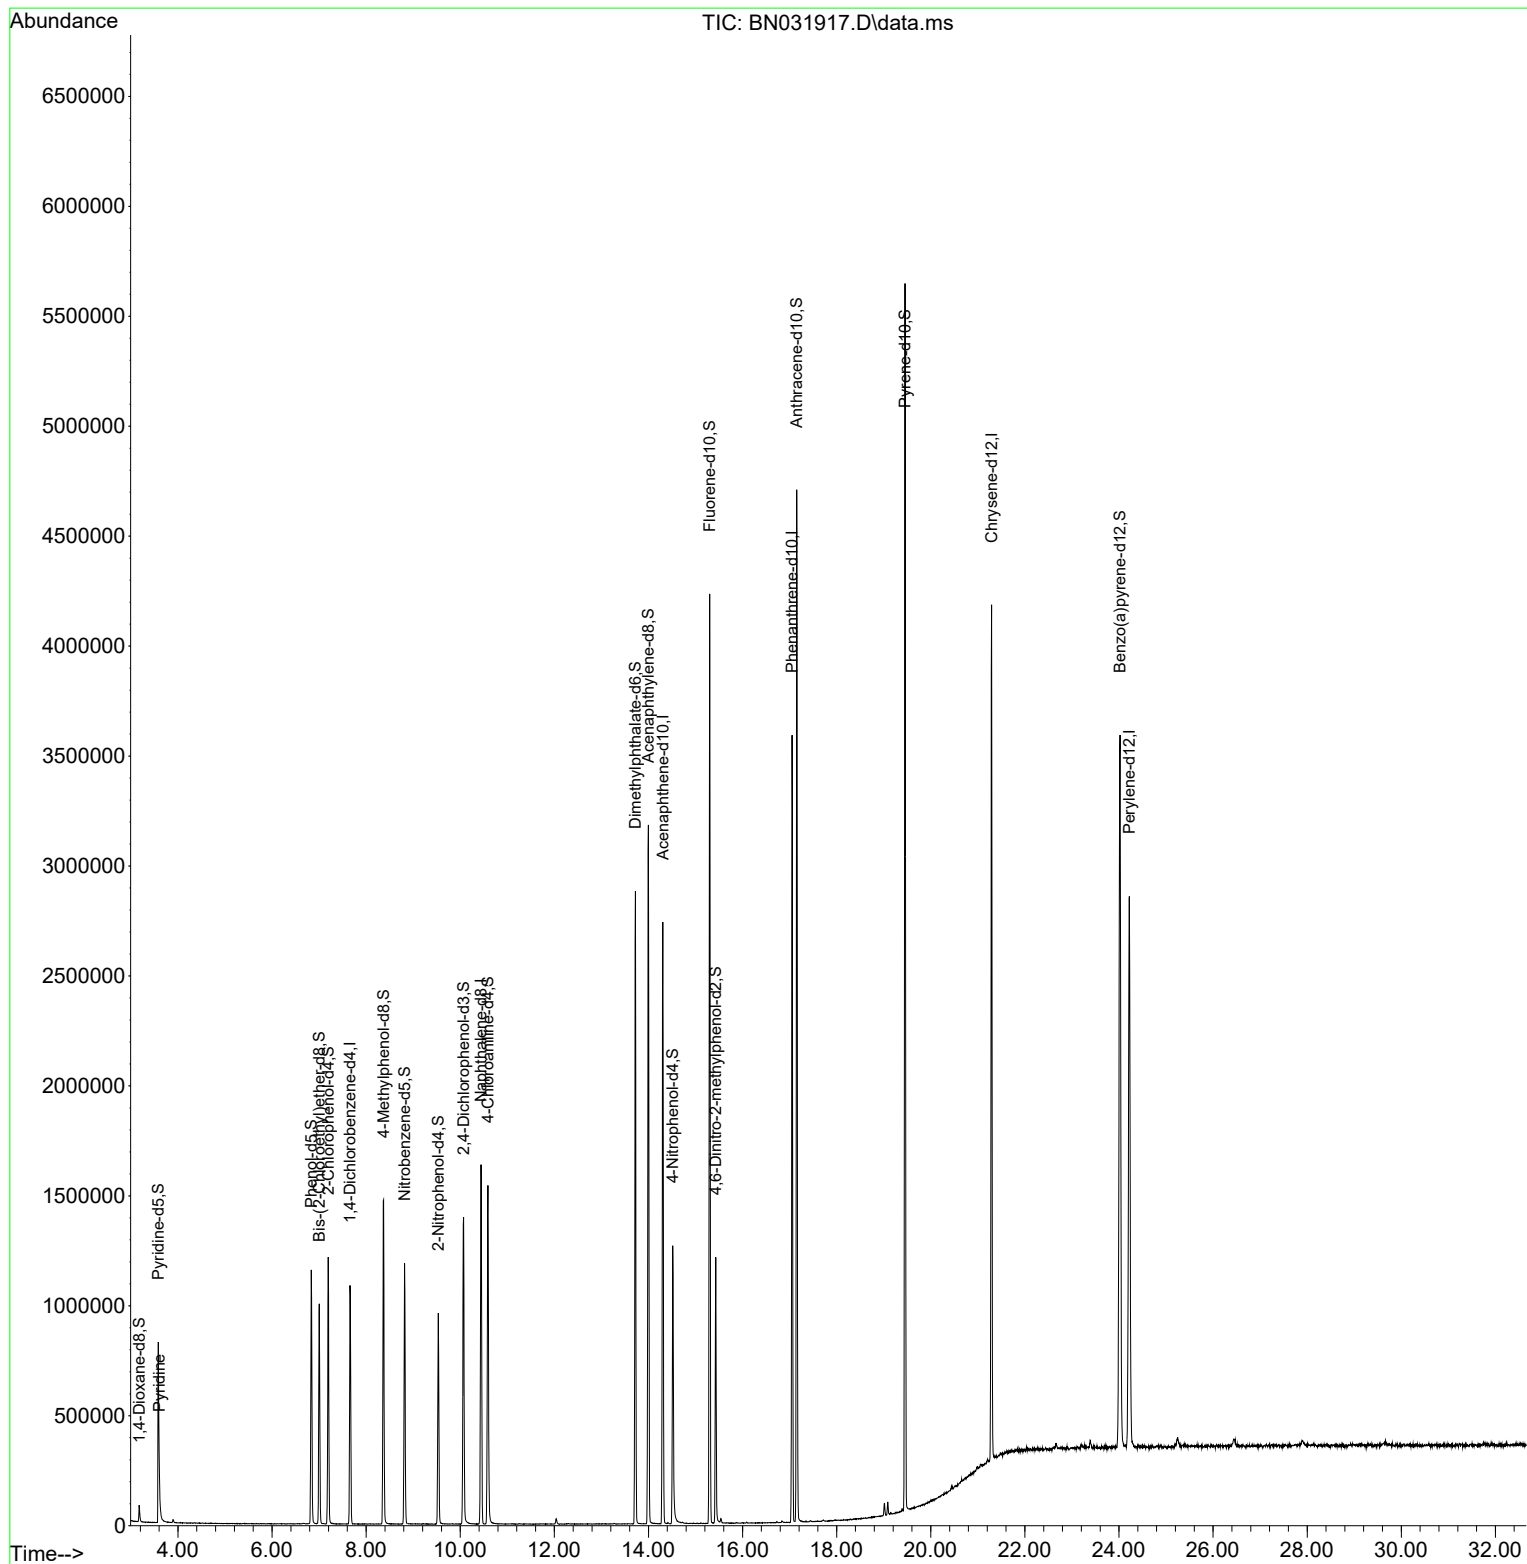

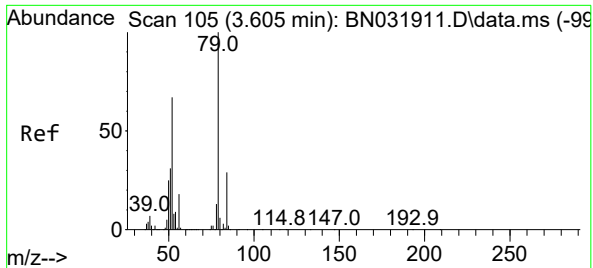

#5
 Pyridine
 Concen: 1.015 ng/ul
 RT: 3.605 min Scan# 10
 Delta R.T. 0.006 min
 Lab File: BN031917.D
 Acq: 11 Jun 2024 19:40

Instrument :
 BNA_N
 ClientSampleId :
 SBLK309

Tgt Ion:	79	Resp:	21029
Ion	Ratio	Lower	Upper
79	100		
52	223.3	53.0	79.6#
51	37.6	23.3	34.9#

