




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031982.D
Acq On : 13 Jun 2024 18:15
Operator : MA/JU
Sample : P2663-07
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH694

Manual IntegrationsAPPROVED

Quant Time: Jun 13 19:00:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 11 22:28:10 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/14/2024
Supervised By :mohammad ahmed 06/14/2024

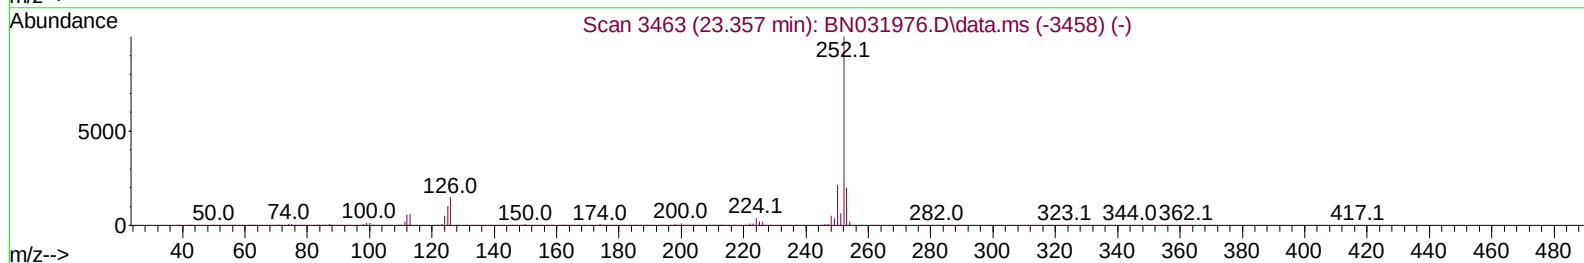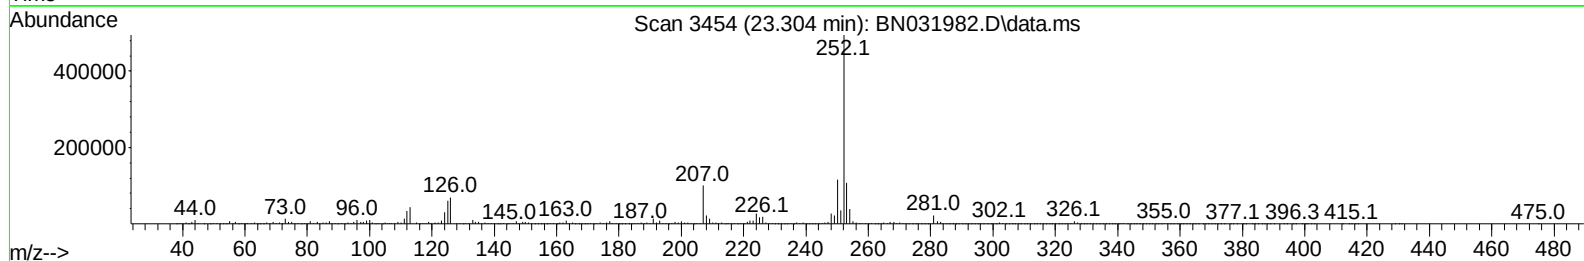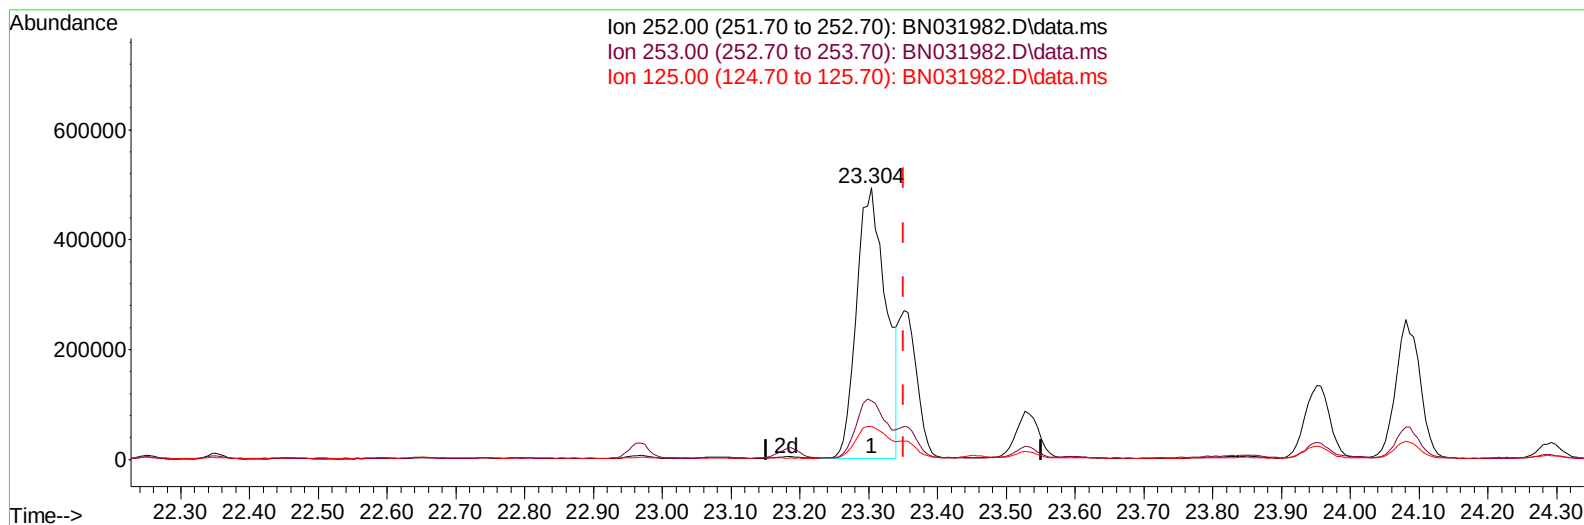

TIC: BN031982.D\data.ms

(91) Benzo(k)fluoranthene

23.304min (-0.047) 22.69 ng/u1

response 1468743

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.00	21.68
125.00	11.80	12.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031982.D
Acq On : 13 Jun 2024 18:15
Operator : MA/JU
Sample : P2663-07
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH694

Manual IntegrationsAPPROVED

Quant Time: Jun 13 19:00:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 11 22:28:10 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/14/2024
Supervised By :mohammad ahmed 06/14/2024

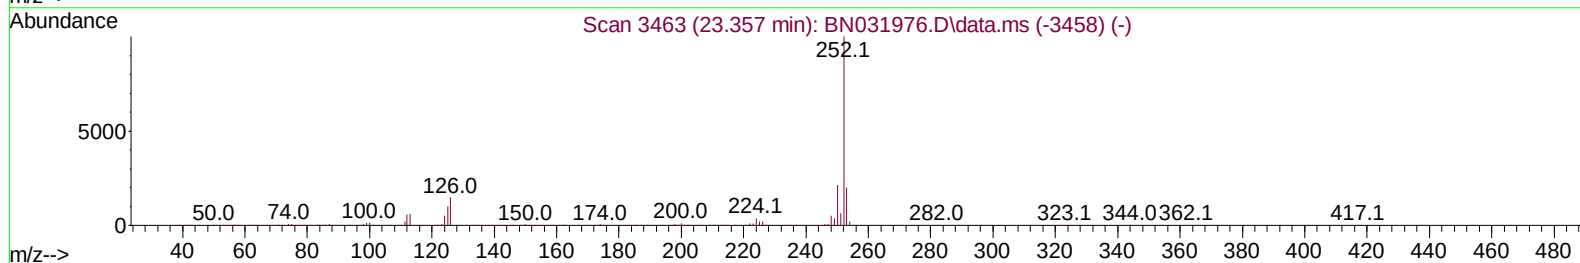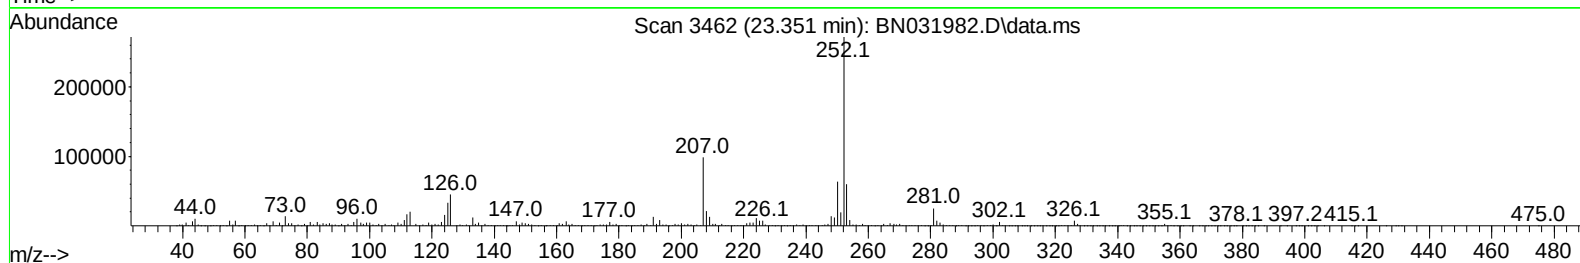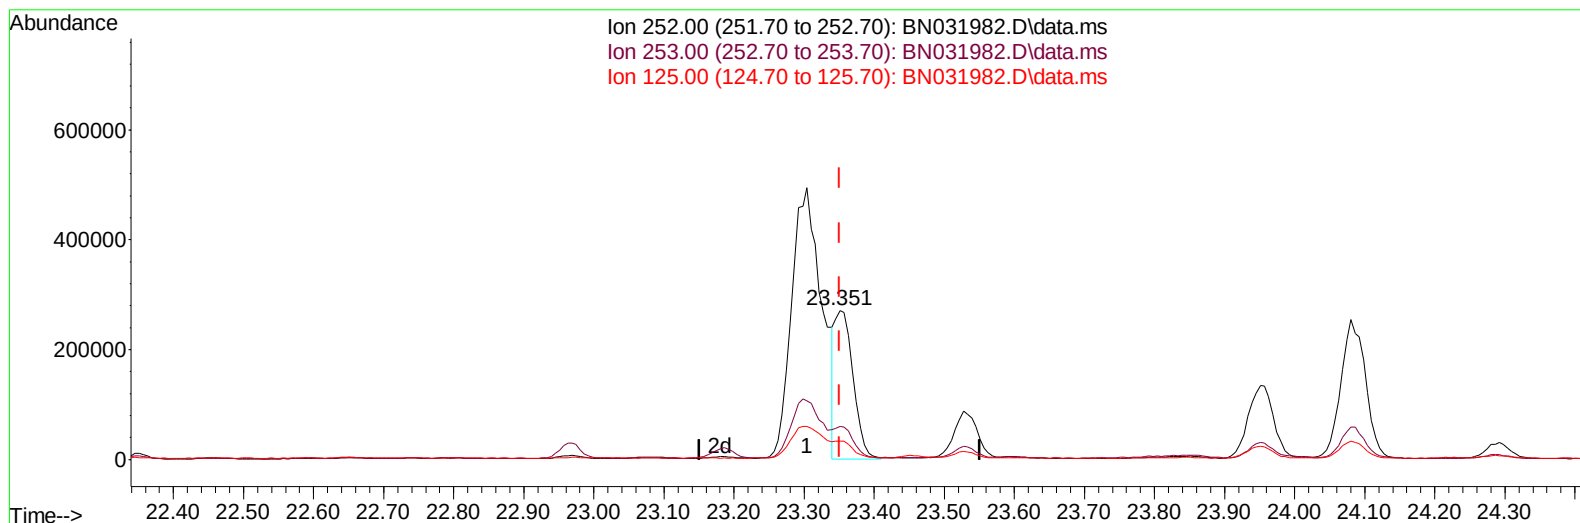

TIC: BN031982.D\data.ms

(91) Benzo(k)fluoranthene

23.351min (+ 0.000) 7.56 ng/ul m

response 489157

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.00	21.95
125.00	11.80	12.41
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031982.D
Acq On : 13 Jun 2024 18:15
Operator : MA/JU
Sample : P2663-07
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH694

Manual IntegrationsAPPROVED

Quant Time: Jun 13 19:00:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 11 22:28:10 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/14/2024
Supervised By :mohammad ahmed 06/14/2024

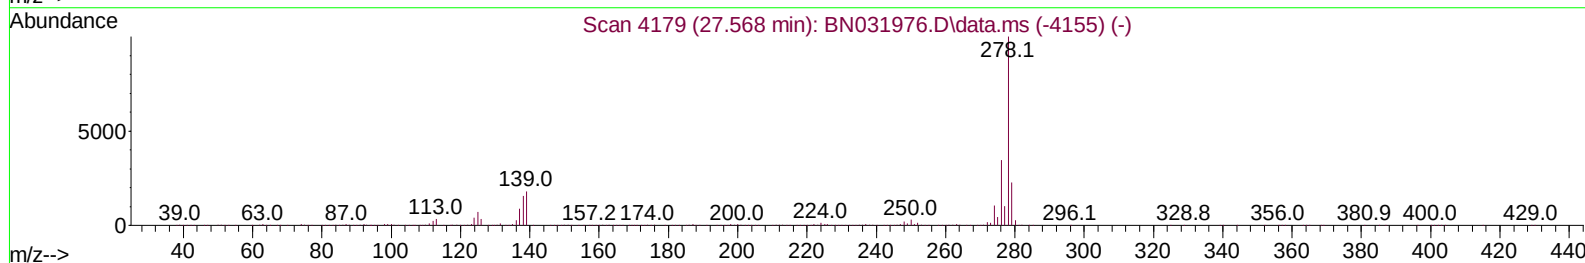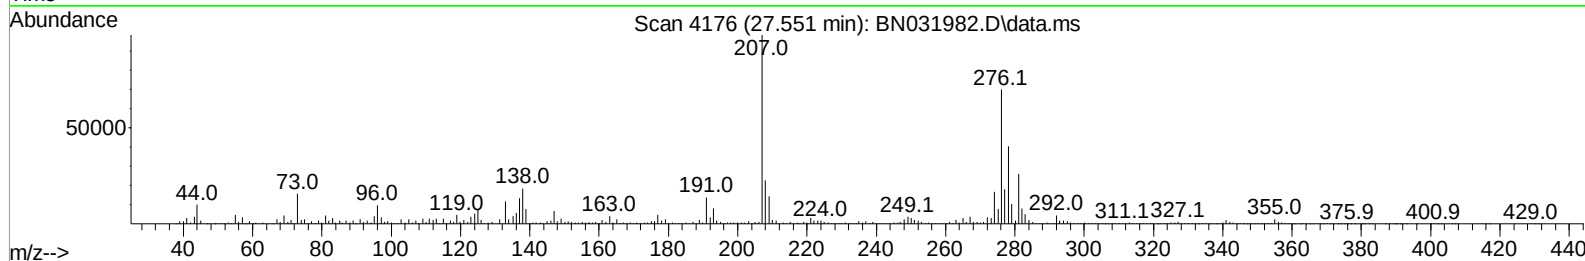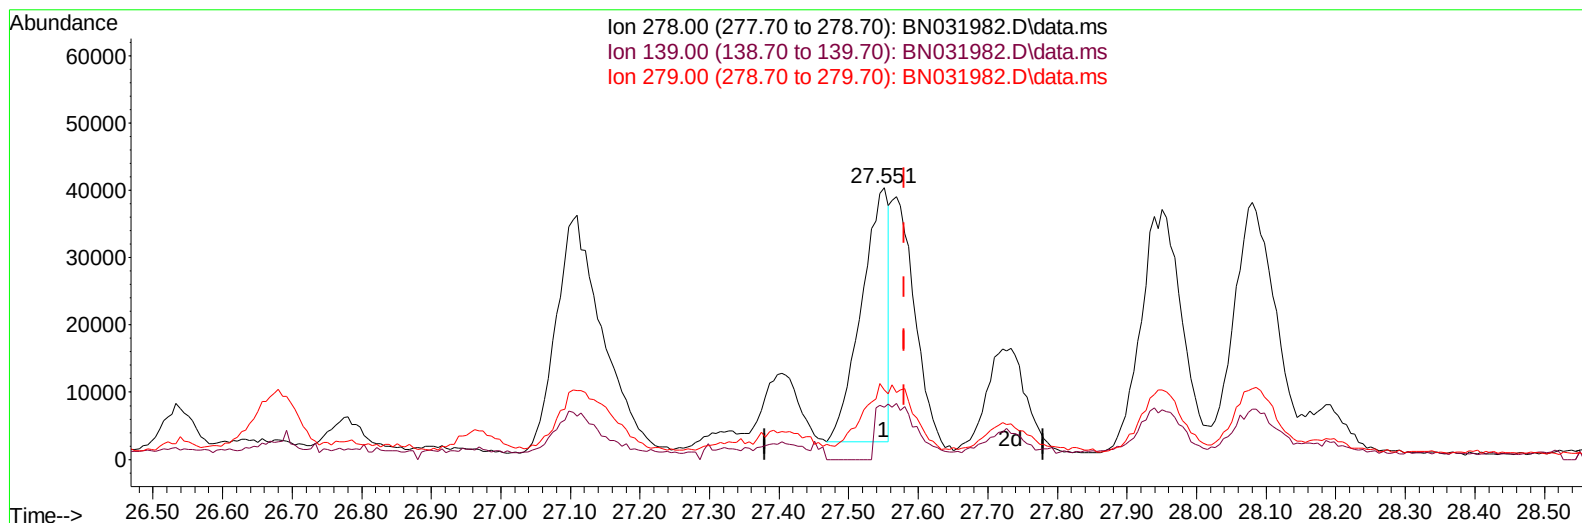

TIC: BN031982.D\data.ms

(95) Dibenzo(a,h)anthracene

27.551min (-0.029) 1.76 ng/u1

response 102120

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	18.80	19.27
279.00	21.70	25.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031982.D
Acq On : 13 Jun 2024 18:15
Operator : MA/JU
Sample : P2663-07
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH694

Manual IntegrationsAPPROVED

Quant Time: Jun 13 19:00:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 11 22:28:10 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/14/2024
Supervised By :mohammad ahmed 06/14/2024

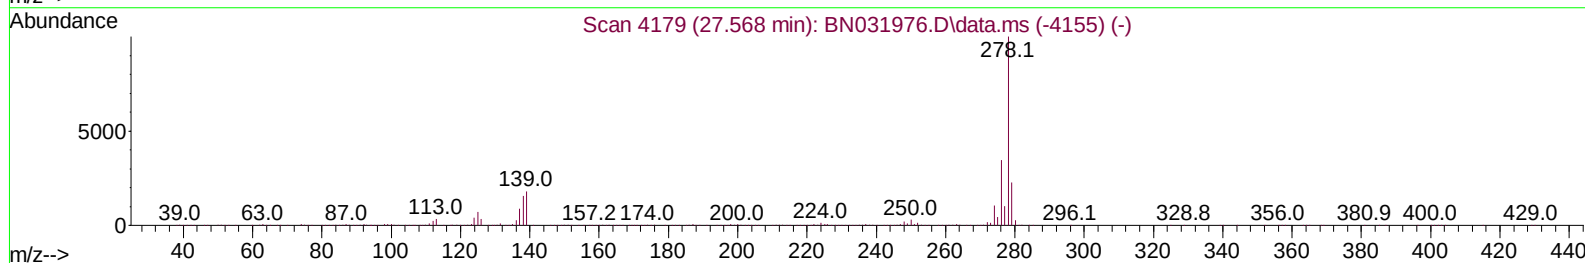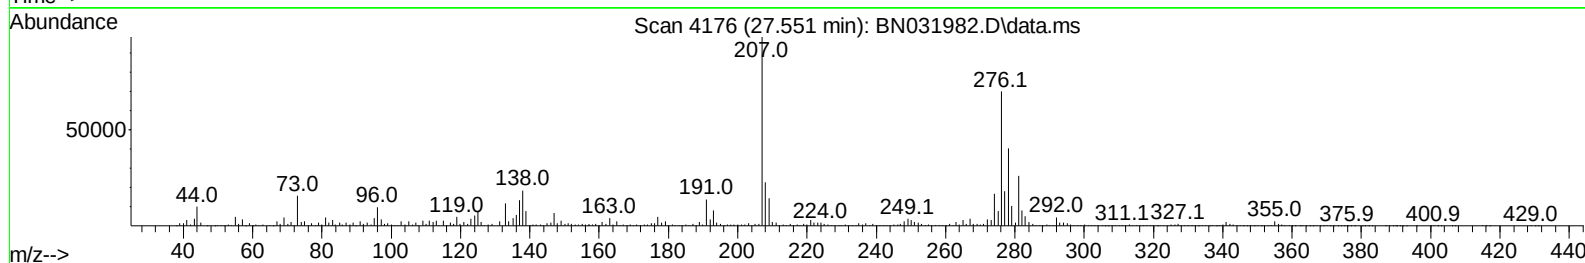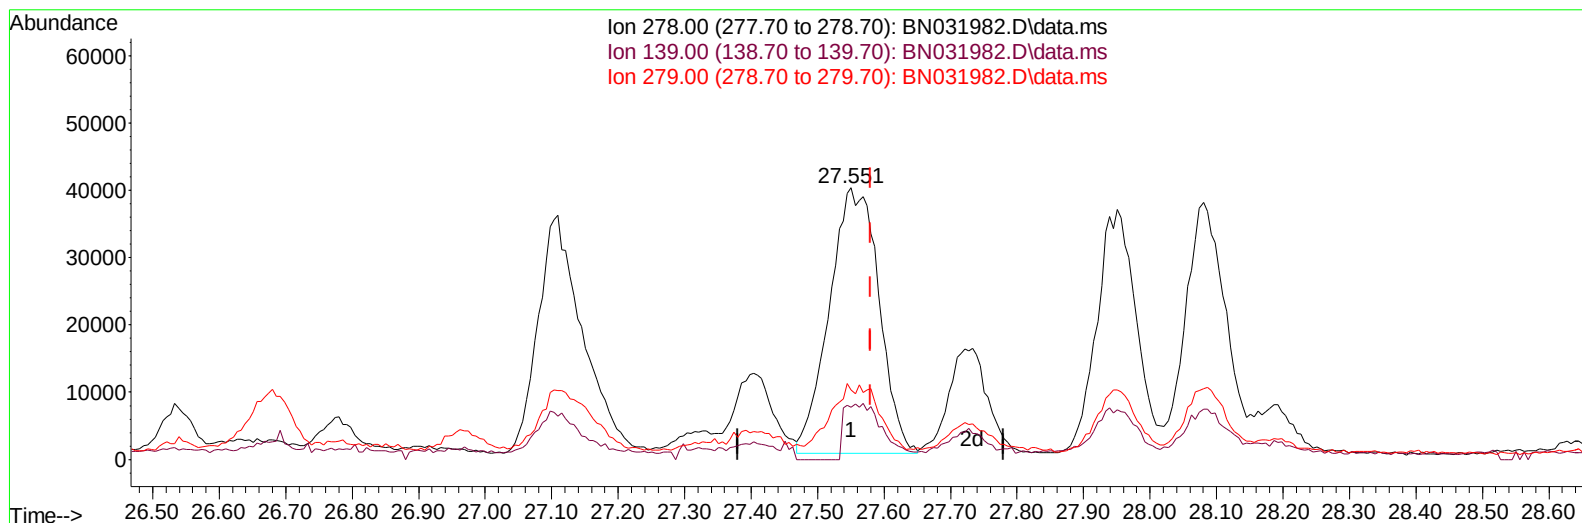

TIC: BN031982.D\data.ms

(95) Dibenzo(a,h)anthracene

27.551min (-0.029) 3.50 ng/ul m

response 203531

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	18.80	19.27
279.00	21.70	25.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031982.D
 Acq On : 13 Jun 2024 18:15
 Operator : MA/JU
 Sample : P2663-07
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH694

Manual IntegrationsAPPROVED

Quant Time: Jun 13 19:00:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 11 22:28:10 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/14/2024
 Supervised By :mohammad ahmed 06/14/2024

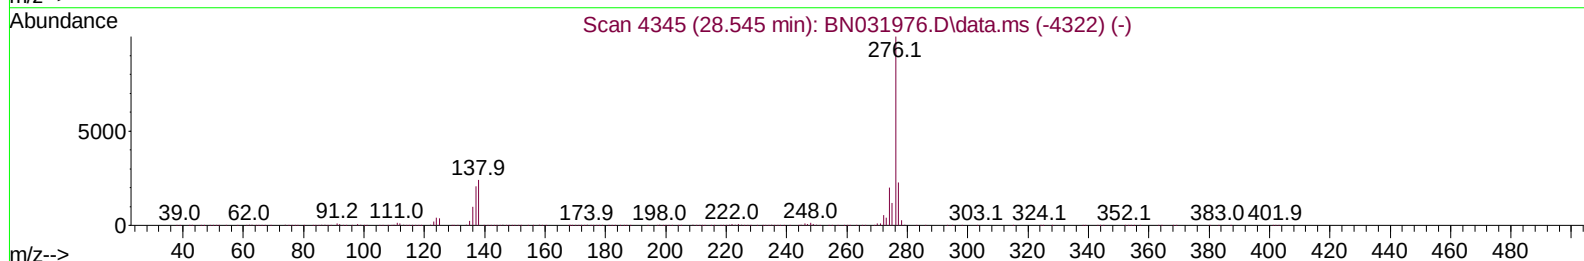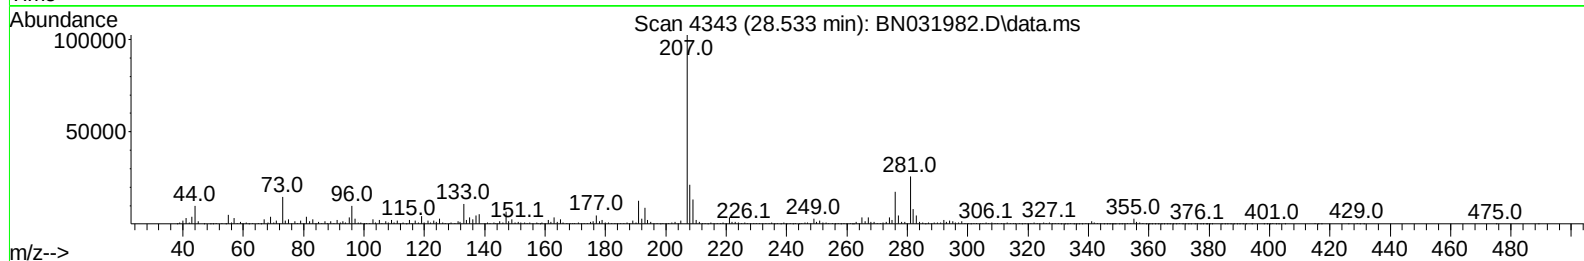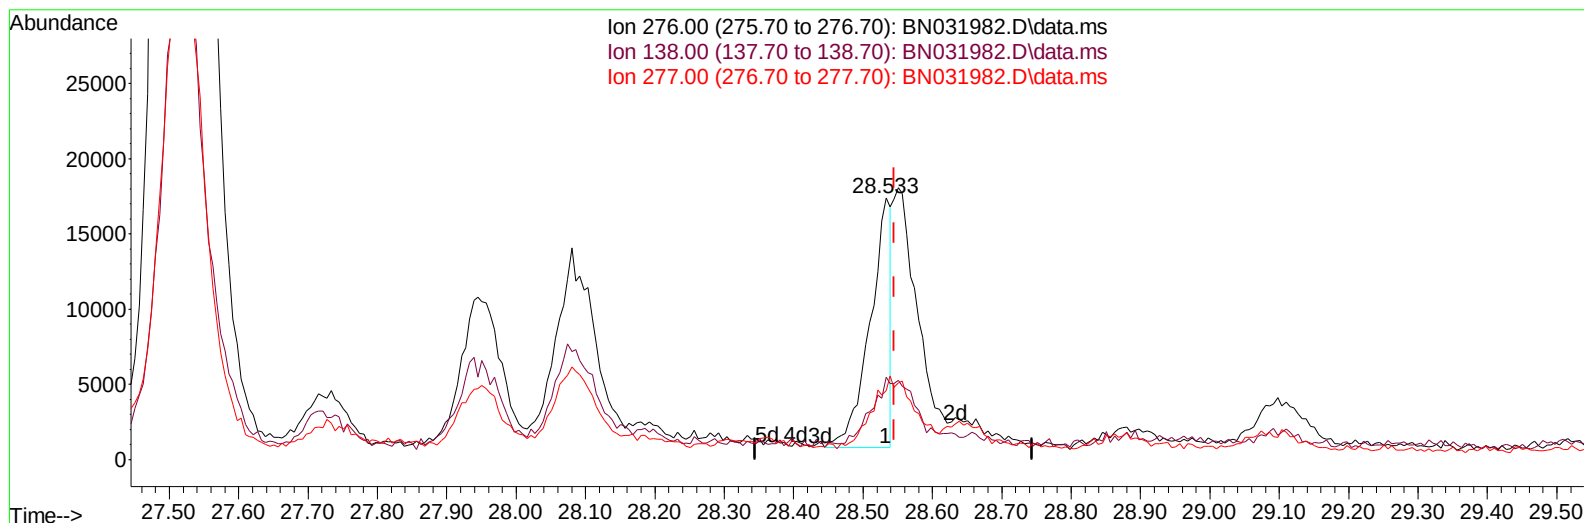

TIC: BN031982.D\data.ms

(96) Benzo(g,h,i)perylene

28.533min (-0.012) 0.62 ng/u1

response 34986

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	26.10	31.45#
277.00	22.50	26.32
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031982.D
Acq On : 13 Jun 2024 18:15
Operator : MA/JU
Sample : P2663-07
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH694

Manual IntegrationsAPPROVED

Quant Time: Jun 13 19:00:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 11 22:28:10 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/14/2024
Supervised By :mohammad ahmed 06/14/2024

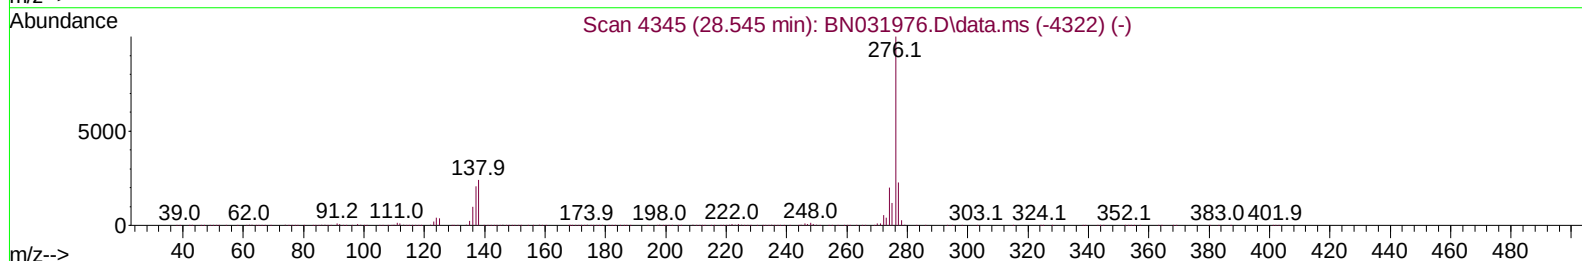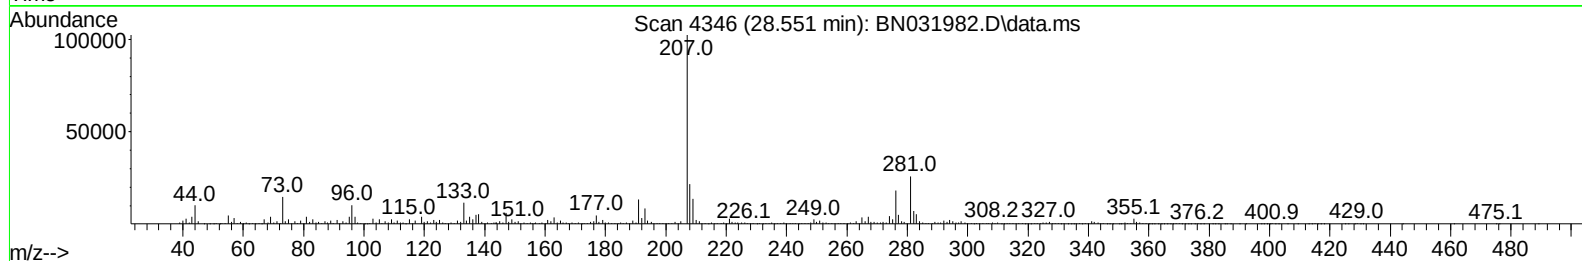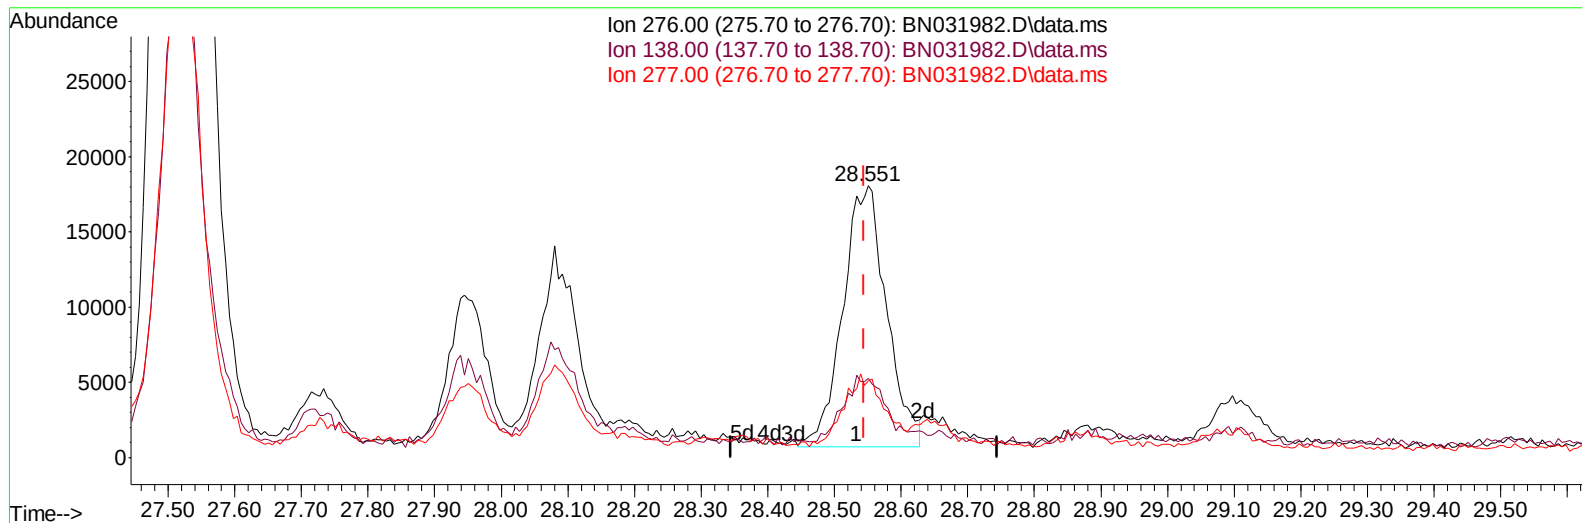

TIC: BN031982.D\data.ms

(96) Benzo(g,h,i)perylene

28.551min (+ 0.006) 1.39 ng/ul m

response 78858

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	26.10	29.09
277.00	22.50	28.22#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031982.D
 Acq On : 13 Jun 2024 18:15
 Operator : MA/JU
 Sample : P2663-07
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH694

Manual IntegrationsAPPROVED

Quant Time: Jun 13 19:02:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 11 22:28:10 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/14/2024
 Supervised By :mohammad ahmed 06/14/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.658	152		347398	20.000	ng/ul	0.00
20) Naphthalene-d8	10.440	136		1481776	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.304	164		883966	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.051	188		1516815	20.000	ng/ul	0.00
79) Chrysene-d12	21.292	240		927457	20.000	ng/ul	0.00
88) Perylene-d12	24.221	264		1103562	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.176	96		39155	4.663	ng/uL	0.00
4) Pyridine-d5	3.605	84		11686	0.494	ng/ul	0.02
7) Phenol-d5	6.840	99		816235	27.407	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.999	67		508695	29.202	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132		714236	31.431	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113		567615	23.381	ng/ul	0.00
21) Nitrobenzene-d5	8.816	128		377573	33.326	ng/ul	0.00
24) 2-Nitrophenol-d4	9.534	143		385080	32.903	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165		639684	29.278	ng/ul	0.00
31) 4-Chloroaniline-d4	10.581	131		565699	17.438	ng/ul	0.00
46) Dimethylphthalate-d6	13.722	166		1997024	32.429	ng/ul	0.00
49) Acenaphthylene-d8	13.993	160		2296675	32.434	ng/ul	0.00
54) 4-Nitrophenol-d4	14.528	143		100378	8.141	ng/ul	0.00
60) Fluorene-d10	15.298	176		1644910	31.568	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.434	200		62751	8.230	ng/ul	0.00
73) Anthracene-d10	17.151	188		2135291	32.882	ng/ul	0.00
81) Pyrene-d10	19.457	212		1777291	35.811	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.022	264		1318495	25.021	ng/ul	0.00
Target Compounds							
						Qvalue	
16) Acetophenone	8.481	105		66771	1.815	ng/ul	95
30) Naphthalene	10.493	128		81410	1.062	ng/ul	98
36) 2-Methylnaphthalene	12.110	142		79460	1.516	ng/ul	98
50) Acenaphthylene	14.028	152		151030	1.887	ng/ul	99
72) Phenanthrene	17.092	178		1222681	15.824	ng/ul	99
74) Anthracene	17.187	178		201339	2.572	ng/ul	99
77) Carbazole	17.463	167		114358	1.713	ng/ul	99
80) Fluoranthene	19.122	202		2295808	38.707	ng/ul	96
82) Pyrene	19.486	202		1674000	27.508	ng/ul	95
85) Benzo(a)anthracene	21.275	228		1020192	16.434	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.198	149		46026	1.099	ng/ul	98
87) Chrysene	21.333	228		1115262	19.233	ng/ul	97
90) Benzo(b)fluoranthene	23.304	252		1468743	22.266	ng/ul	99
91) Benzo(k)fluoranthene	23.351	252		489157m	7.557	ng/ul	
93) Benzo(a)pyrene	24.080	252		617497	9.995	ng/ul	96
94) Indeno(1,2,3-cd)pyrene	27.521	276		582501	8.182	ng/ul	94
95) Dibenzo(a,h)anthracene	27.551	278		203531m	3.502	ng/ul	
96) Benzo(g,h,i)perylene	28.551	276		78858m	1.393	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031982.D
 Acq On : 13 Jun 2024 18:15
 Operator : MA/JU
 Sample : P2663-07
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH694

Manual IntegrationsAPPROVED

Quant Time: Jun 13 19:02:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 11 22:28:10 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/14/2024
 Supervised By :mohammad ahmed 06/14/2024

