

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031962.D
 Acq On : 13 Jun 2024 05:08
 Operator : MA/JU
 Sample : P2695-21
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4D61

Quant Time: Jun 13 05:39:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 11 22:28:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.658	152	377030	20.000	ng/ul	0.00
20) Naphthalene-d8	10.440	136	1535478	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.304	164	882620	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.051	188	1439416	20.000	ng/ul	0.00
79) Chrysene-d12	21.286	240	1027278	20.000	ng/ul	0.00
88) Perylene-d12	24.221	264	1215228	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	18879	2.072	ng/uL	0.00
4) Pyridine-d5	3.587	84	225843	8.803	ng/ul	0.00
7) Phenol-d5	6.840	99	220641	6.826	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	591293	31.275	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132	641774	26.022	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	414284	15.724	ng/ul	0.00
21) Nitrobenzene-d5	8.816	128	428368	36.487	ng/ul	0.00
24) 2-Nitrophenol-d4	9.534	143	418142	34.479	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	686773	30.333	ng/ul	0.00
31) 4-Chloroaniline-d4	10.587	131	930663	27.685	ng/ul	0.00
46) Dimethylphthalate-d6	13.722	166	2272105	36.952	ng/ul	0.00
49) Acenaphthylene-d8	13.998	160	2516824	35.597	ng/ul	0.00
54) 4-Nitrophenol-d4	14.534	143	61148	4.967	ng/ul	0.01
60) Fluorene-d10	15.298	176	1794928	34.500	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.434	200	155859	21.542	ng/ul	0.00
73) Anthracene-d10	17.151	188	2549015	41.363	ng/ul	0.00
81) Pyrene-d10	19.457	212	2406245	43.772	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.021	264	2461003	42.411	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.481	105	58007	1.453	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031962.D
Acq On : 13 Jun 2024 05:08
Operator : MA/JU
Sample : P2695-21
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4D61


Quant Time: Jun 13 05:39:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 11 22:28:10 2024
Response via : Initial Calibration

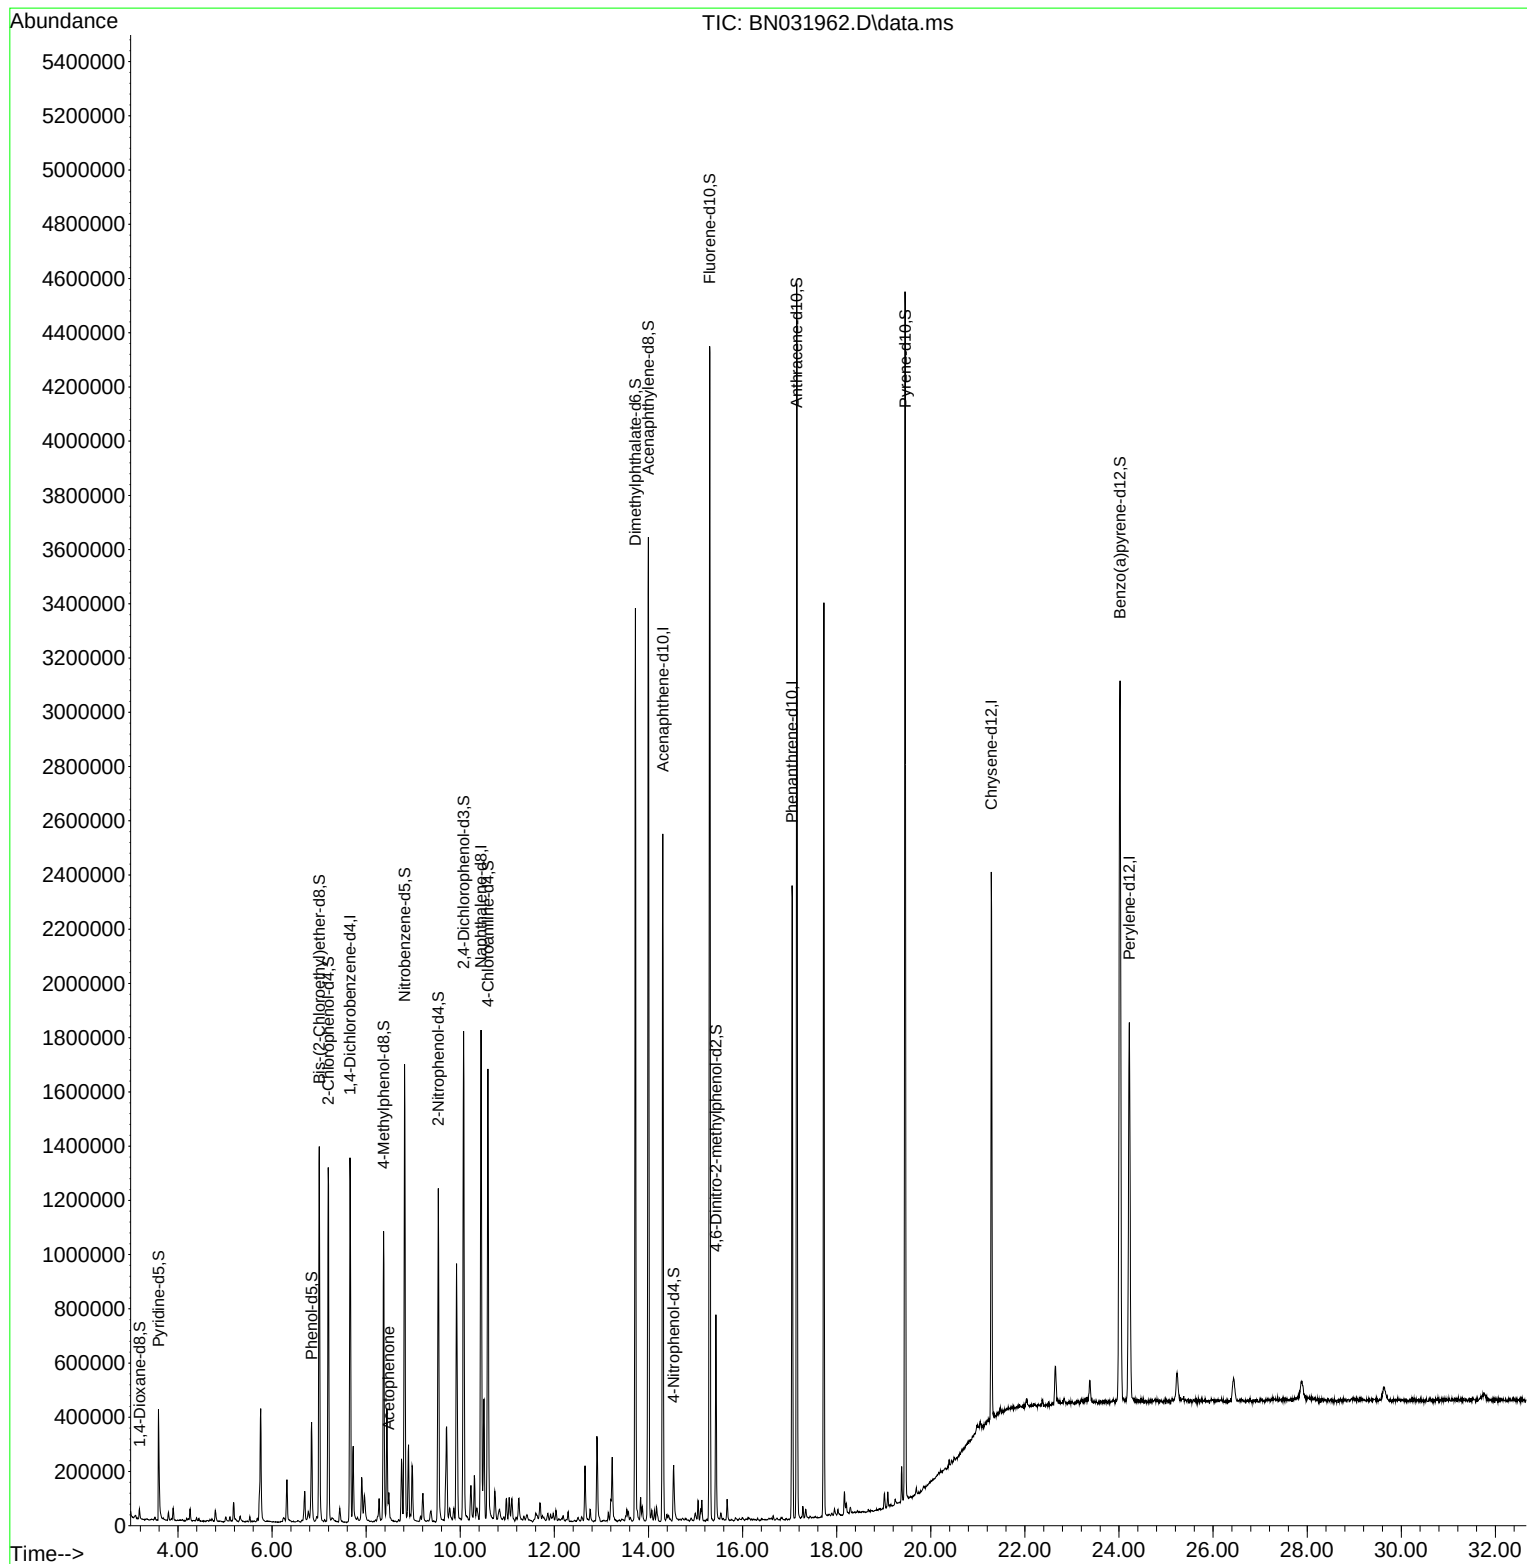

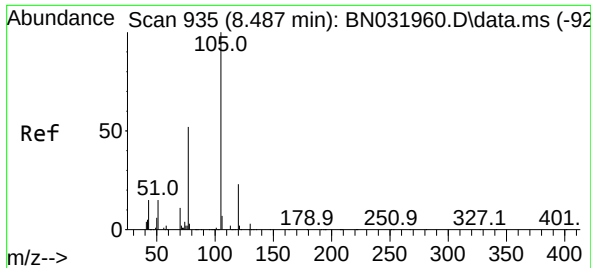

#16
 Acetophenone
 Concen: 1.453 ng/ul
 RT: 8.481 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BN031962.D
 Acq: 13 Jun 2024 05:08

Instrument :
 BNA_N
 ClientSampleId :
 A4D61

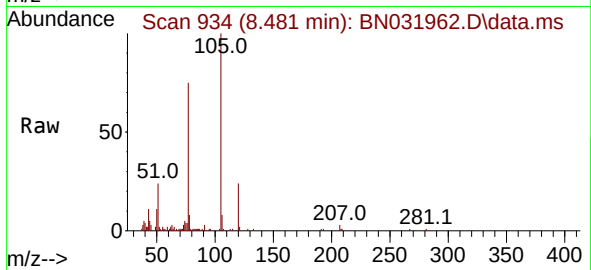

Tgt Ion:	105	Resp:	58007
Ion	Ratio	Lower	Upper
105	100		
77	75.0	58.6	87.8
51	24.0	17.2	25.8

