

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031912.D
 Acq On : 11 Jun 2024 15:45
 Operator : MA/JU
 Sample : PB161248BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK248

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031912.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	42	rVB	75324	111777	1.36%	0.132%
2	3.581	99	101	122	rBV	736074	1250539	15.21%	1.479%
3	3.899	150	155	166	rVB	72255	117134	1.42%	0.139%
4	4.334	224	229	231	rBV2	6099	9716	0.12%	0.011%
5	6.834	647	654	664	rBV	1227948	1959655	23.83%	2.318%
6	7.005	676	683	692	rBV	1062613	1695694	20.62%	2.005%
7	7.193	707	715	727	rBV	1292487	2039979	24.81%	2.413%
8	7.658	786	794	802	rBV	942234	1566516	19.05%	1.853%
9	8.369	906	915	928	rBV	1545563	2594353	31.55%	3.068%
10	8.816	983	991	1004	rBV	1245797	2054729	24.99%	2.430%
11	9.534	1105	1113	1131	rBV	1001478	1629911	19.82%	1.928%
12	10.069	1196	1204	1226	rBV	1439783	2570841	31.27%	3.040%
13	10.440	1259	1267	1277	rVB	1422315	2428643	29.54%	2.872%
14	10.587	1283	1292	1312	rBV	1476419	2757524	33.54%	3.261%
15	12.040	1534	1539	1548	rBV	22027	46485	0.57%	0.055%
16	13.722	1817	1825	1839	rBV	3111556	4406174	53.59%	5.211%
17	13.998	1864	1872	1891	rBV	3379531	5102543	62.06%	6.034%
18	14.304	1917	1924	1936	rBV	2440325	3568453	43.40%	4.220%
19	14.410	1940	1942	1949	rVB7	5276	9306	0.11%	0.011%
20	14.516	1954	1960	1982	rBV	1280282	2171861	26.41%	2.569%
21	14.716	1991	1994	2004	rVB9	5768	12435	0.15%	0.015%
22	15.298	2086	2093	2102	rBV	4246245	6406703	77.92%	7.577%
23	15.428	2108	2115	2130	rBV	1299777	1826977	22.22%	2.161%
24	15.540	2130	2134	2140	rVB3	21536	36591	0.45%	0.043%
25	16.739	2334	2338	2343	rVB5	5440	8495	0.10%	0.010%
26	16.839	2348	2355	2362	rBV	8007	16269	0.20%	0.019%
27	17.051	2384	2391	2401	rBV	3037360	4434835	53.94%	5.245%
28	17.151	2401	2408	2423	rBV	4824660	7043975	85.67%	8.330%
29	17.445	2454	2458	2462	rBV3	6427	8883	0.11%	0.011%
30	19.016	2721	2725	2729	rBV2	57791	83303	1.01%	0.099%
31	19.086	2733	2737	2742	rBV	59251	85681	1.04%	0.101%
32	19.451	2793	2799	2810	rBV	5780502	8207435	99.82%	9.706%
33	21.292	3106	3112	3121	rVB2	3296918	4904267	59.65%	5.800%
34	24.021	3567	3576	3590	rVB2	3458881	8222226	100.00%	9.724%
35	24.221	3601	3610	3621	rBV	2090943	5167367	62.85%	6.111%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031912.D
Acq On : 11 Jun 2024 15:45
Operator : MA/JU
Sample : PB161248BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK248

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 84557275

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031912.D
Acq On : 11 Jun 2024 15:45
Operator : MA/JU
Sample : PB161248BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK248

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

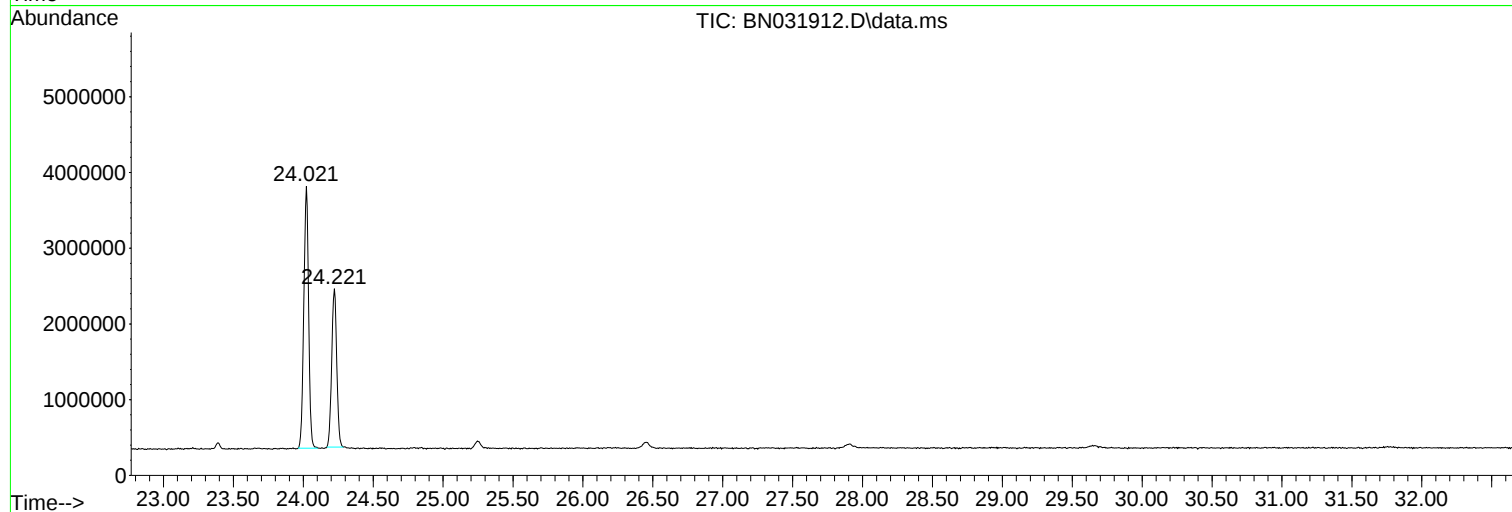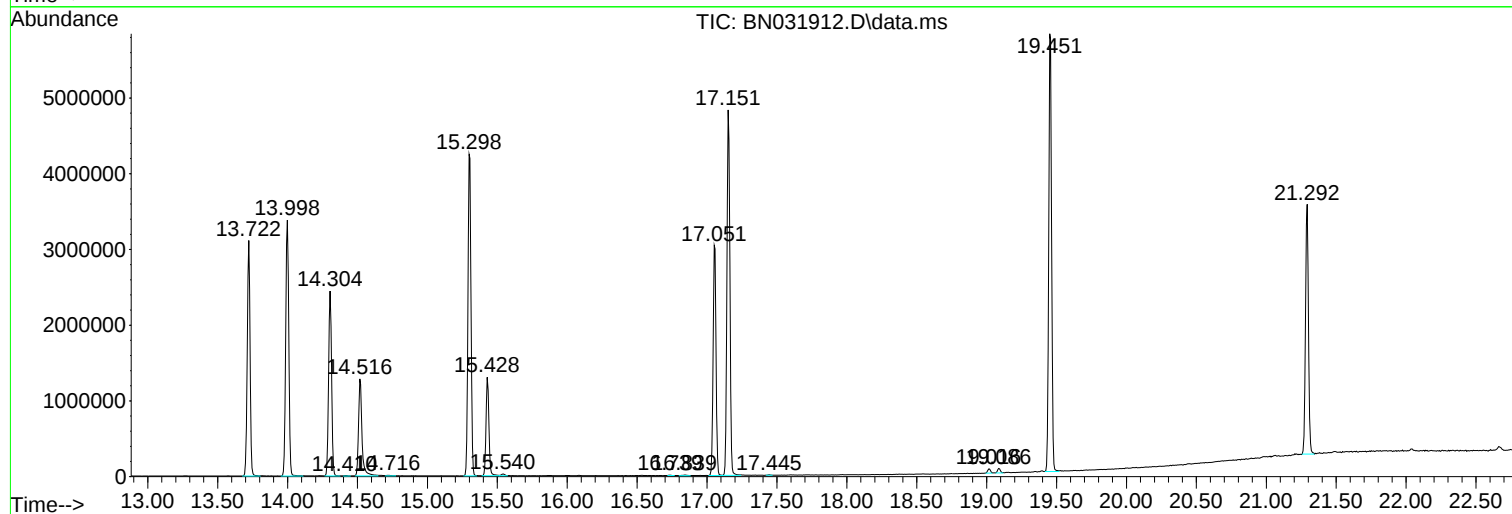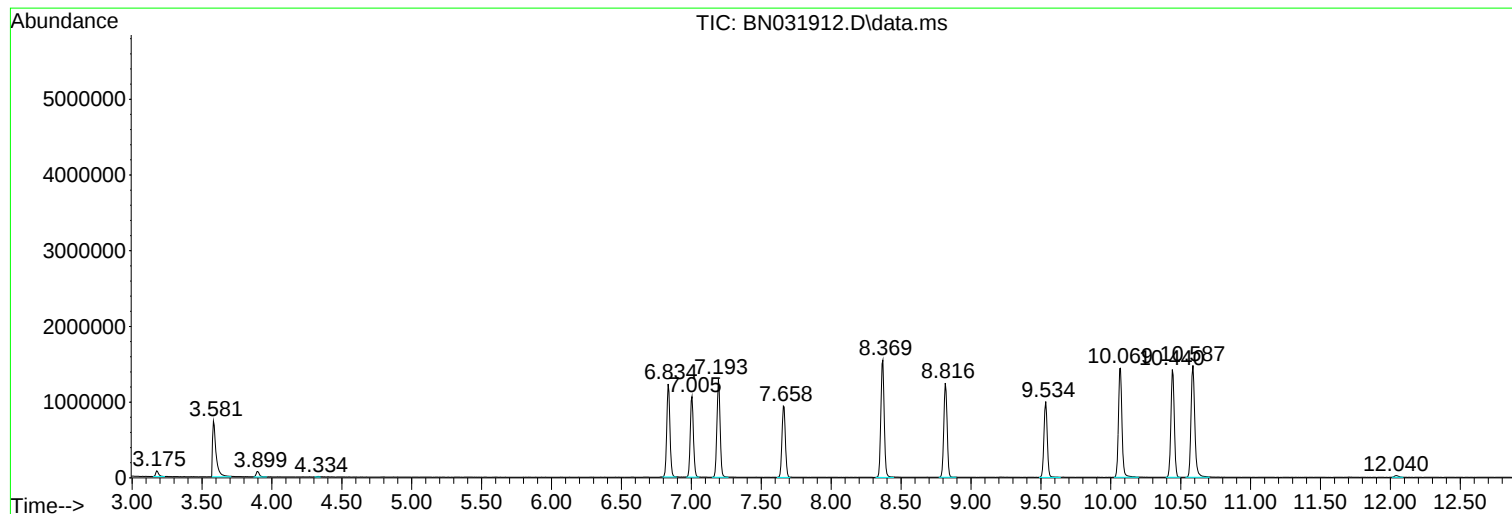

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031912.D
Acq On : 11 Jun 2024 15:45
Operator : MA/JU
Sample : PB161248BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK248

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031912.D
Acq On : 11 Jun 2024 15:45
Operator : MA/JU
Sample : PB161248BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK248

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc