

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031914.D
 Acq On : 11 Jun 2024 17:21
 Operator : MA/JU
 Sample : P2642-18DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4DG2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	39	rVB	12044	19463	0.14%	0.009%
2	3.628	106	109	114	rBV4	8970	15992	0.12%	0.007%
3	3.893	150	154	160	rVB	18194	26064	0.19%	0.012%
4	6.034	512	518	521	rBV3	10633	15307	0.11%	0.007%
5	6.857	645	658	673	rBV2	1450226	2693824	19.75%	1.254%
6	6.999	676	682	691	rBV	220218	342262	2.51%	0.159%
7	7.093	691	698	705	rVB	407528	609875	4.47%	0.284%
8	7.222	708	720	728	rBV2	939854	1874273	13.74%	0.872%
9	7.546	766	775	783	rBV	546792	874209	6.41%	0.407%
10	7.657	786	794	796	rBV	1122672	1722874	12.63%	0.802%
11	7.693	796	800	808	rVB	2113828	3355665	24.60%	1.562%
12	7.905	829	836	841	rBV8	6964	13993	0.10%	0.007%
13	8.004	845	853	864	rVV	1439748	2380308	17.45%	1.108%
14	8.369	907	915	923	rBV	314891	536731	3.94%	0.250%
15	8.463	923	931	950	rVV	1309913	2090322	15.33%	0.973%
16	8.722	968	975	984	rVB	1167452	1987992	14.57%	0.925%
17	8.816	984	991	994	rBV	251390	431376	3.16%	0.201%
18	8.857	994	998	1007	rVB	448157	719285	5.27%	0.335%
19	9.210	1052	1058	1065	rBV4	12876	25654	0.19%	0.012%
20	9.534	1102	1113	1114	rBV	194045	299902	2.20%	0.140%
21	9.563	1114	1118	1131	rVB	476514	815889	5.98%	0.380%
22	9.769	1148	1153	1162	rBV10	5920	13735	0.10%	0.006%
23	9.863	1162	1169	1178	rVV	898083	1390556	10.19%	0.647%
24	10.093	1197	1208	1222	rBV2	740812	1802344	13.21%	0.839%
25	10.440	1259	1267	1271	rBV	1674367	2873722	21.07%	1.338%
26	10.493	1271	1276	1285	rVV	3185476	5299104	38.85%	2.466%
27	10.587	1285	1292	1310	rVV	162005	377127	2.76%	0.176%
28	10.740	1314	1318	1326	rVB3	9443	15473	0.11%	0.007%
29	11.016	1359	1365	1370	rBV8	9289	17342	0.13%	0.008%
30	11.075	1370	1375	1383	rVB6	10642	20683	0.15%	0.010%
31	11.193	1389	1395	1401	rBV2	28870	65965	0.48%	0.031%
32	11.734	1479	1487	1505	rBV	1626419	2678929	19.64%	1.247%
33	12.540	1617	1624	1628	rBV	16895	25875	0.19%	0.012%
34	12.651	1637	1643	1649	rBV5	9549	19068	0.14%	0.009%
35	12.728	1649	1656	1662	rVV	1177497	1832237	13.43%	0.853%
36	12.798	1662	1668	1683	rVV	2423741	4027171	29.53%	1.874%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031914.D
 Acq On : 11 Jun 2024 17:21
 Operator : MA/JU
 Sample : P2642-18DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4DG2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

37	12.934	1683	1691	1694	rVV8	12162	40715	0.30%	0.019%
38	12.969	1695	1697	1701	rVB5	13028	16238	0.12%	0.008%
39	13.175	1725	1732	1738	rVV	1718343	2674444	19.61%	1.245%
40	13.222	1738	1740	1747	rVB2	12590	21708	0.16%	0.010%
41	13.357	1758	1763	1773	rVB2	21154	35772	0.26%	0.017%
42	13.569	1793	1799	1803	rBV6	10253	15199	0.11%	0.007%
43	13.722	1816	1825	1833	rBV	744559	1051627	7.71%	0.489%
44	13.892	1846	1854	1863	rBV	3457234	4864517	35.66%	2.264%
45	14.028	1864	1877	1886	rVB2	4676548	8144657	59.71%	3.791%
46	14.304	1917	1924	1929	rVV	2810428	4114132	30.16%	1.915%
47	14.369	1929	1935	1942	rVV	4070543	5906698	43.30%	2.749%
48	14.434	1942	1946	1953	rVB	61495	83430	0.61%	0.039%
49	14.539	1953	1964	1974	rBV3	3276095	6570887	48.17%	3.058%
50	14.616	1974	1977	1982	rVV	75439	147914	1.08%	0.069%
51	14.681	1982	1988	2008	rVV	1999037	2892210	21.20%	1.346%
52	14.816	2009	2011	2018	rVB6	8887	17087	0.13%	0.008%
53	14.934	2026	2031	2043	rVB2	41345	68899	0.51%	0.032%
54	15.139	2056	2066	2080	rBV	5489062	7404012	54.28%	3.446%
55	15.298	2085	2093	2098	rBV	1078219	1625204	11.92%	0.756%
56	15.357	2098	2103	2110	rVV	5421249	7682529	56.32%	3.576%
57	15.428	2110	2115	2127	rVB	249725	370889	2.72%	0.173%
58	15.604	2141	2145	2152	rVB	26937	37479	0.27%	0.017%
59	15.851	2182	2187	2190	rBV3	11835	24189	0.18%	0.011%
60	15.892	2190	2194	2198	rVV	24322	38152	0.28%	0.018%
61	16.028	2212	2217	2224	rBV5	36798	75068	0.55%	0.035%
62	16.216	2243	2249	2254	rBV2	45370	63220	0.46%	0.029%
63	16.357	2266	2273	2283	rBV	5793128	8432561	61.82%	3.925%
64	16.704	2325	2332	2342	rBV	3805933	5535179	40.58%	2.576%
65	16.869	2353	2360	2369	rVB7	30682	91942	0.67%	0.043%
66	16.975	2374	2378	2380	rBV5	11728	18965	0.14%	0.009%
67	17.057	2385	2392	2395	rVV	3477015	5073484	37.20%	2.361%
68	17.098	2395	2399	2404	rVV	2379601	3344019	24.52%	1.556%
69	17.151	2404	2408	2411	rVV	1212892	1858624	13.63%	0.865%
70	17.186	2411	2414	2427	rVB	3155948	4219772	30.94%	1.964%
71	17.333	2437	2439	2447	rVB4	13837	23881	0.18%	0.011%
72	17.469	2457	2462	2466	rVB	30519	45989	0.34%	0.021%
73	17.604	2480	2485	2489	rBV7	11951	18879	0.14%	0.009%
74	17.669	2493	2496	2502	rVV2	19806	32290	0.24%	0.015%
75	17.733	2502	2507	2512	rVB	147906	188975	1.39%	0.088%
76	17.957	2540	2545	2551	rBV2	101568	171689	1.26%	0.080%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031914.D
 Acq On : 11 Jun 2024 17:21
 Operator : MA/JU
 Sample : P2642-18DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4DG2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

77	18.027	2551	2557	2563	rBV	6536736	8502364	62.34%	3.957%
78	18.122	2568	2573	2577	rVB5	24935	46005	0.34%	0.021%
79	18.245	2590	2594	2598	rBV3	16982	30538	0.22%	0.014%
80	18.327	2604	2608	2612	rBV4	38567	65762	0.48%	0.031%
81	18.416	2620	2623	2628	rVB	24050	31255	0.23%	0.015%
82	18.475	2629	2633	2643	rVB	296601	419471	3.08%	0.195%
83	18.910	2704	2707	2711	rVB2	115229	128796	0.94%	0.060%
84	19.016	2722	2725	2727	rBV3	20534	24849	0.18%	0.012%
85	19.045	2727	2730	2735	rVV2	65097	95550	0.70%	0.044%
86	19.122	2736	2743	2753	rVB	8172094	10830804	79.41%	5.041%
87	19.245	2761	2764	2771	rBV4	54663	95759	0.70%	0.045%
88	19.363	2780	2784	2788	rBV	72505	102473	0.75%	0.048%
89	19.457	2794	2800	2801	rBV	1596503	2098039	15.38%	0.977%
90	19.486	2801	2805	2816	rVB	3948273	5501157	40.33%	2.560%
91	20.151	2915	2918	2923	rBV	88406	102270	0.75%	0.048%
92	21.127	3081	3084	3089	rVB2	160358	194493	1.43%	0.091%
93	21.204	3092	3097	3103	rVV	9562497	12705906	93.15%	5.914%
94	21.280	3103	3110	3116	rVV2	6042628	13639762	100.00%	6.349%
95	21.339	3116	3120	3129	rVB	7675594	10736182	78.71%	4.997%
96	23.363	3455	3464	3477	rVB	5090144	11356137	83.26%	5.286%
97	24.021	3569	3576	3589	rVB2	762104	1899920	13.93%	0.884%
98	24.221	3602	3610	3626	rVB	2176472	5853359	42.91%	2.724%
99	27.574	4169	4180	4200	rVB	1633868	6034582	44.24%	2.809%




Sum of corrected areas: 214849149

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031914.D
Acq On : 11 Jun 2024 17:21
Operator : MA/JU
Sample : P2642-18DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4DG2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

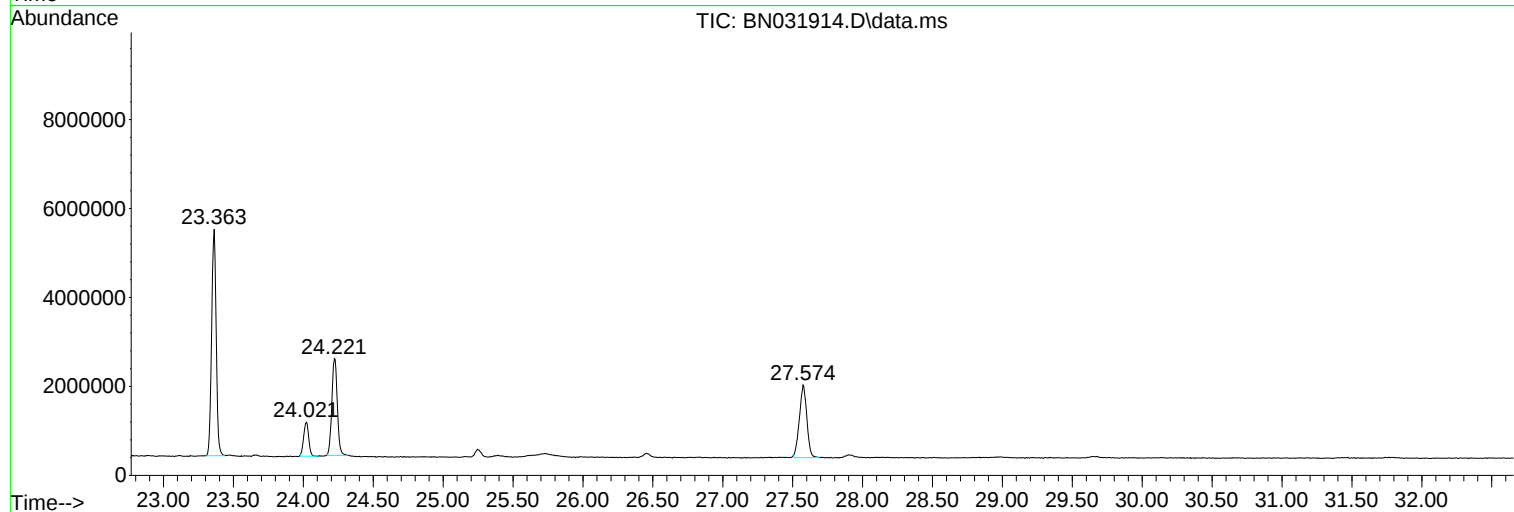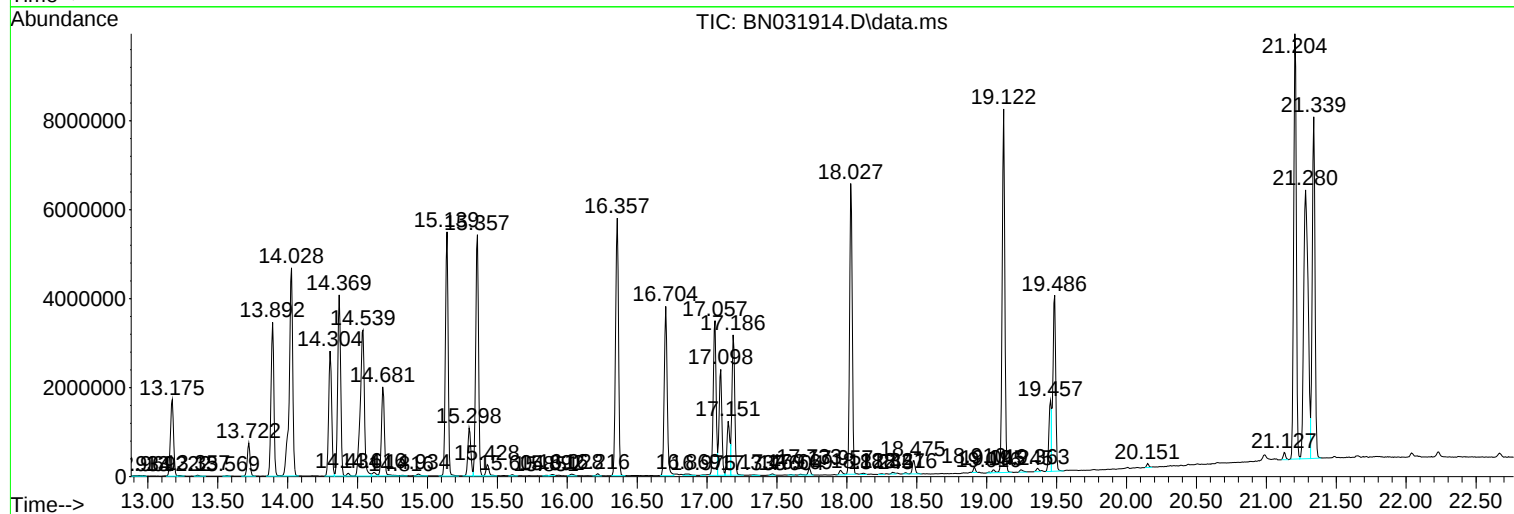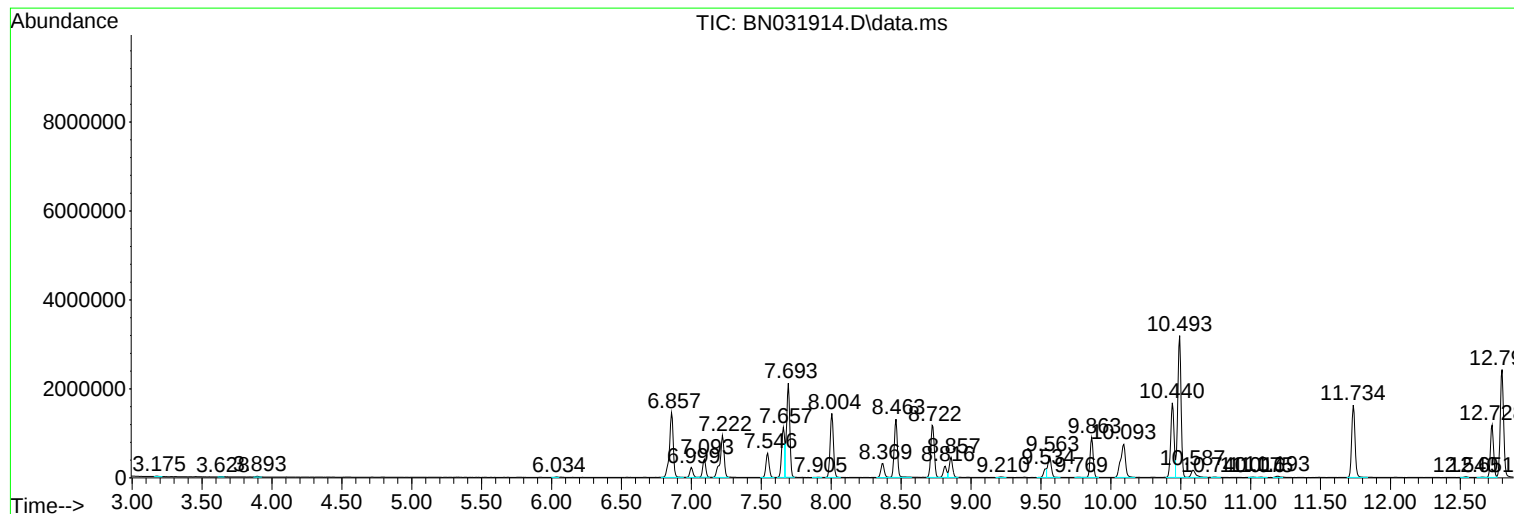

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031914.D
Acq On : 11 Jun 2024 17:21
Operator : MA/JU
Sample : P2642-18DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4DG2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031914.D
Acq On : 11 Jun 2024 17:21
Operator : MA/JU
Sample : P2642-18DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4DG2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc