

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031915.D
 Acq On : 11 Jun 2024 18:21
 Operator : MA/JU
 Sample : P2642-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4BH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031915.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	28	32	39	rVB	40992	58273	0.93%	0.081%
2	3.446	74	78	84	rBV	24565	43793	0.70%	0.061%
3	3.581	99	101	119	rBV	350177	612789	9.76%	0.854%
4	3.893	150	154	160	rVB	22525	33048	0.53%	0.046%
5	4.117	187	192	193	rBV5	6146	9122	0.15%	0.013%
6	5.758	466	471	477	rBV	22856	37837	0.60%	0.053%
7	5.928	494	500	505	rBV9	3357	7497	0.12%	0.010%
8	6.828	645	653	666	rBV	719474	1180626	18.81%	1.646%
9	6.999	673	682	691	rBV	640612	1001258	15.95%	1.396%
10	7.187	707	714	725	rBV	727317	1199110	19.10%	1.671%
11	7.275	725	729	740	rVB2	11591	25205	0.40%	0.035%
12	7.658	785	794	801	rBV	1100918	1777591	28.31%	2.478%
13	7.728	801	806	815	rVB2	24251	49106	0.78%	0.068%
14	8.363	906	914	920	rBV	944977	1576985	25.12%	2.198%
15	8.422	920	924	931	rVB	52424	92285	1.47%	0.129%
16	8.811	983	990	999	rBV	713751	1218110	19.40%	1.698%
17	9.210	1053	1058	1065	rBV3	9629	14734	0.23%	0.021%
18	9.381	1079	1087	1099	rBV	102985	164609	2.62%	0.229%
19	9.528	1104	1112	1122	rBV	577130	967854	15.42%	1.349%
20	9.763	1147	1152	1160	rBV10	5261	12222	0.19%	0.017%
21	10.063	1196	1203	1221	rBV	922715	1599713	25.48%	2.230%
22	10.440	1259	1267	1274	rBV	1656530	2828511	45.05%	3.942%
23	10.587	1284	1292	1312	rBV	869739	1684532	26.83%	2.348%
24	10.993	1355	1361	1367	rBV2	27031	50029	0.80%	0.070%
25	11.187	1388	1394	1407	rBV	64978	152469	2.43%	0.213%
26	12.034	1532	1538	1545	rBV2	16843	30778	0.49%	0.043%
27	12.110	1547	1551	1558	rVB2	10777	18127	0.29%	0.025%
28	12.334	1583	1589	1596	rVB2	10113	20461	0.33%	0.029%
29	13.128	1720	1724	1730	rVB5	11758	19235	0.31%	0.027%
30	13.481	1776	1784	1792	rBV10	8603	28109	0.45%	0.039%
31	13.628	1802	1809	1813	rBV3	10665	22345	0.36%	0.031%
32	13.675	1813	1817	1818	rBV3	7290	8848	0.14%	0.012%
33	13.722	1818	1825	1834	rVB	1823327	2652865	42.26%	3.698%
34	13.857	1845	1848	1851	rVB5	5332	6565	0.10%	0.009%
35	13.998	1863	1872	1882	rBV	2049417	3211263	51.15%	4.476%
36	14.128	1891	1894	1900	rVB6	6365	9400	0.15%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031915.D
 Acq On : 11 Jun 2024 18:21
 Operator : MA/JU
 Sample : P2642-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4BH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

37	14.204	1903	1907	1912	rVB7	5839	9347	0.15%	0.013%
38	14.304	1916	1924	1931	rVV	2795121	4086070	65.09%	5.695%
39	14.369	1931	1935	1943	rVB	77124	125731	2.00%	0.175%
40	14.516	1954	1960	1973	rBV	708057	1301045	20.72%	1.813%
41	14.616	1975	1977	1984	rVV5	16619	26001	0.41%	0.036%
42	14.704	1987	1992	2002	rVB	52945	100866	1.61%	0.141%
43	14.828	2009	2013	2019	rVB8	6012	10657	0.17%	0.015%
44	14.975	2036	2038	2042	rVB5	5880	7137	0.11%	0.010%
45	15.022	2042	2046	2048	rBV5	5134	7577	0.12%	0.011%
46	15.093	2053	2058	2062	rBV6	17078	30314	0.48%	0.042%
47	15.298	2086	2093	2099	rBV	2839316	4025412	64.12%	5.611%
48	15.351	2099	2102	2109	rVB2	84986	120000	1.91%	0.167%
49	15.428	2109	2115	2127	rBV	689077	1017199	16.20%	1.418%
50	15.516	2127	2130	2132	rBV3	11850	15217	0.24%	0.021%
51	15.651	2149	2153	2162	rVB	26420	51597	0.82%	0.072%
52	15.734	2163	2167	2171	rBV6	5907	7958	0.13%	0.011%
53	15.792	2173	2177	2186	rVB	21732	47925	0.76%	0.067%
54	15.869	2186	2190	2191	rBV3	10404	13037	0.21%	0.018%
55	16.028	2213	2217	2224	rBV7	16804	33797	0.54%	0.047%
56	16.169	2238	2241	2245	rVB6	9474	11825	0.19%	0.016%
57	16.410	2278	2282	2287	rVB5	13991	25924	0.41%	0.036%
58	16.710	2330	2333	2340	rVB2	27672	46636	0.74%	0.065%
59	16.810	2347	2350	2353	rVB4	28166	36436	0.58%	0.051%
60	16.869	2357	2360	2367	rVB	54024	85361	1.36%	0.119%
61	16.934	2368	2371	2374	rBV5	15884	18459	0.29%	0.026%
62	17.051	2385	2391	2395	rBV	3284948	4973268	79.22%	6.932%
63	17.092	2395	2398	2403	rVV	1018909	1475706	23.51%	2.057%
64	17.151	2403	2408	2419	rVB	2940400	4381947	69.80%	6.107%
65	17.463	2457	2461	2465	rVB	69809	94456	1.50%	0.132%
66	17.645	2487	2492	2499	rVB5	33314	81671	1.30%	0.114%
67	17.928	2536	2540	2541	rBV	88370	99312	1.58%	0.138%
68	17.957	2541	2545	2547	rBV	146030	209464	3.34%	0.292%
69	18.122	2568	2573	2577	rBV2	150324	268030	4.27%	0.374%
70	18.286	2597	2601	2604	rBV3	48427	61926	0.99%	0.086%
71	18.434	2623	2626	2630	rVB	70575	85894	1.37%	0.120%
72	18.481	2631	2634	2637	rVB2	43156	56912	0.91%	0.079%
73	18.522	2638	2641	2644	rBV4	38903	50708	0.81%	0.071%
74	18.722	2672	2675	2680	rBV4	49136	67536	1.08%	0.094%
75	19.116	2737	2742	2750	rVB	1343606	1795605	28.60%	2.503%
76	19.245	2761	2764	2771	rVB2	83637	129207	2.06%	0.180%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031915.D
Acq On : 11 Jun 2024 18:21
Operator : MA/JU
Sample : P2642-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BH1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

77	19.451	2794	2799	2803	rBV	3854377	5771672	91.94%	8.044%
78	20.986	3057	3060	3067	rVB4	173540	288512	4.60%	0.402%
79	21.292	3105	3112	3117	rBV	3882407	6277954	100.00%	8.750%
80	21.333	3117	3119	3130	rVB	487783	667450	10.63%	0.930%
81	23.292	3448	3452	3460	rBV	226712	560633	8.93%	0.781%
82	24.021	3568	3576	3583	rBV2	1953142	4575064	72.88%	6.377%
83	24.221	3602	3610	3632	rVB	2206442	6087436	96.97%	8.485%




Sum of corrected areas: 71747195

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031915.D
Acq On : 11 Jun 2024 18:21
Operator : MA/JU
Sample : P2642-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

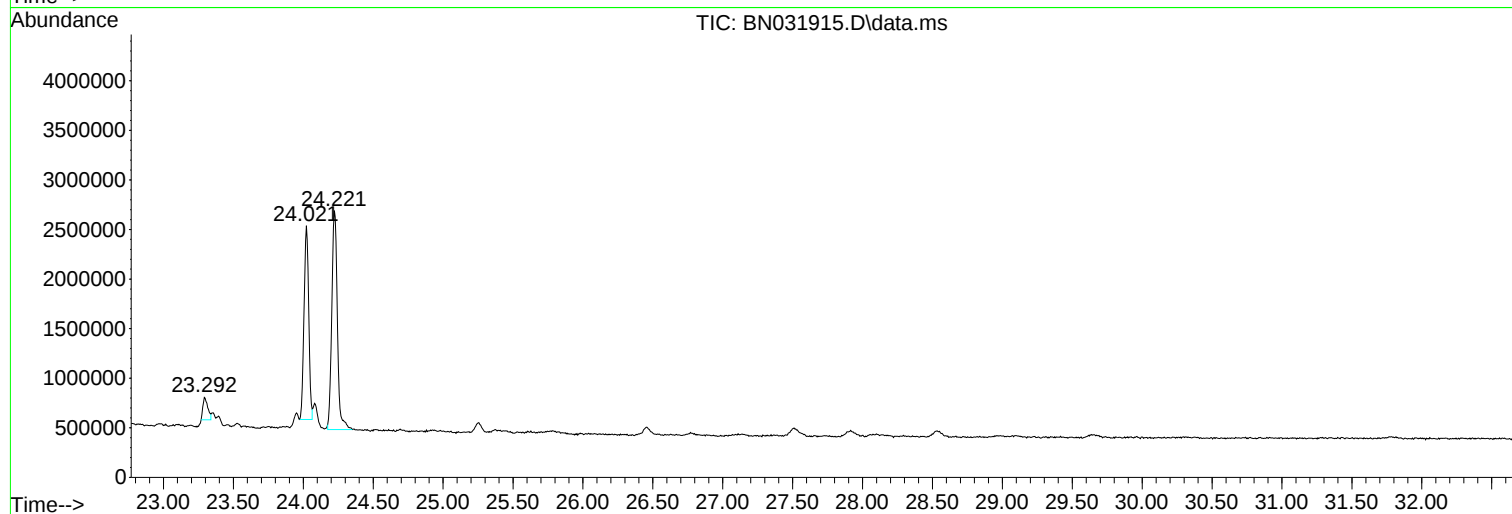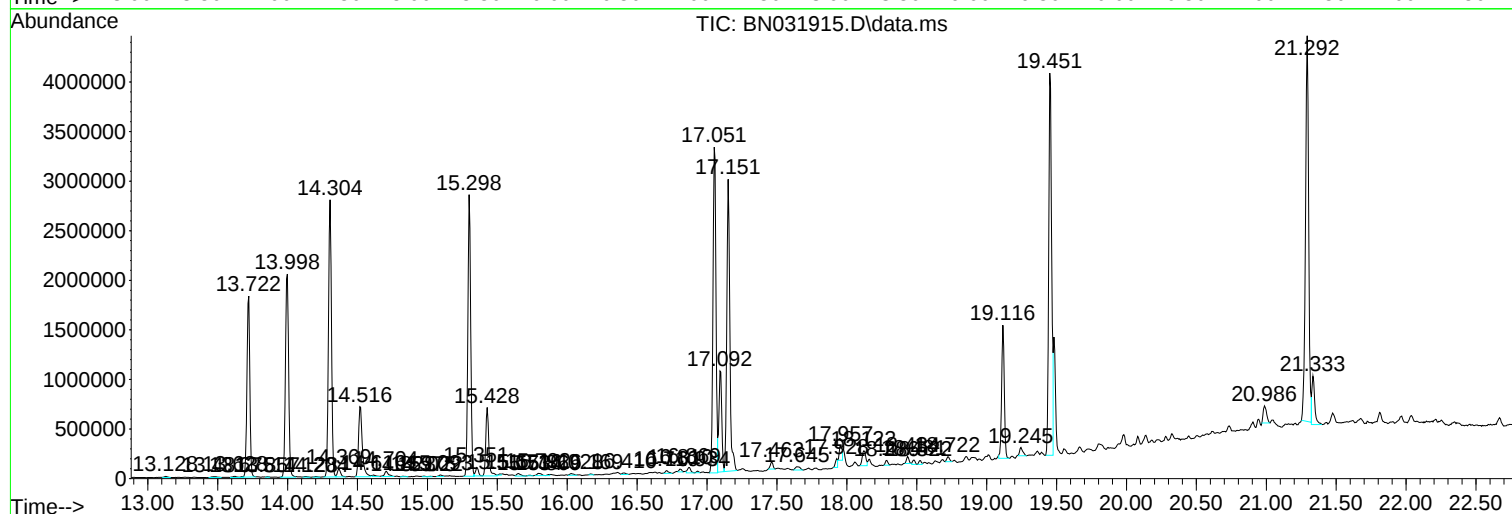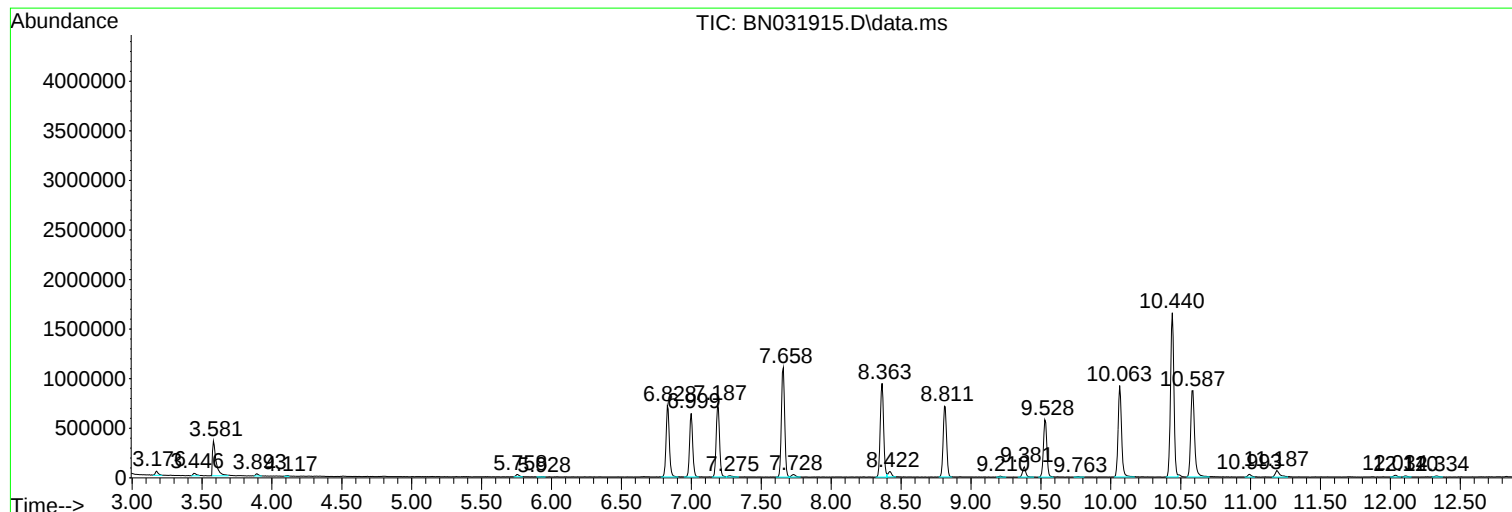

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031915.D
Acq On : 11 Jun 2024 18:21
Operator : MA/JU
Sample : P2642-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031915.D
Acq On : 11 Jun 2024 18:21
Operator : MA/JU
Sample : P2642-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc