

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031917.D
 Acq On : 11 Jun 2024 19:40
 Operator : MA/JU
 Sample : PB161309BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK309

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	28	32	40	rVB	74349	99548	1.26%	0.117%
2	3.581	98	101	121	rBV	820740	1361350	17.22%	1.597%
3	3.893	150	154	163	rVB	14034	23119	0.29%	0.027%
4	6.834	645	654	669	rBV	1154451	1870759	23.67%	2.194%
5	7.005	672	683	695	rBV	999905	1601481	20.26%	1.878%
6	7.193	707	715	726	rBV	1213164	1930395	24.42%	2.264%
7	7.658	787	794	804	rBV	1084945	1765912	22.34%	2.071%
8	8.369	906	915	929	rBV	1474622	2491311	31.52%	2.922%
9	8.816	983	991	1003	rBV	1185423	1949046	24.66%	2.286%
10	9.534	1106	1113	1127	rBV	959528	1571310	19.88%	1.843%
11	10.069	1194	1204	1226	rBV	1395654	2504439	31.68%	2.937%
12	10.440	1258	1267	1276	rBV	1634987	2798229	35.40%	3.282%
13	10.587	1284	1292	1310	rBV	1539027	2727683	34.51%	3.199%
14	12.040	1532	1539	1551	rVB2	25312	51050	0.65%	0.060%
15	13.722	1818	1825	1838	rBV	2878025	4150016	52.50%	4.867%
16	13.998	1864	1872	1886	rBV	3177639	4924120	62.29%	5.775%
17	14.304	1917	1924	1937	rBV	2736309	4128135	52.22%	4.842%
18	14.516	1953	1960	1983	rBV	1264919	2111217	26.71%	2.476%
19	14.722	1989	1995	2003	rVB10	5108	11061	0.14%	0.013%
20	15.298	2086	2093	2103	rBV	4227325	6093776	77.09%	7.147%
21	15.428	2109	2115	2130	rBV	1208977	1715557	21.70%	2.012%
22	15.540	2130	2134	2140	rVB2	20696	33999	0.43%	0.040%
23	16.834	2351	2354	2359	rBV2	6853	10143	0.13%	0.012%
24	17.051	2384	2391	2401	rBV	3580090	5078101	64.24%	5.956%
25	17.151	2401	2408	2420	rBV	4692771	6652828	84.16%	7.803%
26	19.016	2721	2725	2730	rVB2	54403	78349	0.99%	0.092%
27	19.086	2732	2737	2743	rBV	60227	88676	1.12%	0.104%
28	19.386	2786	2788	2793	rBV4	13666	18307	0.23%	0.021%
29	19.451	2793	2799	2811	rBV	5582356	7807332	98.77%	9.157%
30	21.292	3106	3112	3121	rVB	3877496	5626898	71.18%	6.600%
31	24.021	3567	3576	3589	rVB2	3230844	7904848	100.00%	9.271%
32	24.221	3601	3610	3622	rVB	2489402	6083315	76.96%	7.135%




Sum of corrected areas: 85262310

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031917.D
Acq On : 11 Jun 2024 19:40
Operator : MA/JU
Sample : PB161309BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK309

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

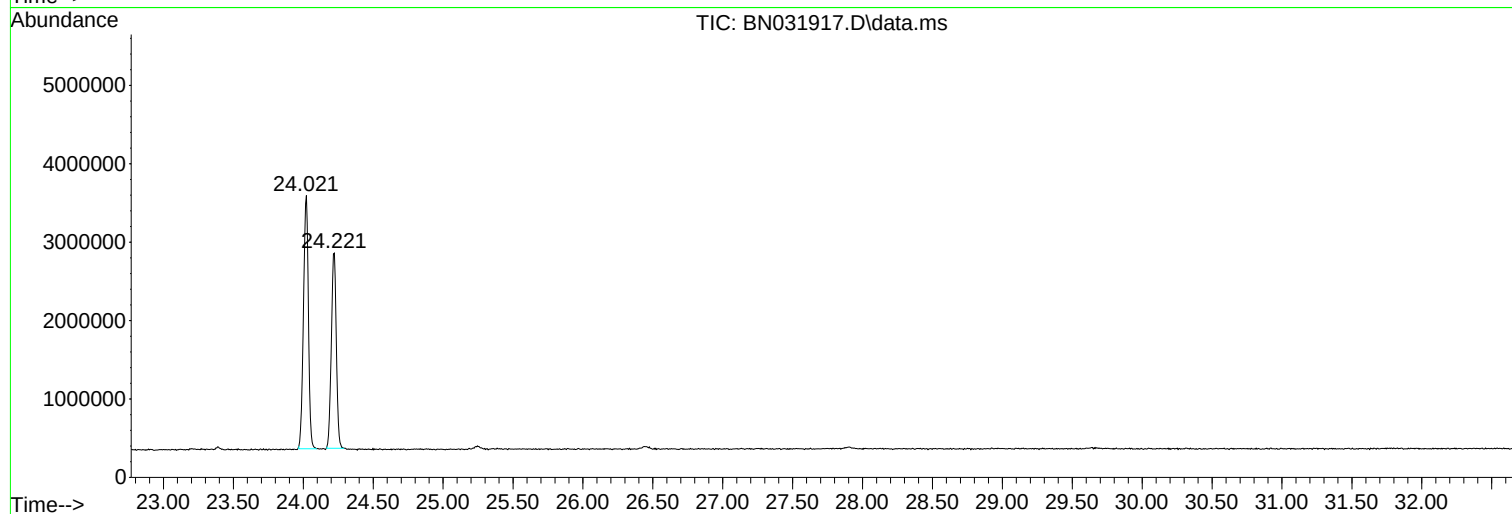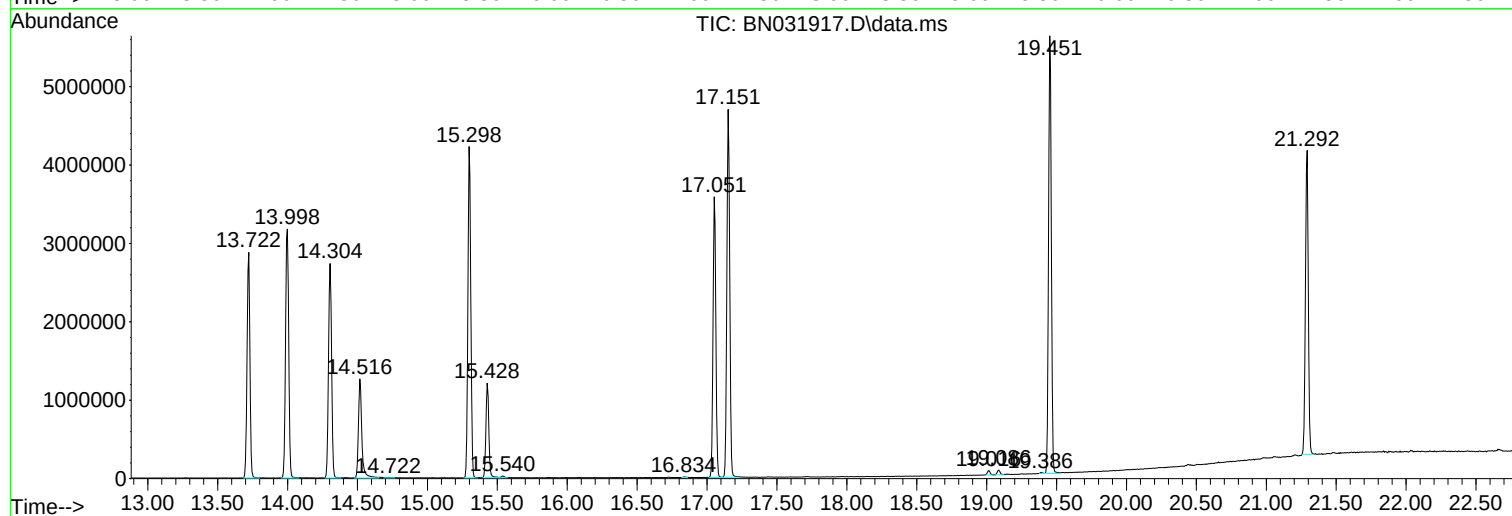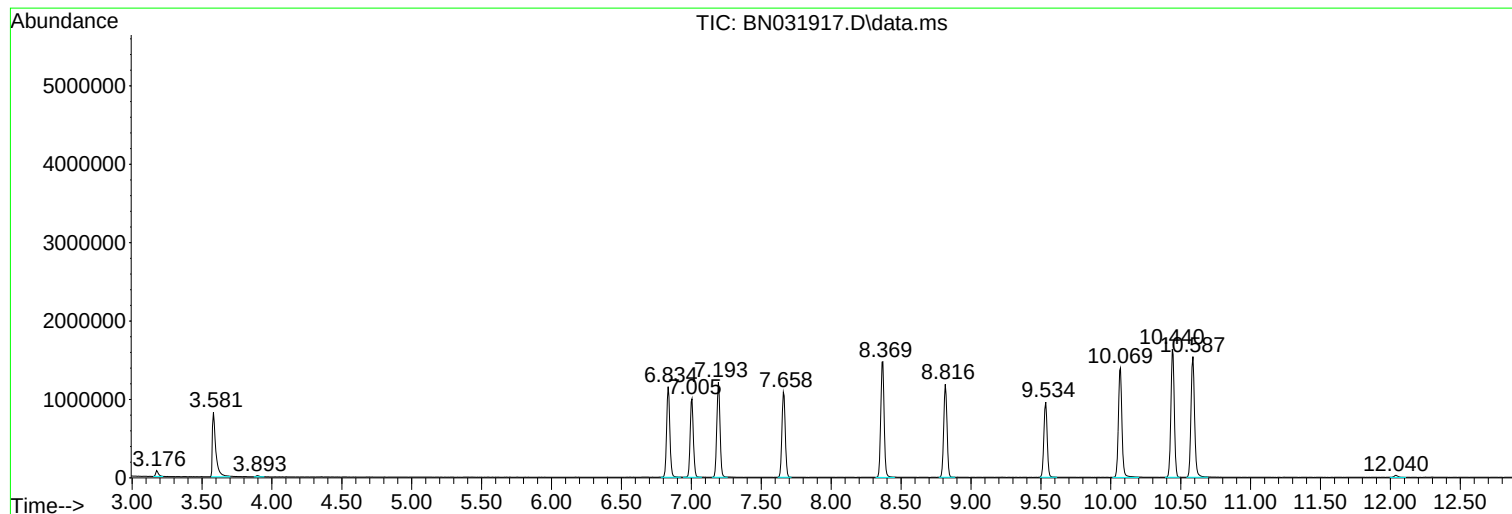

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031917.D
Acq On : 11 Jun 2024 19:40
Operator : MA/JU
Sample : PB161309BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK309

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031917.D
Acq On : 11 Jun 2024 19:40
Operator : MA/JU
Sample : PB161309BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK309

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc