

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031933.D
 Acq On : 12 Jun 2024 09:29
 Operator : MA/JU
 Sample : PB161332BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK332

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031933.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.170	27	31	43	rVB	81724	129756	1.47%	0.135%
2	3.575	97	100	129	rBV	987975	1661816	18.89%	1.734%
3	3.887	149	153	161	rVB	17534	29240	0.33%	0.031%
4	6.828	646	653	665	rBV	1453490	2337796	26.57%	2.439%
5	6.993	672	681	692	rBV	1188596	1909763	21.70%	1.992%
6	7.187	707	714	724	rBV	1485659	2389849	27.16%	2.493%
7	7.652	786	793	805	rBV	1333145	2148807	24.42%	2.242%
8	8.363	905	914	928	rBV	1849632	3112380	35.37%	3.247%
9	8.810	981	990	1002	rBV	1455171	2408220	27.37%	2.513%
10	9.528	1104	1112	1123	rBV	1187331	1995503	22.68%	2.082%
11	10.063	1194	1203	1218	rBV	1805606	3174727	36.08%	3.312%
12	10.434	1257	1266	1275	rBV	2004679	3432476	39.01%	3.581%
13	10.581	1283	1291	1304	rBV	1899987	3283433	37.32%	3.426%
14	12.034	1532	1538	1548	rBV	32321	59765	0.68%	0.062%
15	13.716	1816	1824	1837	rBV	3402161	4783469	54.36%	4.991%
16	13.992	1864	1871	1886	rBV2	3919772	5930488	67.40%	6.187%
17	14.298	1916	1923	1934	rBV	3250722	4918970	55.90%	5.132%
18	14.416	1939	1943	1950	rVB5	5957	10130	0.12%	0.011%
19	14.516	1953	1960	1980	rBV	1500091	2526121	28.71%	2.636%
20	14.716	1990	1994	2002	rVB9	6611	15026	0.17%	0.016%
21	15.251	2077	2085	2086	rBV7	5174	9857	0.11%	0.010%
22	15.298	2086	2093	2105	rVB	5052449	7161863	81.40%	7.472%
23	15.428	2108	2115	2124	rBV	1439871	2005043	22.79%	2.092%
24	15.534	2129	2133	2143	rVB	26553	48078	0.55%	0.050%
25	16.522	2297	2301	2306	rVB5	6955	10839	0.12%	0.011%
26	16.728	2329	2336	2341	rBV7	7389	15692	0.18%	0.016%
27	16.834	2350	2354	2362	rVB	11171	17774	0.20%	0.019%
28	17.051	2384	2391	2400	rBV	4124273	5860213	66.60%	6.114%
29	17.151	2401	2408	2422	rVV	5356930	7774242	88.36%	8.111%
30	17.339	2436	2440	2445	rBV6	6771	12226	0.14%	0.013%
31	17.433	2452	2456	2463	rBV4	9562	19758	0.22%	0.021%
32	17.951	2541	2544	2551	rVB8	10849	16100	0.18%	0.017%
33	18.492	2633	2636	2639	rVB4	8388	11017	0.13%	0.011%
34	19.016	2720	2725	2731	rBV2	70585	107800	1.23%	0.112%
35	19.086	2732	2737	2742	rBV	69161	109871	1.25%	0.115%
36	19.392	2786	2789	2791	rVB3	22174	22863	0.26%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031933.D
Acq On : 12 Jun 2024 09:29
Operator : MA/JU
Sample : PB161332BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK332

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	19.451	2793	2799	2807	rBV	6550864	8798810	100.00%	9.180%
38	21.292	3106	3112	3122	rVB	3940068	5767574	65.55%	6.017%
39	24.015	3567	3575	3586	rVB2	2725269	6644332	75.51%	6.932%
40	24.221	3601	3610	3622	rVB	2031303	5177018	58.84%	5.401%




Sum of corrected areas: 95848705

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031933.D
Acq On : 12 Jun 2024 09:29
Operator : MA/JU
Sample : PB161332BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK332

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

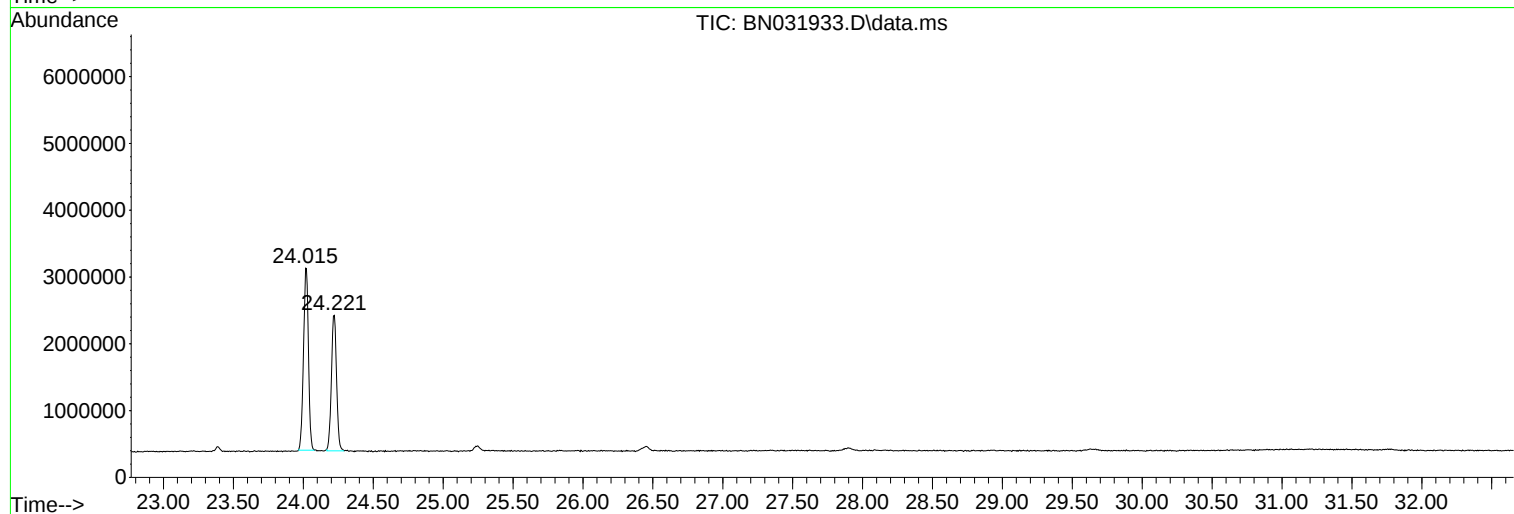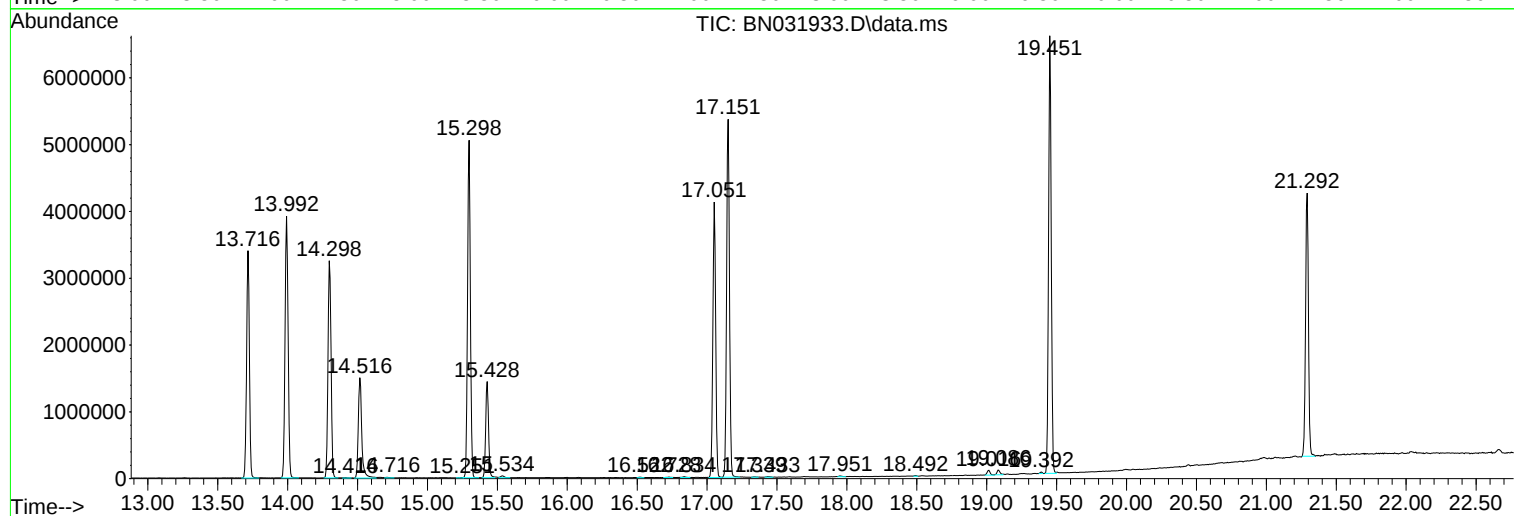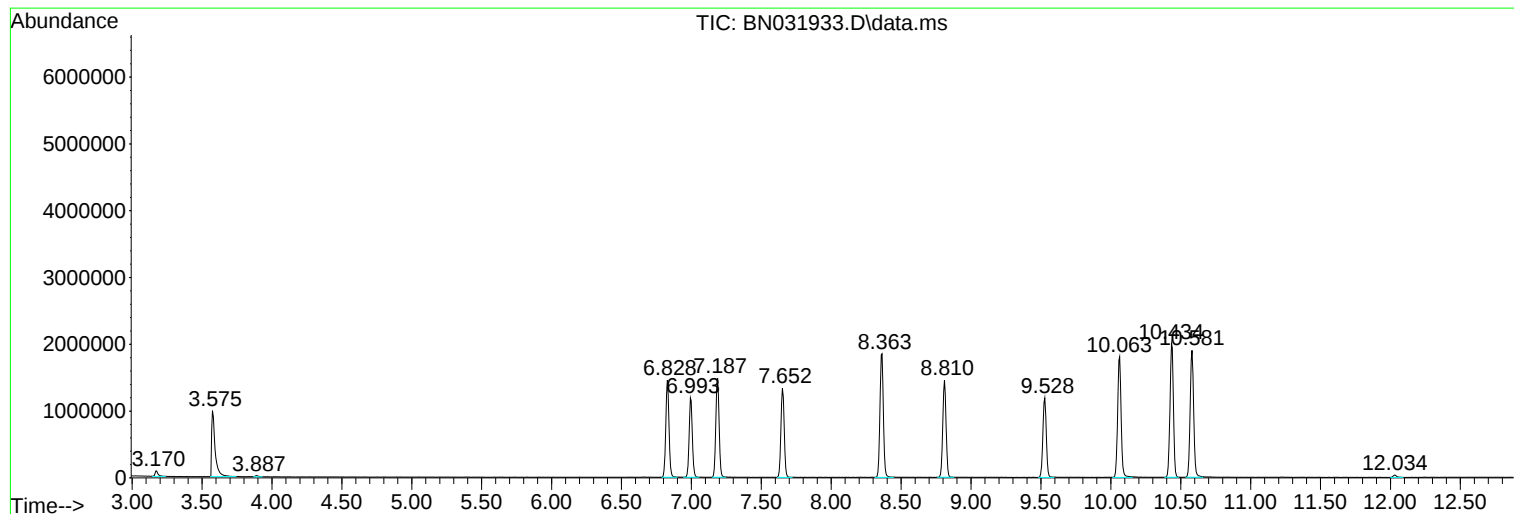

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031933.D
Acq On : 12 Jun 2024 09:29
Operator : MA/JU
Sample : PB161332BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK332

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031933.D
Acq On : 12 Jun 2024 09:29
Operator : MA/JU
Sample : PB161332BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK332

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc