

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031945.D
 Acq On : 12 Jun 2024 17:22
 Operator : MA/JU
 Sample : PB161332BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK332

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031945.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	28	32	43	rVB	87617	120304	1.53%	0.133%
2	3.581	97	101	128	rBV	1069350	1683919	21.44%	1.860%
3	3.899	150	155	162	rVB	18215	29820	0.38%	0.033%
4	6.834	646	654	667	rBV	1464907	2330612	29.68%	2.574%
5	6.999	676	682	694	rVB	1173252	1885532	24.01%	2.082%
6	7.193	706	715	725	rBV	1485764	2387876	30.41%	2.637%
7	7.658	787	794	807	rVB	1336880	2128346	27.10%	2.350%
8	8.363	906	914	927	rBV	1869699	3111102	39.61%	3.436%
9	8.816	982	991	1006	rBV	1480563	2405387	30.63%	2.656%
10	9.528	1105	1112	1126	rBV	1163877	1994425	25.40%	2.202%
11	10.063	1195	1203	1224	rBV	1815476	3207165	40.84%	3.542%
12	10.440	1259	1267	1278	rVB	2068422	3426133	43.63%	3.783%
13	10.587	1284	1292	1304	rBV	1843994	3346479	42.61%	3.696%
14	12.034	1533	1538	1549	rBV	31424	59207	0.75%	0.065%
15	13.722	1818	1825	1838	rBV	3239986	4706985	59.94%	5.198%
16	13.993	1864	1871	1885	rBV2	3833907	5954803	75.82%	6.576%
17	14.304	1916	1924	1933	rBV	3229141	4846274	61.71%	5.352%
18	14.516	1953	1960	1983	rBV	1387716	2354267	29.98%	2.600%
19	14.716	1991	1994	2001	rVB8	4789	8767	0.11%	0.010%
20	15.298	2086	2093	2106	rBV	4771547	7090072	90.28%	7.830%
21	15.428	2109	2115	2127	rVV	1342944	1913303	24.36%	2.113%
22	15.540	2129	2134	2141	rVB	26313	45386	0.58%	0.050%
23	15.869	2185	2190	2196	rBV8	4632	9120	0.12%	0.010%
24	16.087	2221	2227	2229	rBV6	6366	9973	0.13%	0.011%
25	16.728	2333	2336	2341	rVB4	6731	9454	0.12%	0.010%
26	16.834	2351	2354	2360	rVB	9128	12945	0.16%	0.014%
27	17.051	2383	2391	2401	rBV	3950961	5732905	73.00%	6.331%
28	17.151	2401	2408	2423	rVB	5291097	7546735	96.09%	8.334%
29	17.339	2437	2440	2444	rBV4	6537	9842	0.13%	0.011%
30	17.439	2453	2457	2463	rBV2	7427	12306	0.16%	0.014%
31	17.704	2498	2502	2503	rBV3	6979	9797	0.12%	0.011%
32	17.951	2541	2544	2548	rBV5	7541	10016	0.13%	0.011%
33	18.286	2598	2601	2605	rVB4	8399	11697	0.15%	0.013%
34	19.016	2720	2725	2730	rBV2	67234	99980	1.27%	0.110%
35	19.086	2732	2737	2743	rVV	62930	91885	1.17%	0.101%
36	19.451	2793	2799	2806	rBV2	5526252	7853440	100.00%	8.673%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031945.D
Acq On : 12 Jun 2024 17:22
Operator : MA/JU
Sample : PB161332BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK332

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	21.286	3105	3111	3120	rBV2	3013936	4464602	56.85%	4.930%
38	24.016	3567	3575	3587	rVB2	2269146	5401818	68.78%	5.965%
39	24.216	3601	3609	3621	rVB	1649480	4232572	53.89%	4.674%




Sum of corrected areas: 90555251

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031945.D
Acq On : 12 Jun 2024 17:22
Operator : MA/JU
Sample : PB161332BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK332

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

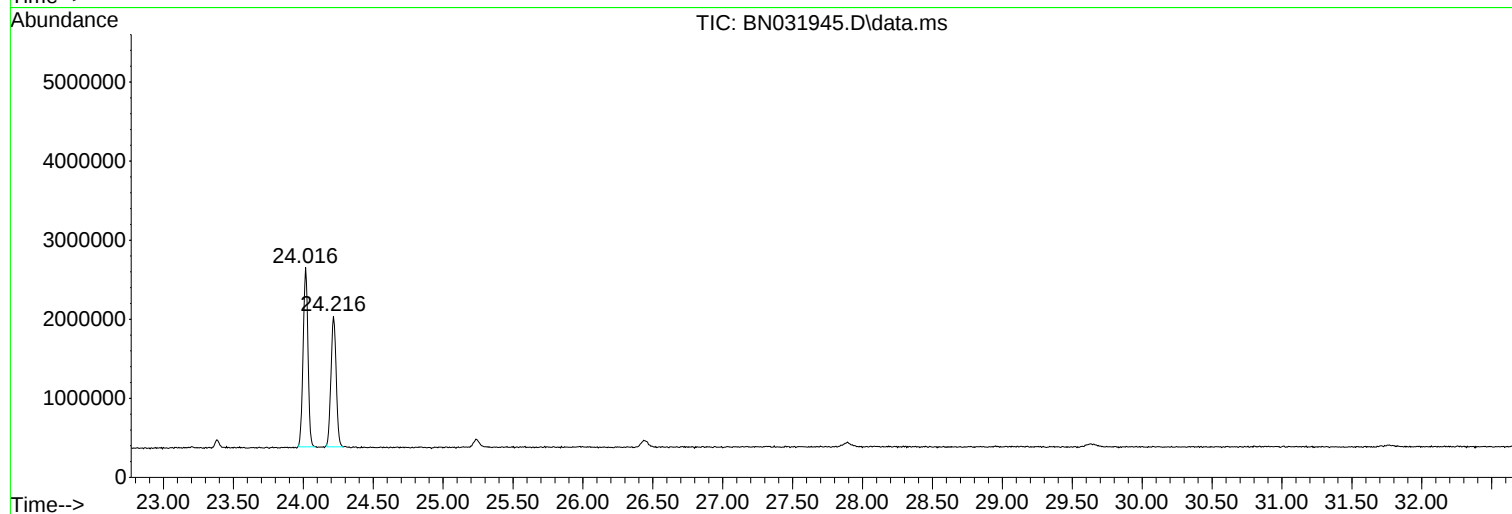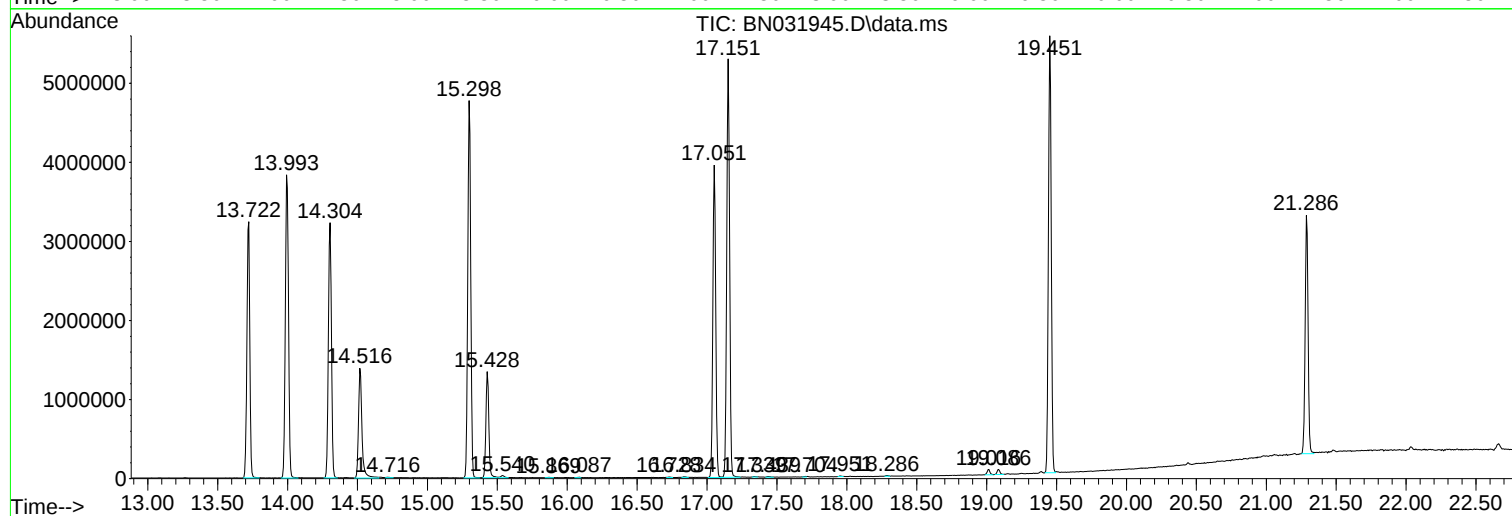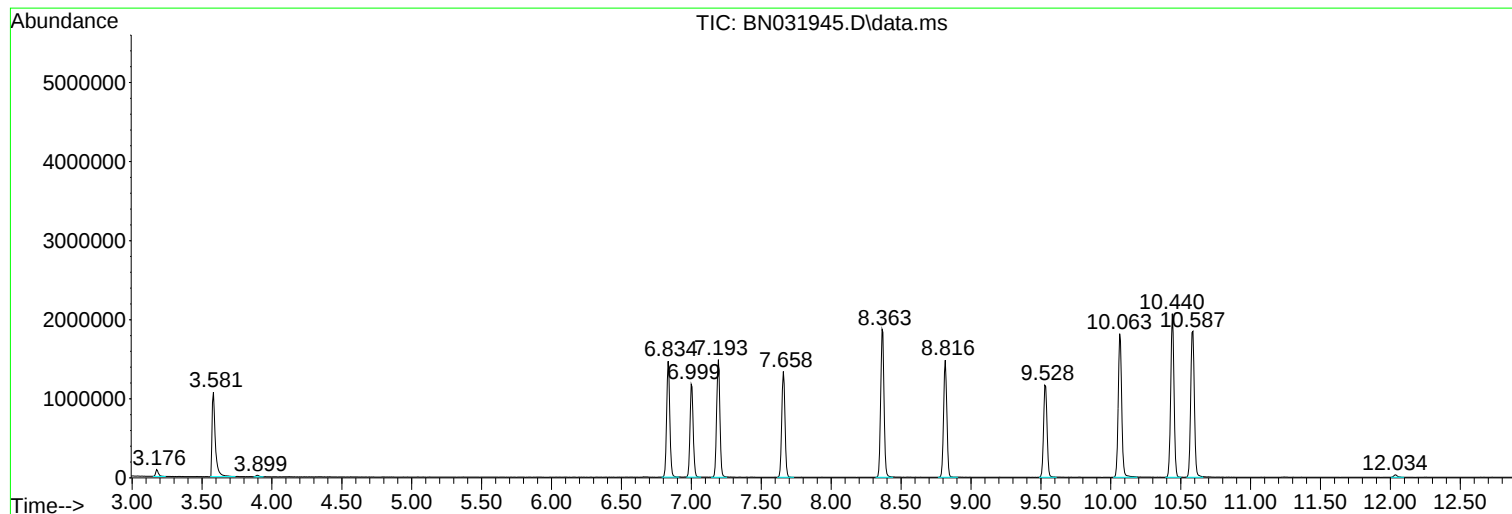

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031945.D
Acq On : 12 Jun 2024 17:22
Operator : MA/JU
Sample : PB161332BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK332

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031945.D
Acq On : 12 Jun 2024 17:22
Operator : MA/JU
Sample : PB161332BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK332

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------