

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031961.D
 Acq On : 13 Jun 2024 04:29
 Operator : MA/JU
 Sample : PB161360BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK360

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	28	33	40	rBV	101634	137953	2.13%	0.164%
2	3.581	97	101	117	rBV	1345860	1962748	30.33%	2.330%
3	3.899	150	155	159	rVB	19933	25524	0.39%	0.030%
4	6.669	621	626	632	rBV9	3694	7948	0.12%	0.009%
5	6.840	647	655	669	rBV	1700562	2742204	42.38%	3.256%
6	7.005	671	683	694	rVB	1395381	2228935	34.45%	2.646%
7	7.193	708	715	728	rBV	1779517	2882757	44.55%	3.423%
8	7.657	786	794	804	rBV	1436672	2335902	36.10%	2.773%
9	8.369	907	915	931	rBV	2127013	3533385	54.60%	4.195%
10	8.816	983	991	1002	rBV	1626701	2711789	41.91%	3.220%
11	9.534	1105	1113	1125	rBV	1388536	2277616	35.20%	2.704%
12	10.069	1196	1204	1224	rBV	2029144	3524910	54.47%	4.185%
13	10.440	1259	1267	1278	rBV	1976610	3404668	52.62%	4.042%
14	10.587	1284	1292	1312	rBV	2047577	3551739	54.89%	4.217%
15	12.040	1533	1539	1547	rBV	32434	64819	1.00%	0.077%
16	13.269	1744	1748	1753	rBV4	5772	10405	0.16%	0.012%
17	13.722	1818	1825	1838	rBV	3310402	4706000	72.73%	5.587%
18	13.998	1864	1872	1886	rBV	3747082	5741806	88.73%	6.817%
19	14.304	1917	1924	1933	rBV	2873083	4162982	64.33%	4.943%
20	14.528	1955	1962	1979	rBV	1093746	1905494	29.45%	2.262%
21	14.669	1983	1986	1990	rVV6	7750	13417	0.21%	0.016%
22	14.710	1990	1993	2001	rVB9	6559	15462	0.24%	0.018%
23	15.298	2086	2093	2103	rBV	4219201	6470809	100.00%	7.683%
24	15.434	2110	2116	2125	rBV	869314	1241346	19.18%	1.474%
25	15.539	2130	2134	2139	rVB2	23622	40396	0.62%	0.048%
26	15.863	2187	2189	2196	rVB7	4542	7657	0.12%	0.009%
27	16.086	2222	2227	2231	rBV5	6302	11144	0.17%	0.013%
28	16.728	2333	2336	2340	rVB6	6334	9020	0.14%	0.011%
29	16.839	2350	2355	2361	rVB3	7018	12683	0.20%	0.015%
30	17.051	2385	2391	2401	rBV	2591463	3885734	60.05%	4.614%
31	17.151	2401	2408	2421	rVV2	4002228	5955285	92.03%	7.071%
32	17.328	2432	2438	2445	rBV5	34308	82583	1.28%	0.098%
33	17.439	2454	2457	2463	rVB5	6957	10947	0.17%	0.013%
34	18.286	2598	2601	2605	rBV5	9650	15104	0.23%	0.018%
35	19.016	2721	2725	2730	rBV2	47998	72274	1.12%	0.086%
36	19.086	2733	2737	2741	rVV2	46484	61277	0.95%	0.073%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031961.D
Acq On : 13 Jun 2024 04:29
Operator : MA/JU
Sample : PB161360BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK360

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	19.386	2786	2788	2793	rBV5	22136	26525	0.41%	0.031%
38	19.451	2793	2799	2807	rBV	3917158	5603803	86.60%	6.653%
39	21.286	3106	3111	3122	rBV	2120172	3191684	49.32%	3.790%
40	24.021	3567	3576	3588	rVB2	2395250	5776780	89.27%	6.859%
41	24.221	3602	3610	3623	rVB2	1500757	3800486	58.73%	4.512%




Sum of corrected areas: 84224000

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031961.D
Acq On : 13 Jun 2024 04:29
Operator : MA/JU
Sample : PB161360BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK360

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

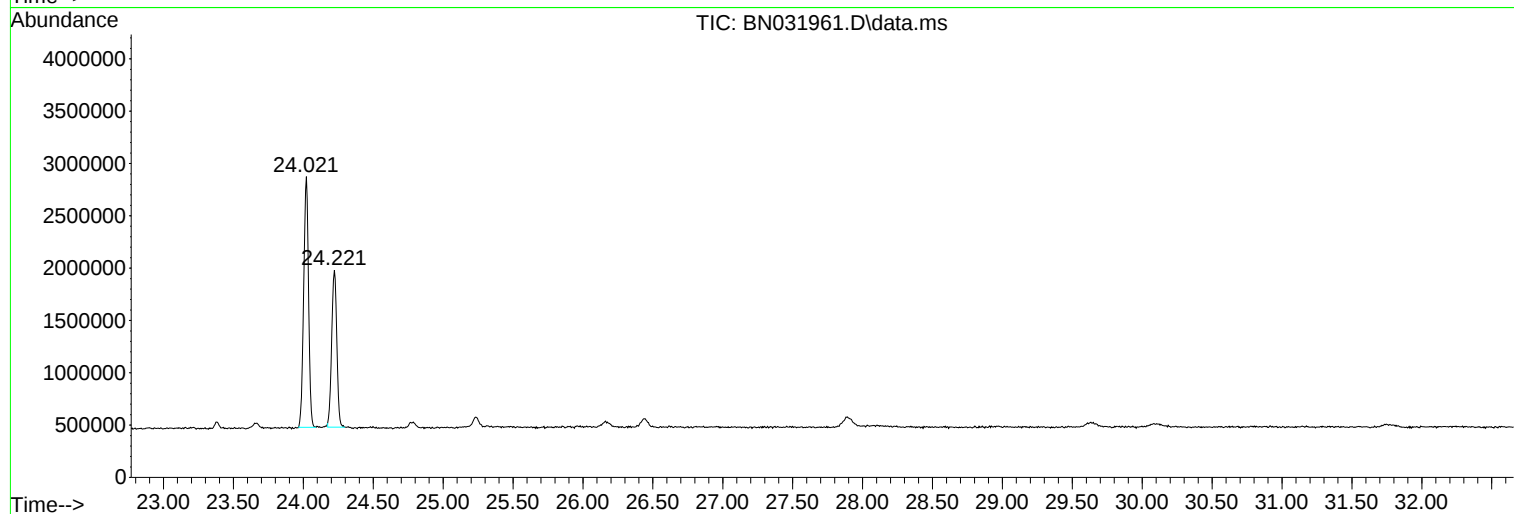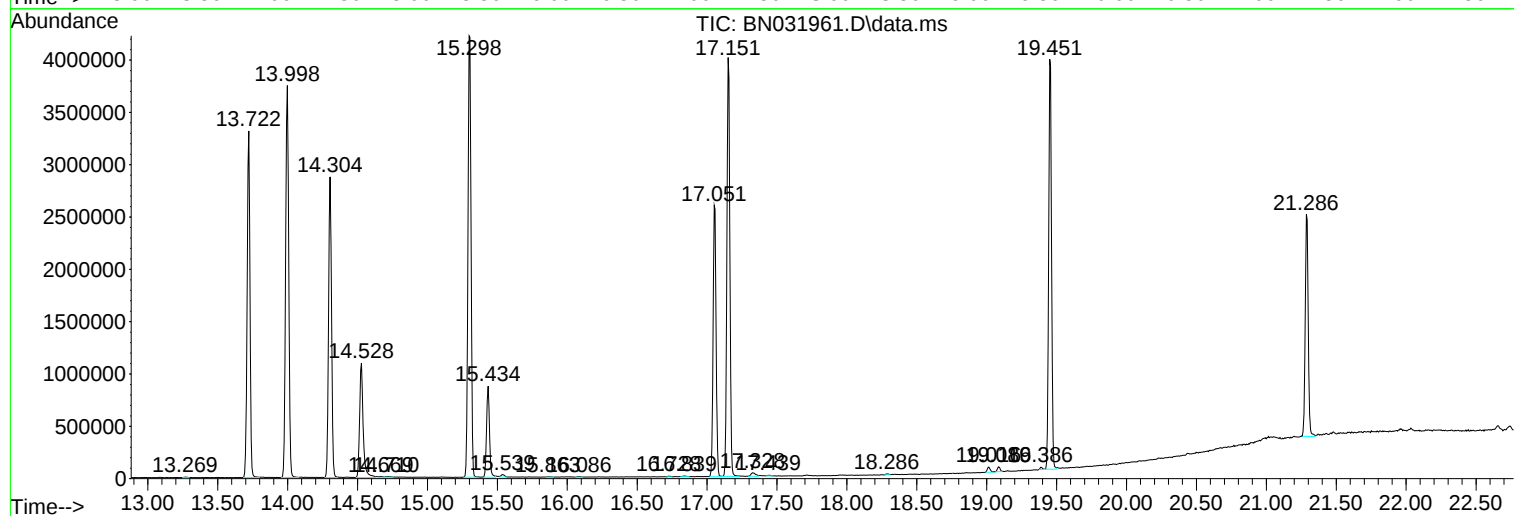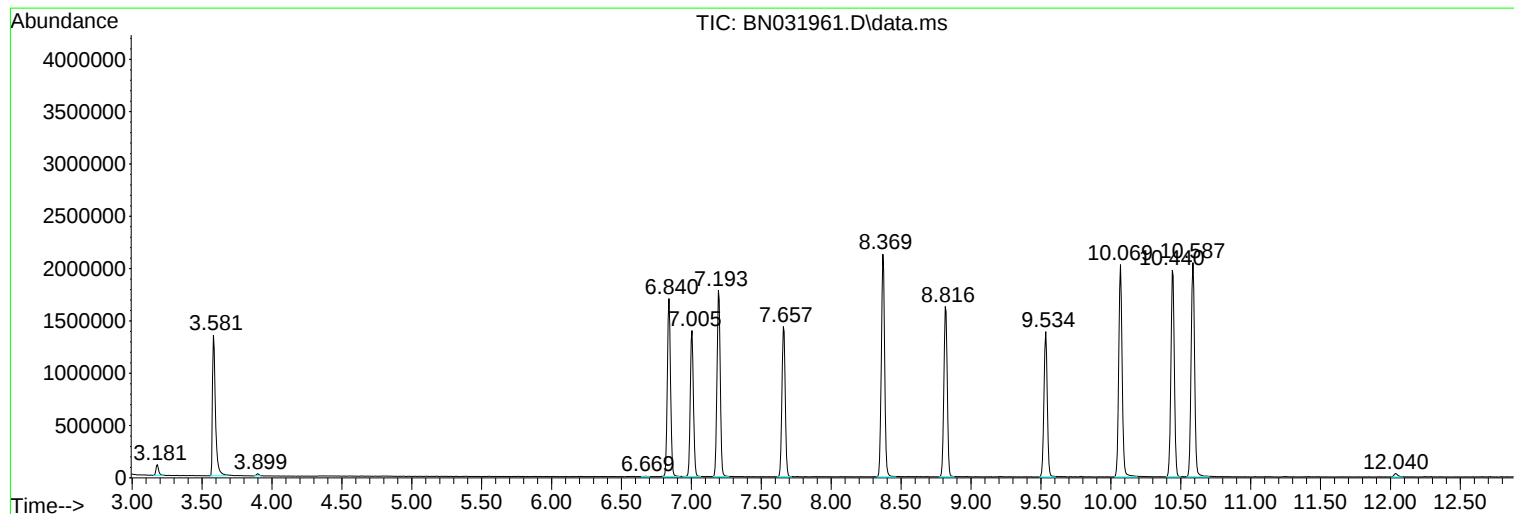

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031961.D
Acq On : 13 Jun 2024 04:29
Operator : MA/JU
Sample : PB161360BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK360

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031961.D
Acq On : 13 Jun 2024 04:29
Operator : MA/JU
Sample : PB161360BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK360

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------