

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
 Data File : BN031977.D
 Acq On : 13 Jun 2024 14:57
 Operator : MA/JU
 Sample : PB161274BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK274

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	40	rVB	90649	127763	2.13%	0.162%
2	3.581	97	101	120	rBV	1222047	1855548	30.94%	2.359%
3	3.893	150	154	159	rBV	16763	23702	0.40%	0.030%
4	6.834	648	654	666	rBV	1547851	2536876	42.30%	3.225%
5	7.005	676	683	695	rVB	1266506	2045561	34.11%	2.600%
6	7.193	707	715	726	rBV	1647847	2640022	44.02%	3.356%
7	7.658	787	794	802	rBV	1403958	2257877	37.65%	2.870%
8	8.369	904	915	931	rBV	1948484	3270295	54.53%	4.157%
9	8.816	983	991	1007	rBV	1560751	2535083	42.27%	3.223%
10	9.528	1103	1112	1126	rBV	1214278	2096644	34.96%	2.665%
11	10.063	1195	1203	1225	rBV	1823171	3273052	54.57%	4.161%
12	10.440	1257	1267	1277	rBV	2012893	3384259	56.43%	4.302%
13	10.587	1284	1292	1307	rBV	1874562	3331343	55.55%	4.235%
14	12.034	1532	1538	1554	rVB	27759	61920	1.03%	0.079%
15	12.251	1570	1575	1580	rVB6	3114	6397	0.11%	0.008%
16	13.269	1744	1748	1753	rBV5	4566	7293	0.12%	0.009%
17	13.722	1817	1825	1835	rBV	2858826	4176493	69.64%	5.309%
18	13.998	1864	1872	1890	rBV	3471320	5315223	88.62%	6.757%
19	14.304	1916	1924	1939	rVB	2746579	4150042	69.20%	5.276%
20	14.522	1955	1961	1982	rBV	951363	1702053	28.38%	2.164%
21	15.298	2086	2093	2104	rBV	4042121	5997442	100.00%	7.624%
22	15.434	2109	2116	2127	rVV	746850	1117776	18.64%	1.421%
23	15.539	2129	2134	2140	rVB	22721	38130	0.64%	0.048%
24	16.086	2223	2227	2234	rVB7	4737	7154	0.12%	0.009%
25	16.728	2333	2336	2341	rVB6	5477	7523	0.13%	0.010%
26	16.845	2351	2356	2364	rVB2	6878	13397	0.22%	0.017%
27	17.051	2384	2391	2401	rBV	2740130	3977460	66.32%	5.056%
28	17.151	2401	2408	2418	rBV	3798963	5424179	90.44%	6.896%
29	17.333	2434	2439	2448	rBV5	18124	48125	0.80%	0.061%
30	17.439	2455	2457	2462	rVB6	6233	7015	0.12%	0.009%
31	19.016	2721	2725	2729	rBV	43185	55220	0.92%	0.070%
32	19.086	2733	2737	2741	rBV	40485	60208	1.00%	0.077%
33	19.386	2786	2788	2793	rVB4	16111	15019	0.25%	0.019%
34	19.451	2793	2799	2807	rBV	3621798	5085597	84.80%	6.465%
35	21.292	3106	3112	3123	rBV	2246130	3263531	54.42%	4.149%
36	24.021	3568	3576	3586	rVB	2080819	4975787	82.97%	6.326%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031977.D
Acq On : 13 Jun 2024 14:57
Operator : MA/JU
Sample : PB161274BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK274

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37 24.221 3602 3610 3621 rVB 1478243 3770360 62.87% 4.793%




Sum of corrected areas: 78661369

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031977.D
Acq On : 13 Jun 2024 14:57
Operator : MA/JU
Sample : PB161274BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK274

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

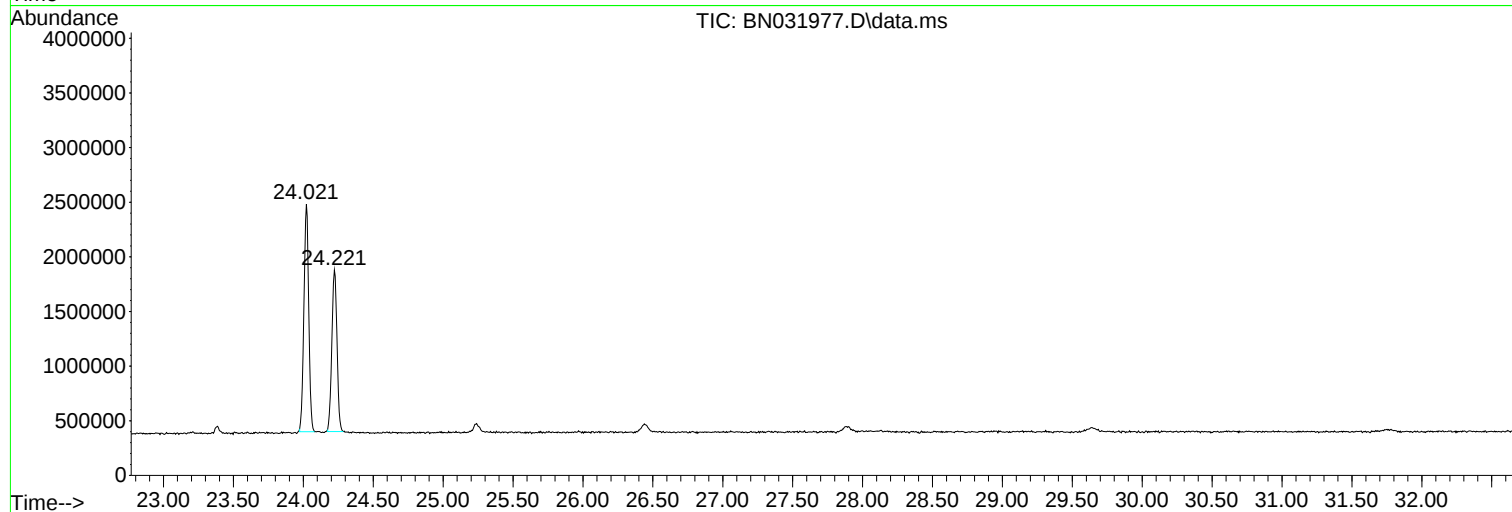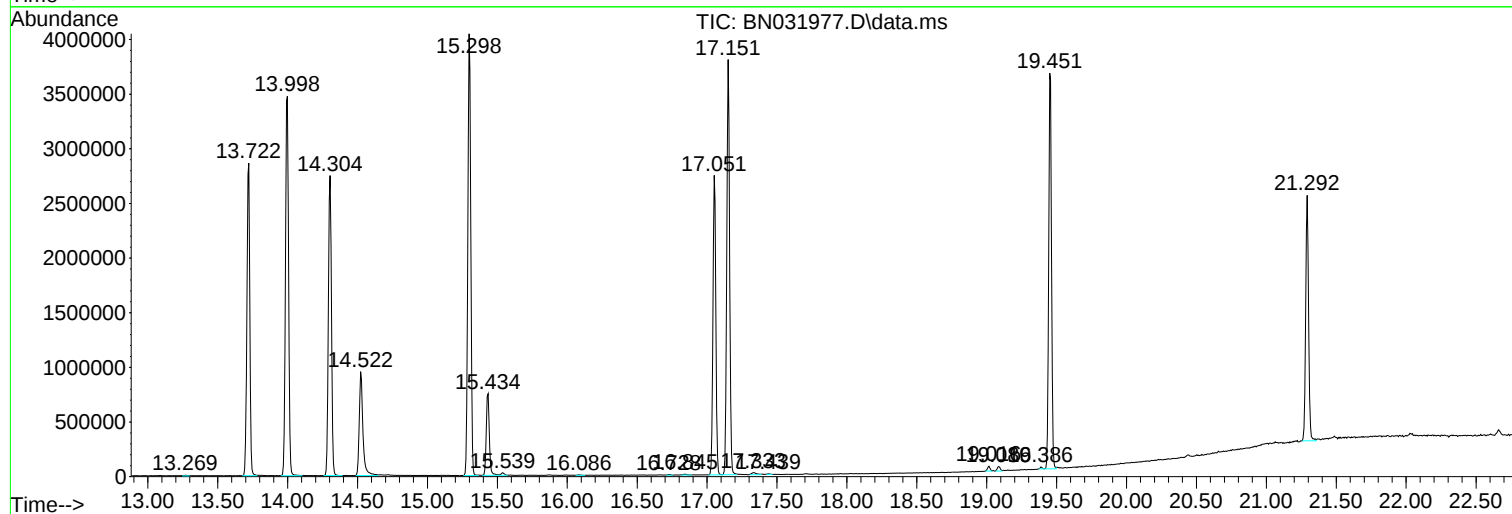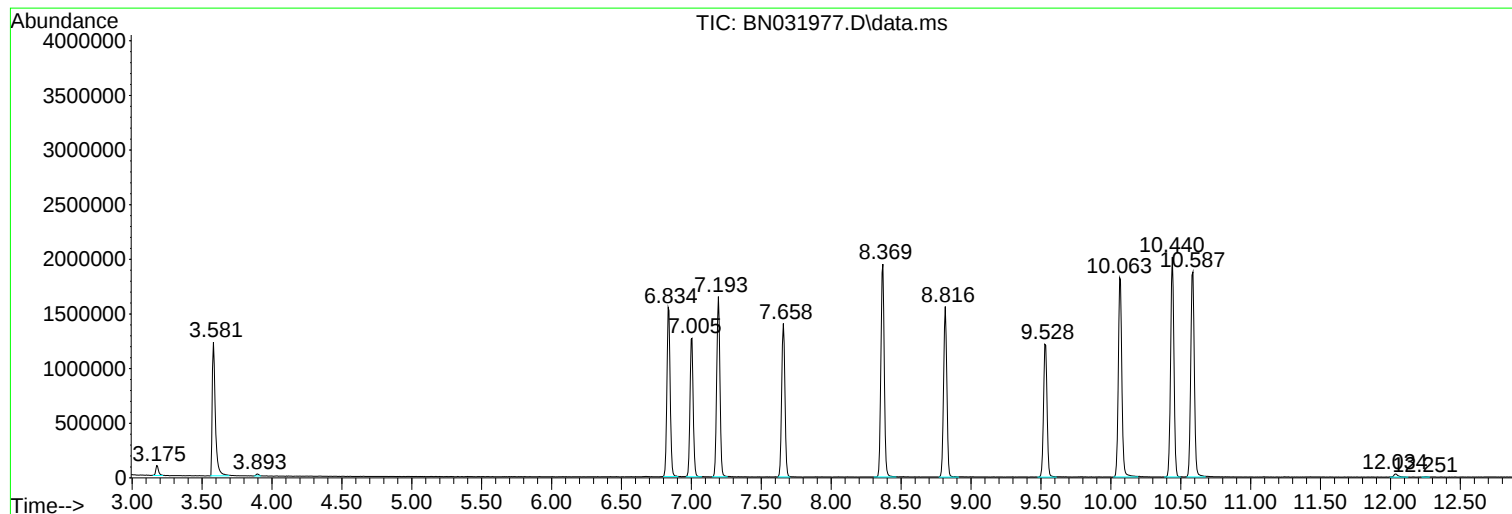

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031977.D
Acq On : 13 Jun 2024 14:57
Operator : MA/JU
Sample : PB161274BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK274

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061224\
Data File : BN031977.D
Acq On : 13 Jun 2024 14:57
Operator : MA/JU
Sample : PB161274BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK274

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc