

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061322\
 Data File : BN020147.D
 Acq On : 13 Jun 2022 12:20
 Operator : CG/JU
 Sample : N3250-16
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYT2

Quant Time: Jun 14 01:04:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	146071	20.000	ng/u1	0.00
20) Naphthalene-d8	10.605	136	688072	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.446	164	447461	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.181	188	938782	20.000	ng/u1	-0.01
79) Chrysene-d12	21.375	240	812899	20.000	ng/u1	0.00
88) Perylene-d12	23.704	264	688001	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	15073	4.469	ng/uL	0.00
4) Pyridine-d5	3.687	84	91231	9.897	ng/u1	0.00
7) Phenol-d5	6.987	99	68627	5.678	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	234836	31.097	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	227481	23.163	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	148418	14.193	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	159393	30.449	ng/u1	0.00
24) 2-Nitrophenol-d4	9.693	143	164886	29.680	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	263265	27.145	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	389962	24.830	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	1117587	34.326	ng/u1	0.00
49) Acenaphthylene-d8	14.134	160	1226412	32.482	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.640	143	24870	3.812	ng/u1	0.00
60) Fluorene-d10	15.434	176	957201	35.529	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	154936	28.491	ng/u1	-0.01
73) Anthracene-d10	17.281	188	1542807	37.656	ng/u1	-0.01
81) Pyrene-d10	19.581	212	1725803	39.162	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.551	264	1275901	37.903	ng/u1	-0.01


Target Compounds					Qvalue
2) 1,4-Dioxane	3.317	88	22851	6.418 ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061322\
Data File : BN020147.D
Acq On : 13 Jun 2022 12:20
Operator : CG/JU
Sample : N3250-16
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYT2


Quant Time: Jun 14 01:04:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

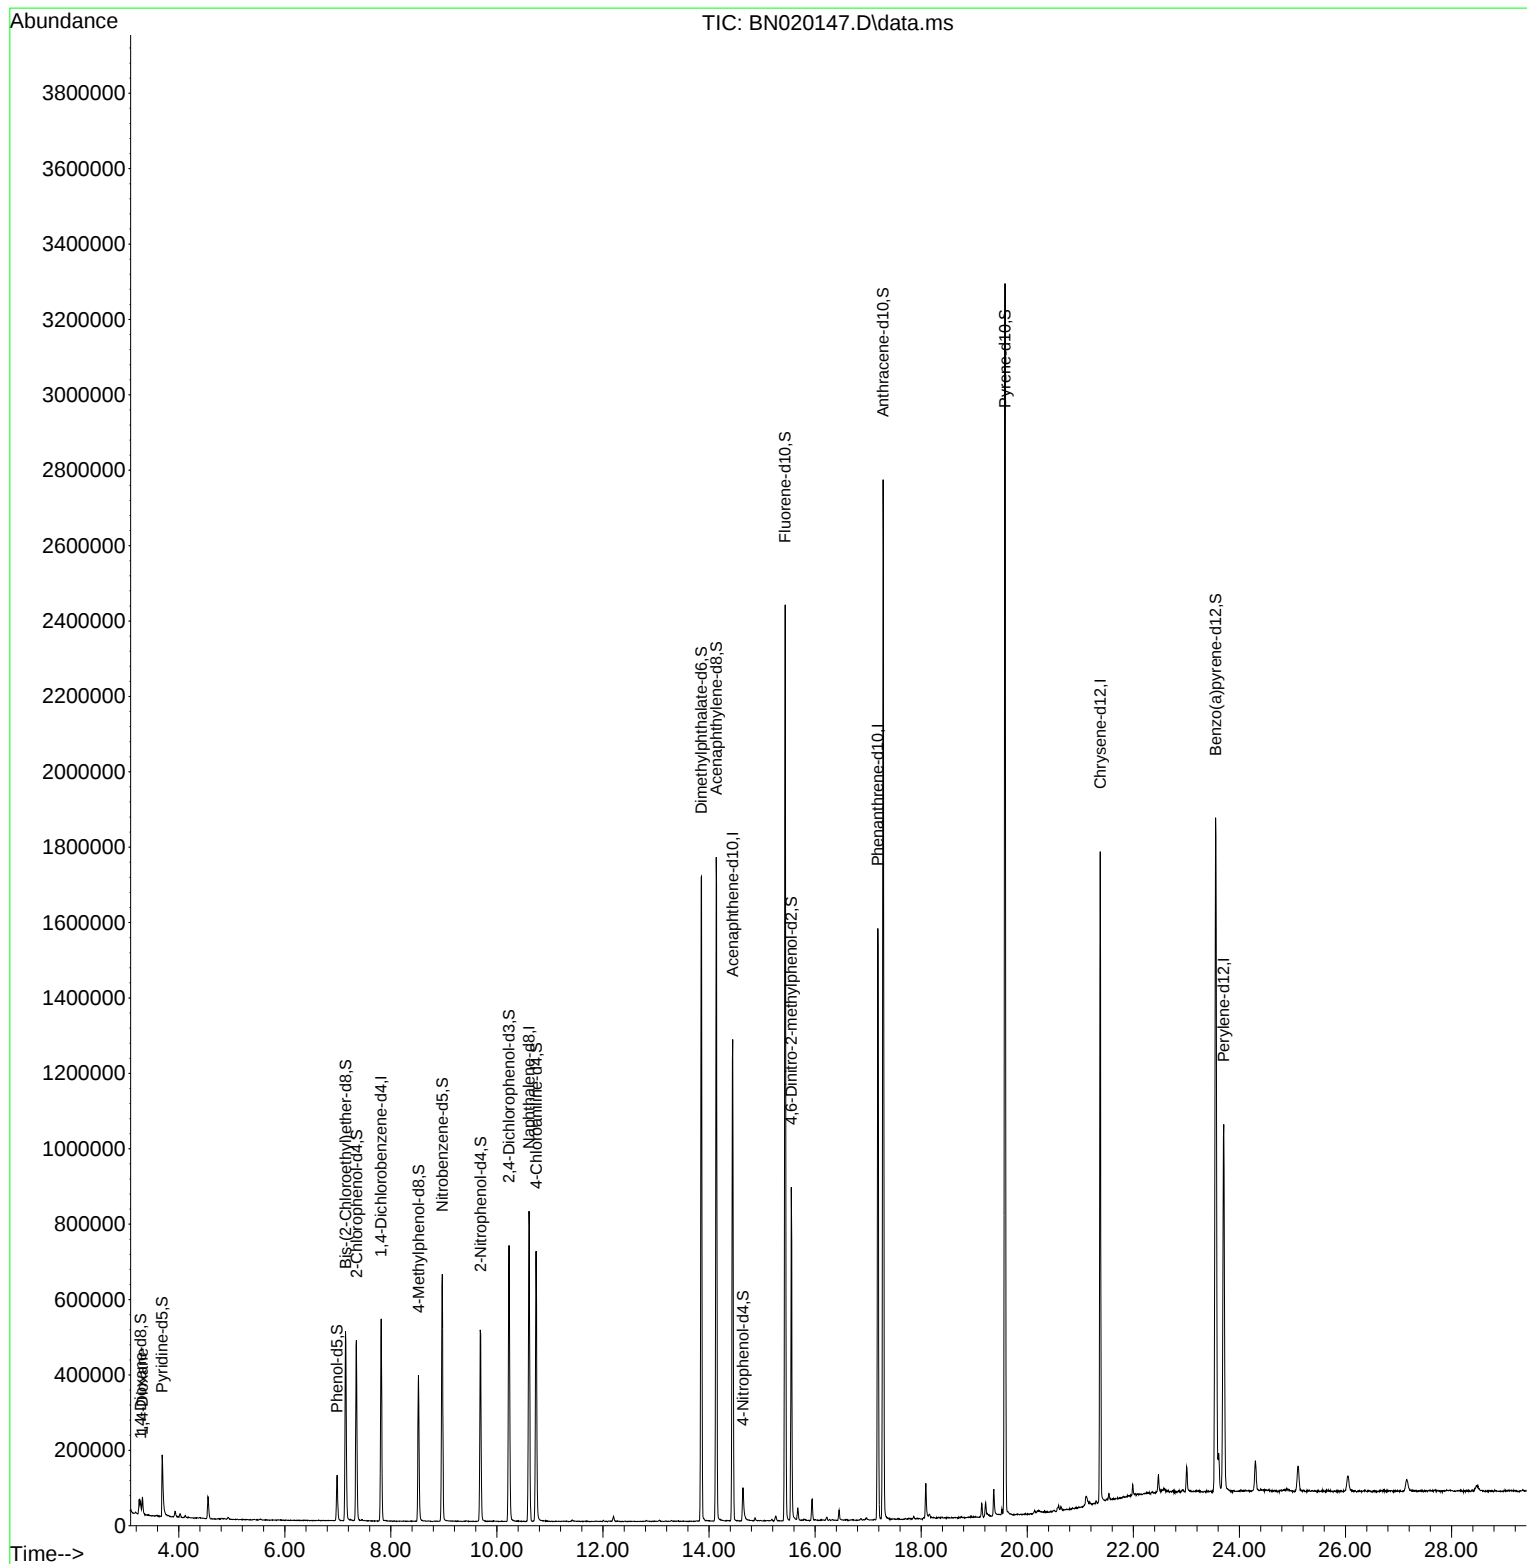

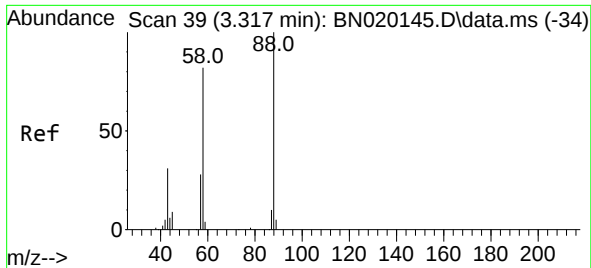

#2
 1,4-Dioxane
 Concen: 6.418 ng/uL
 RT: 3.317 min Scan# 39
 Delta R.T. 0.001 min
 Lab File: BN020147.D
 Acq: 13 Jun 2022 12:20

Instrument :
 BNA_N
 ClientSampleId :
 EXYT2

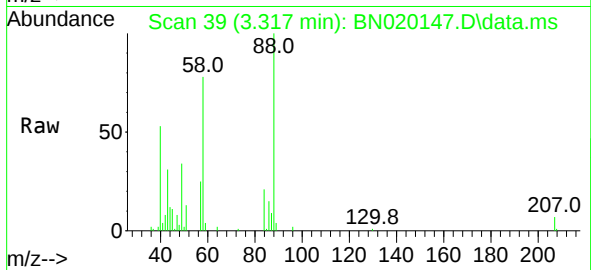

Tgt Ion: 88 Resp: 22851

Ion	Ratio	Lower	Upper
88	100		
43	30.8	22.4	33.6
58	78.0	61.0	91.4

