

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061322\
 Data File : BN020146.D
 Acq On : 13 Jun 2022 11:44
 Operator : CG/JU
 Sample : PB145456BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK456

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020146.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	45	rVB	47558	75929	1.53%	0.146%
2	3.687	99	102	124	rBV	670701	1108767	22.34%	2.130%
3	4.023	156	159	166	rVB3	10176	17134	0.35%	0.033%
4	6.987	656	663	674	rBV	774744	1307008	26.33%	2.510%
5	7.152	684	691	702	rVB	614061	1036843	20.89%	1.992%
6	7.352	717	725	736	rBV	792043	1353867	27.28%	2.600%
7	7.817	797	804	815	rVB	619080	1015063	20.45%	1.950%
8	8.522	917	924	941	rBV	1040780	1732718	34.91%	3.328%
9	8.969	992	1000	1012	rBV	806157	1373041	27.67%	2.637%
10	9.687	1113	1122	1134	rBV	680991	1161413	23.40%	2.231%
11	10.228	1206	1214	1226	rBV	986279	1712506	34.51%	3.289%
12	10.605	1267	1278	1288	rBV	937368	1619722	32.64%	3.111%
13	10.740	1293	1301	1314	rBV	1069553	1924744	38.78%	3.697%
14	12.199	1543	1549	1555	rBV3	16981	28787	0.58%	0.055%
15	13.851	1822	1830	1842	rBV	1905687	2765983	55.73%	5.313%
16	14.134	1871	1878	1892	rBV	2062495	3192146	64.32%	6.131%
17	14.446	1924	1931	1940	rVB	1451468	2246584	45.27%	4.315%
18	14.634	1956	1963	1985	rBV	806953	1307143	26.34%	2.511%
19	15.434	2092	2099	2108	rBV	2686025	3964370	79.88%	7.615%
20	15.551	2113	2119	2133	rVV	886848	1246372	25.11%	2.394%
21	15.675	2133	2140	2149	rVB2	33396	52926	1.07%	0.102%
22	16.216	2227	2232	2238	rBV2	10192	14579	0.29%	0.028%
23	16.869	2337	2343	2347	rBV5	3774	6266	0.13%	0.012%
24	17.181	2390	2396	2406	rBV	1772399	2696674	54.33%	5.180%
25	17.281	2406	2413	2426	rVV	2994784	4456421	89.79%	8.560%
26	19.139	2724	2729	2735	rVB	34144	49018	0.99%	0.094%
27	19.216	2736	2742	2747	rBV	32590	47750	0.96%	0.092%
28	19.516	2790	2793	2797	rBV4	5867	7000	0.14%	0.013%
29	19.581	2797	2804	2815	rBV	3383350	4963052	100.00%	9.533%
30	20.586	2973	2975	2979	rVB2	9781	11378	0.23%	0.022%
31	21.375	3103	3109	3120	rBV	2072692	2671354	53.82%	5.131%
32	21.539	3134	3137	3140	rBV4	9893	11935	0.24%	0.023%
33	21.986	3210	3213	3218	rBV5	17674	23198	0.47%	0.045%
34	22.469	3292	3295	3300	rVB2	30925	45026	0.91%	0.086%
35	23.004	3382	3386	3394	rVB2	52603	84988	1.71%	0.163%
36	23.551	3471	3479	3486	rBV2	2038198	4053044	81.66%	7.785%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061322\
Data File : BN020146.D
Acq On : 13 Jun 2022 11:44
Operator : CG/JU
Sample : PB145456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK456

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	23.704	3497	3505	3518	rVB2	1129816	2337360	47.10%	4.490%
38	24.298	3601	3606	3617	rVB	76315	157050	3.16%	0.302%
39	25.098	3737	3742	3756	rVB3	74177	182974	3.69%	0.351%




Sum of corrected areas: 52062133

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061322\
Data File : BN020146.D
Acq On : 13 Jun 2022 11:44
Operator : CG/JU
Sample : PB145456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

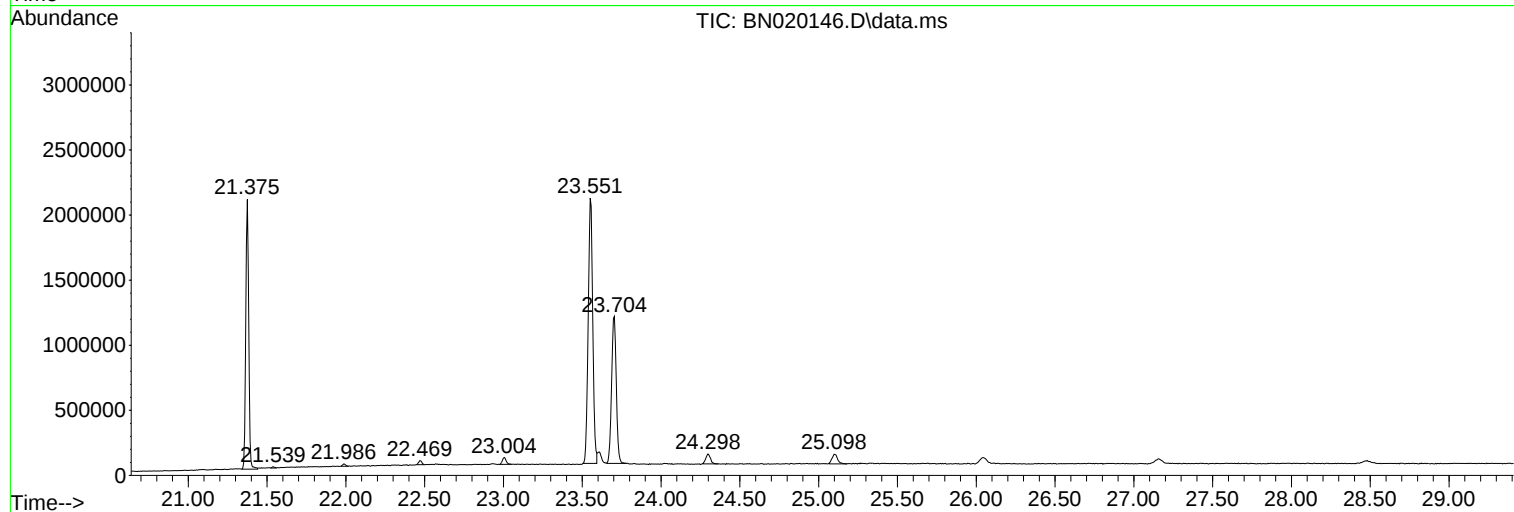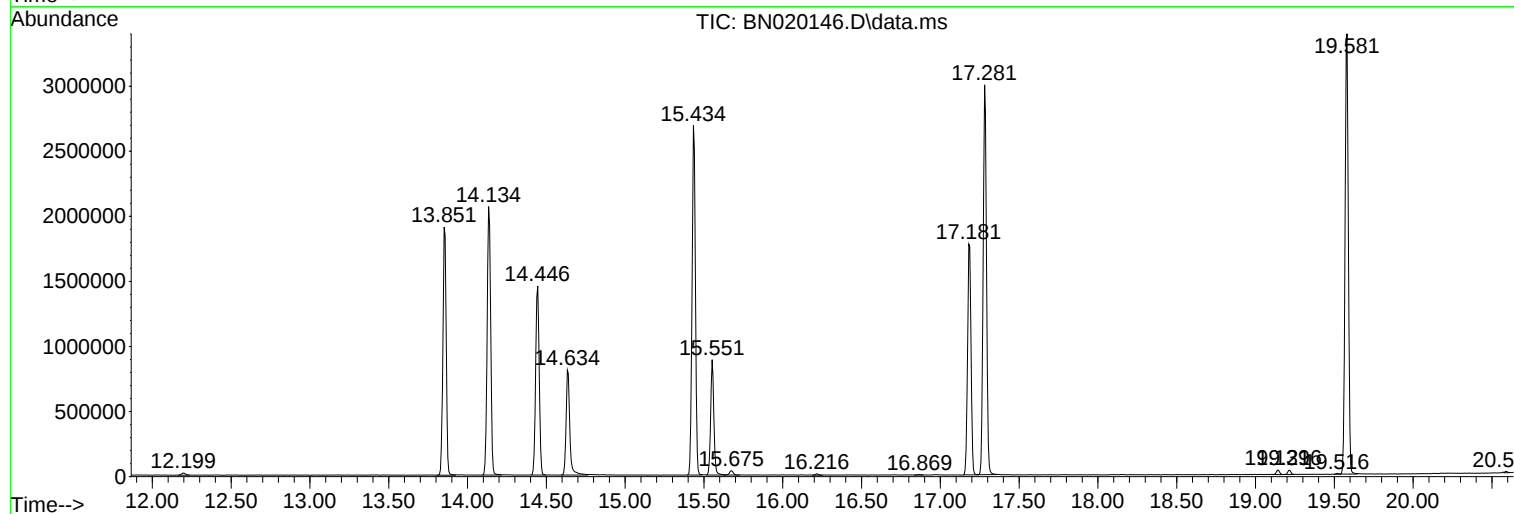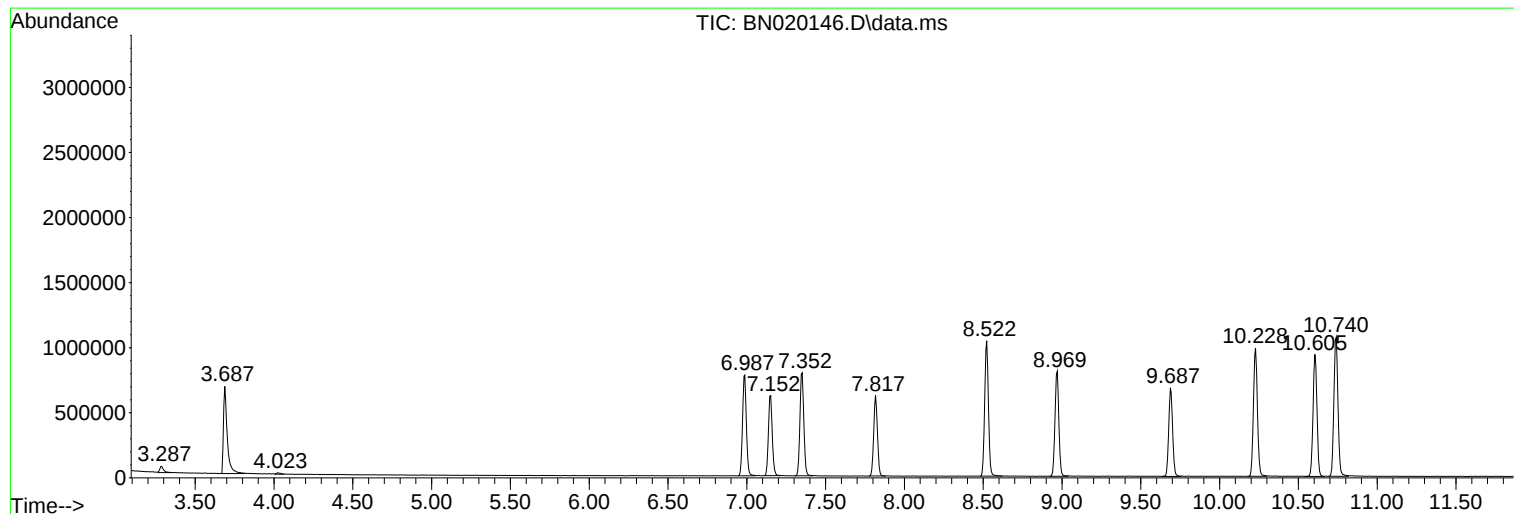

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061322\
Data File : BN020146.D
Acq On : 13 Jun 2022 11:44
Operator : CG/JU
Sample : PB145456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061322\
Data File : BN020146.D
Acq On : 13 Jun 2022 11:44
Operator : CG/JU
Sample : PB145456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------