

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
 Data File : BN037272.D
 Acq On : 14 Jun 2025 21:51
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 16 02:45:34 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 13 18:43:34 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ng	-7.58
7) Naphthalene-d8	0.000	136	0	0.000	ng	-10.36
13) Acenaphthene-d10	0.000	164	0	0.000	ng	-14.22
19) Phenanthrene-d10	0.000	188	0	0.000	ng	-16.97
29) Chrysene-d12	0.000	240	0	0.000	ng	-21.18
35) Perylene-d12	0.000	264	0	0.000	ng	-23.37
System Monitoring Compounds						
4) 2-Fluorophenol	0.000	112	0	0.000	ng	
5) Phenol-d6	0.000	99	0	0.000	ng	
8) Nitrobenzene-d5	0.000	82	0	0.000	ng	
11) 2-Methylnaphthalene-d10	0.000	152	0	0.000	ng	
14) 2,4,6-Tribromophenol	0.000	330	0	0.000	ng	
15) 2-Fluorobiphenyl	0.000	172	0	0.000	ng	
27) Fluoranthene-d10	0.000	212	0	0.000	ng	
31) Terphenyl-d14	0.000	244	0	0.000	ng	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037272.D
Acq On : 14 Jun 2025 21:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 16 02:45:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 13 18:43:34 2025
Response via : Initial Calibration

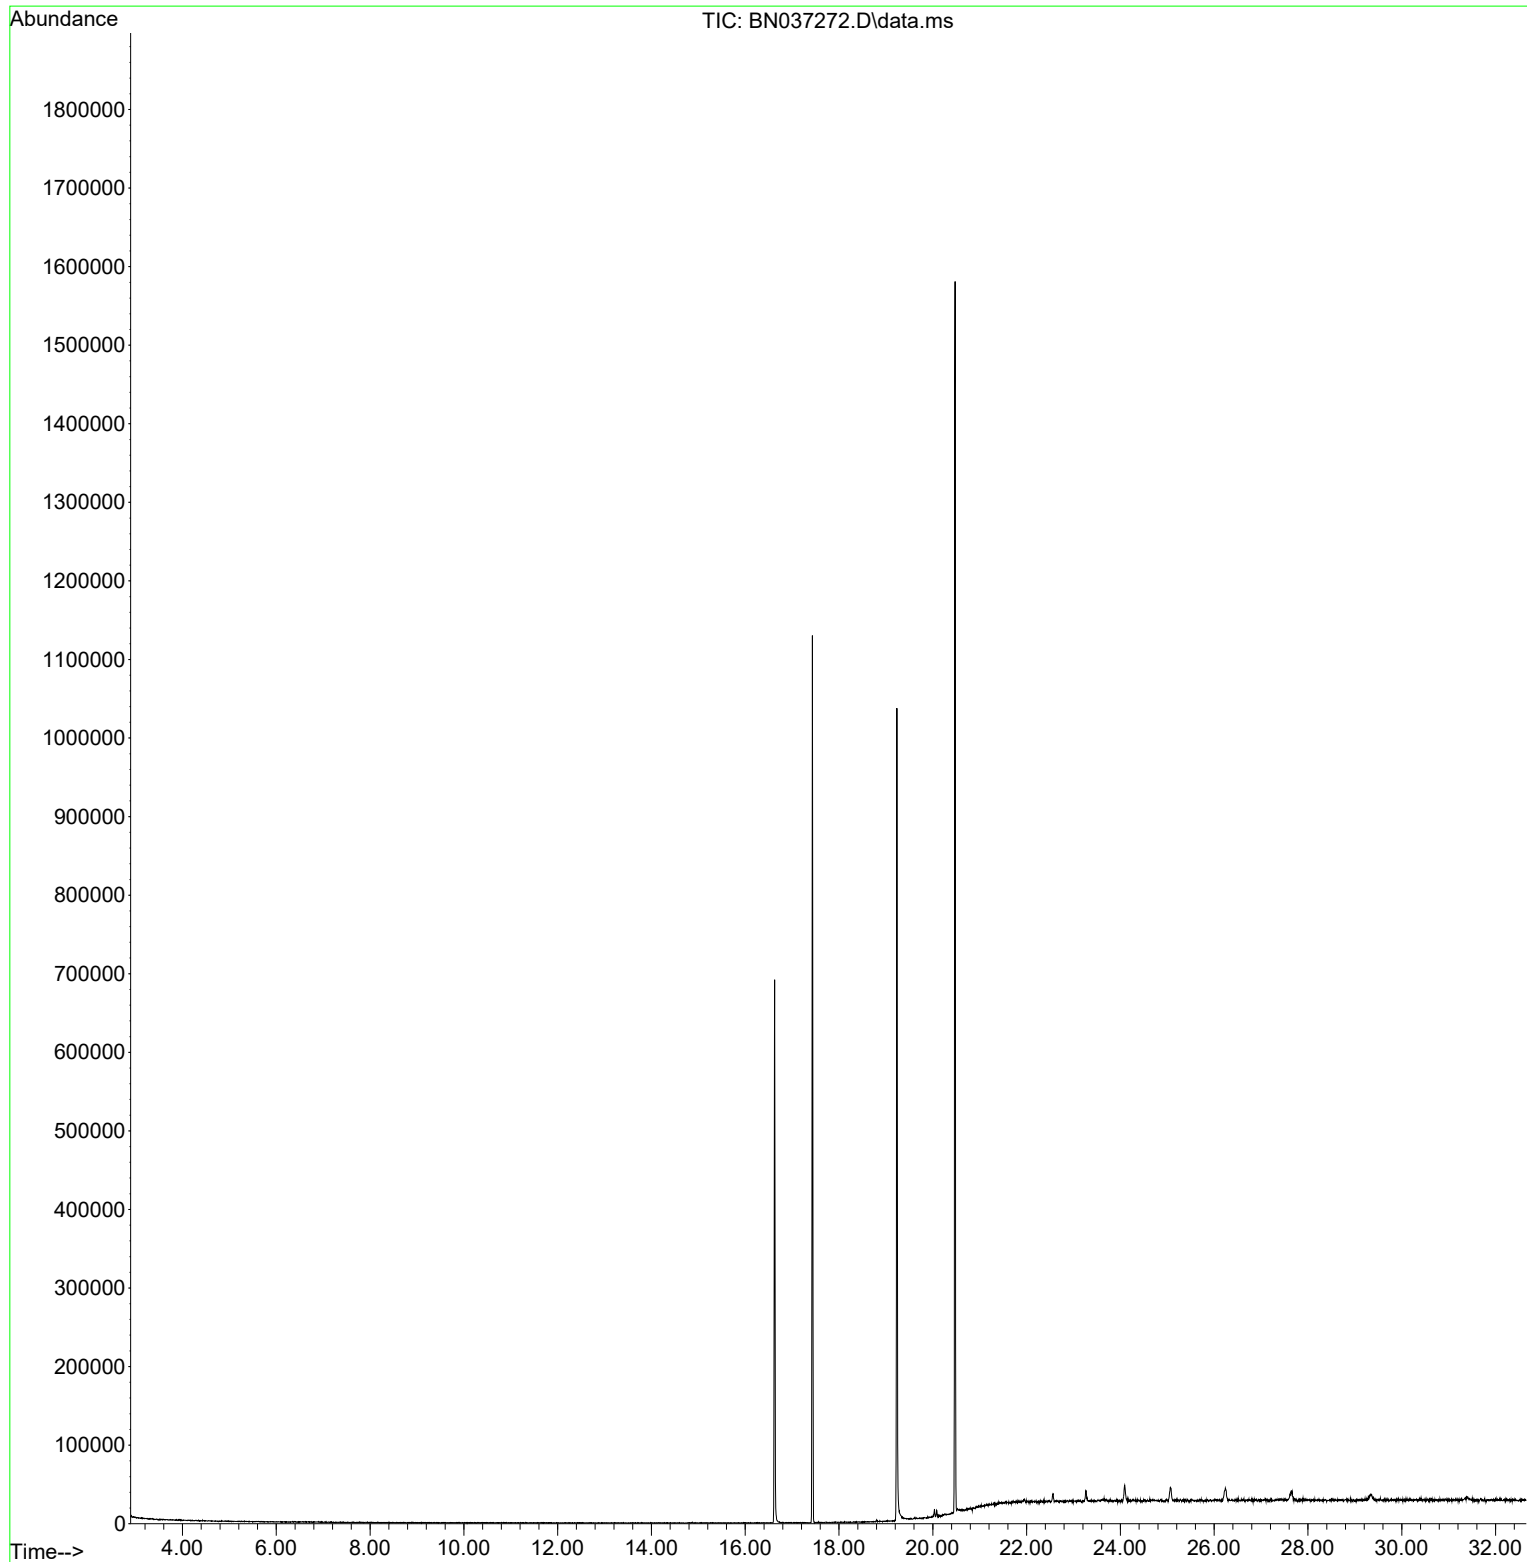


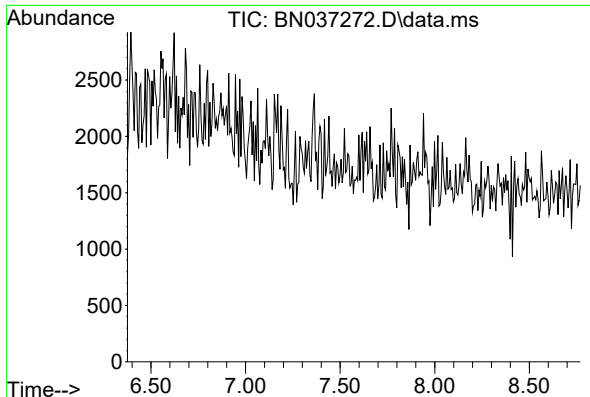


#1
1,4-Dichlorobenzene-d4
Concen: 0.000 ng
Expected RT: 7.58 min

Lab File: BN037272.D
Acq: 14 Jun 2025 21:51

Instrument :
BNA_N
ClientSampleId :
DFTPP


Tgt Ion: 152
Sig Exp Ratio
152 100
150 156.5
115 73.0

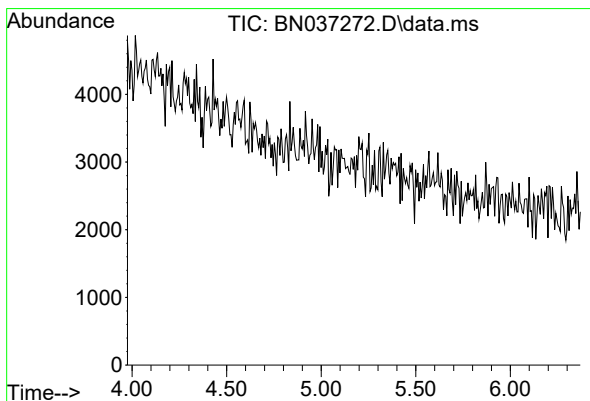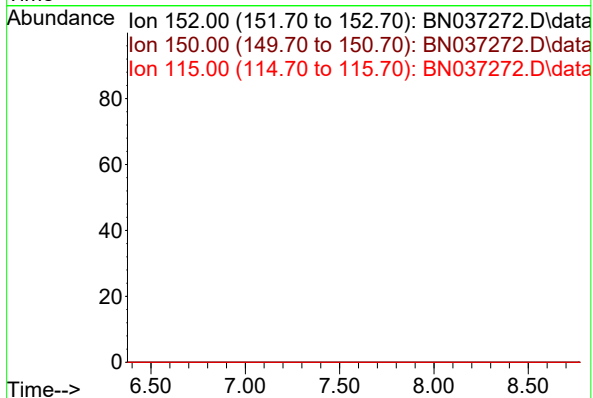


#4
2-Fluorophenol
Concen: 0.000 ng
Expected RT: 5.17 min

Lab File: BN037272.D
Acq: 14 Jun 2025 21:51

Tgt Ion: 112
Sig Exp Ratio
112 100
64 71.5
63 49.7

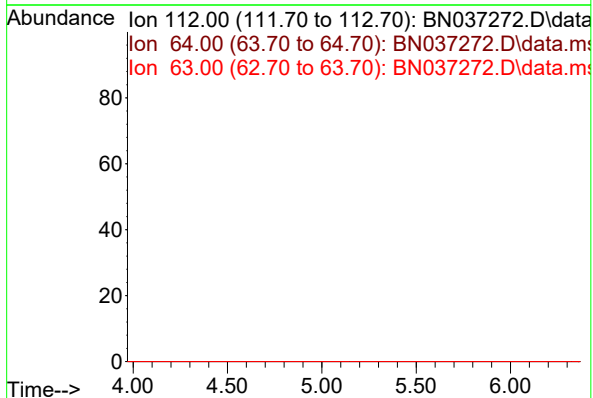


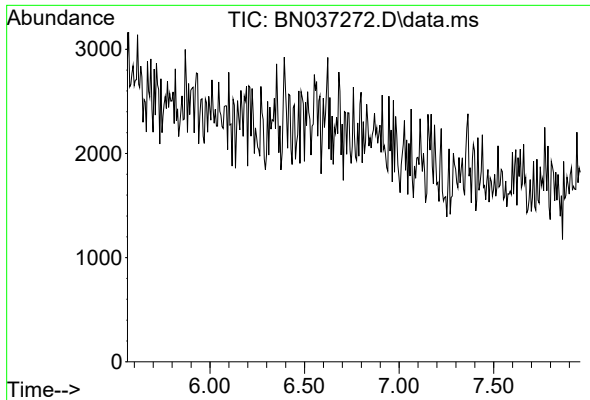


#5
Phenol-d6
Concen: 0.000 ng
Expected RT: 6.76 min

Lab File: BN037272.D
Acq: 14 Jun 2025 21:51

Instrument :
BNA_N
ClientSampleId :
DFTPP


Tgt Ion: 99
Sig Exp Ratio
99 100
42 45.3
71 53.0

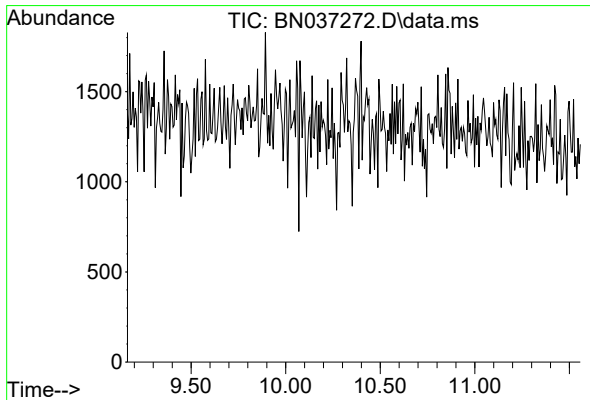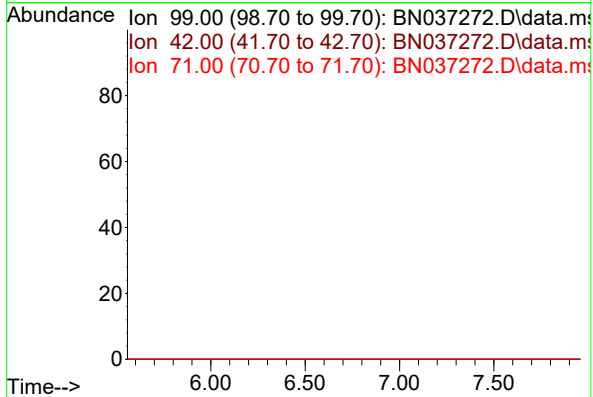


#7
Naphthalene-d8
Concen: 0.000 ng
Expected RT: 10.36 min

Lab File: BN037272.D
Acq: 14 Jun 2025 21:51

Tgt Ion: 136
Sig Exp Ratio
136 100
137 13.2
54 11.5
68 6.7

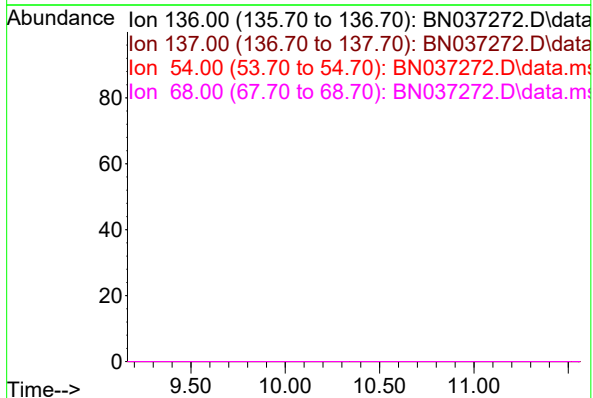


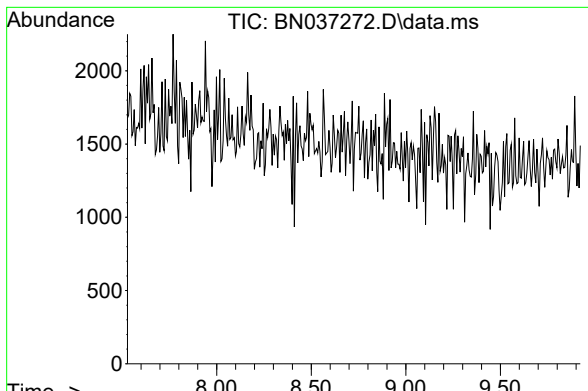


#8
 Nitrobenzene-d5
 Concen: 0.000 ng
 Expected RT: 8.73 min
 Lab File: BN037272.D
 Acq: 14 Jun 2025 21:51

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 82


Sig	Exp Ratio
82	100
128	39.0
54	79.1

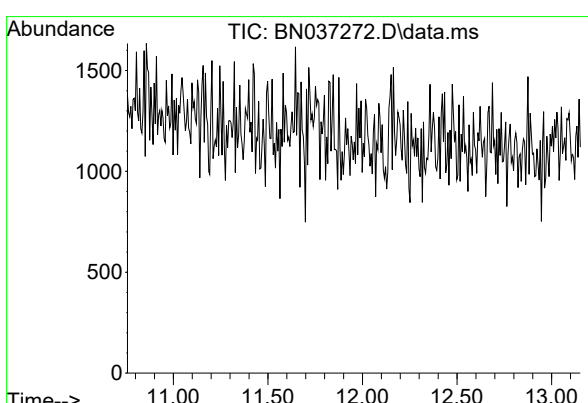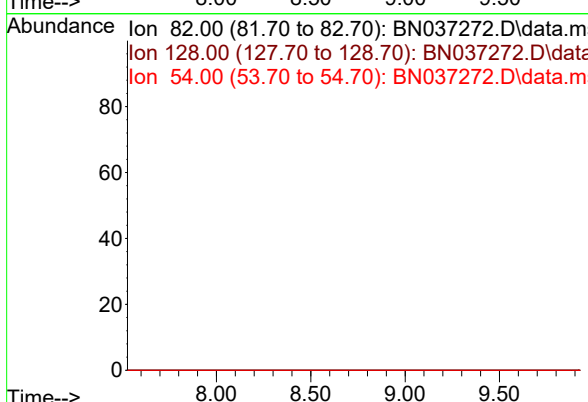


#11
 2-Methylnaphthalene-d10
 Concen: 0.000 ng
 Expected RT: 11.96 min
 Lab File: BN037272.D
 Acq: 14 Jun 2025 21:51

Tgt Ion: 152

Sig	Exp Ratio
152	100
151	22.4


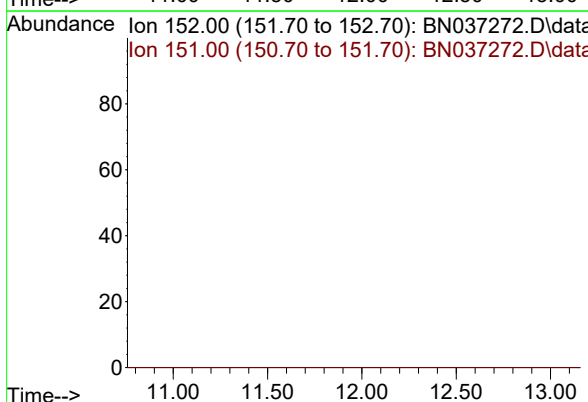


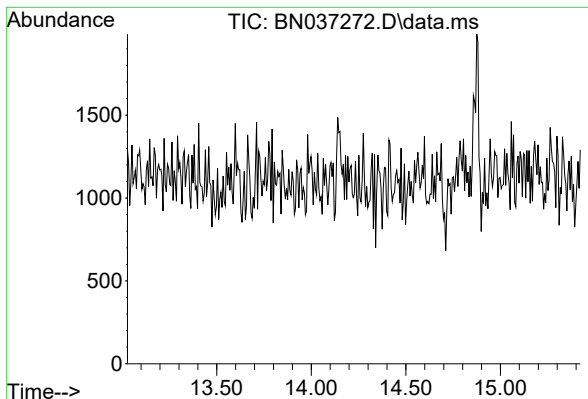

#13
Acenaphthene-d10
Concen: 0.000 ng
Expected RT: 14.22 min
Lab File: BN037272.D
Acq: 14 Jun 2025 21:51


Instrument :
BNA_N
ClientSampleId :
DFTPP


Tgt Ion: 164
Sig Exp Ratio
164 100
162 108.4
160 57.2

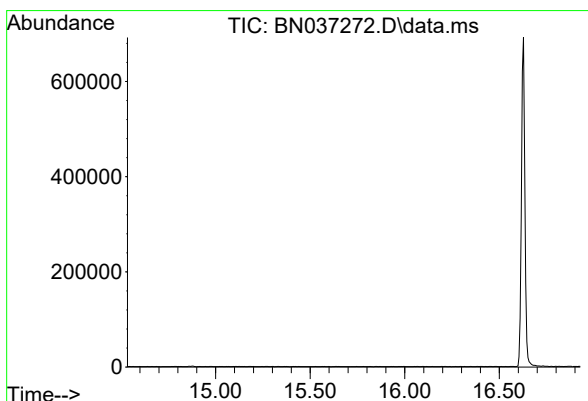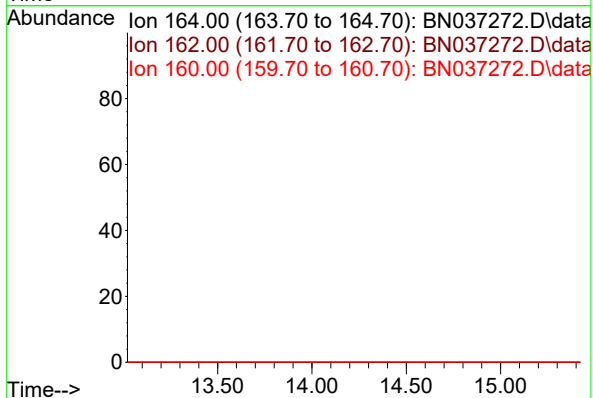

#14
2,4,6-Tribromophenol
Concen: 0.000 ng
Expected RT: 15.73 min
Lab File: BN037272.D
Acq: 14 Jun 2025 21:51

Tgt Ion: 330
Sig Exp Ratio
330 100
332 93.6
141 56.4

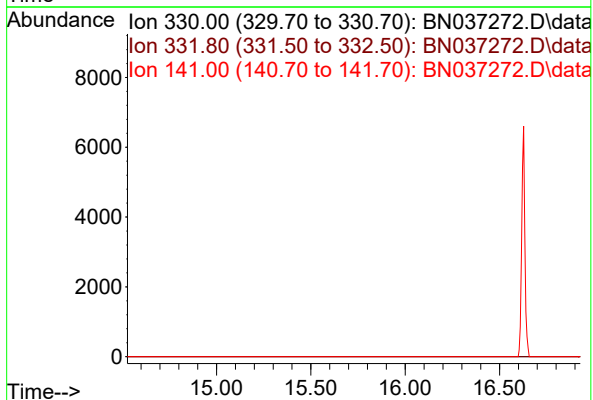


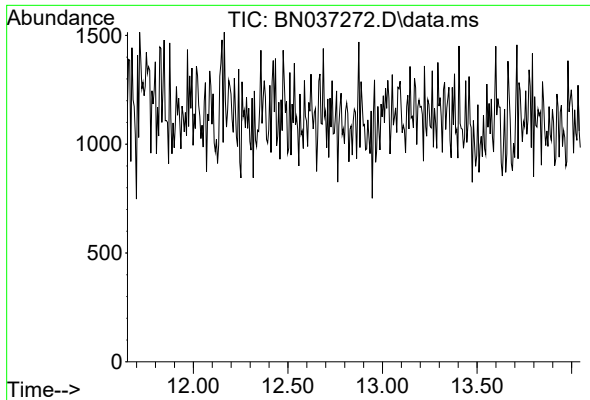


#15
 2-Fluorobiphenyl
 Concen: 0.000 ng
 Expected RT: 12.85 min
 Lab File: BN037272.D
 Acq: 14 Jun 2025 21:51

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 172


Sig	Exp Ratio
172	100
171	37.3
170	26.4

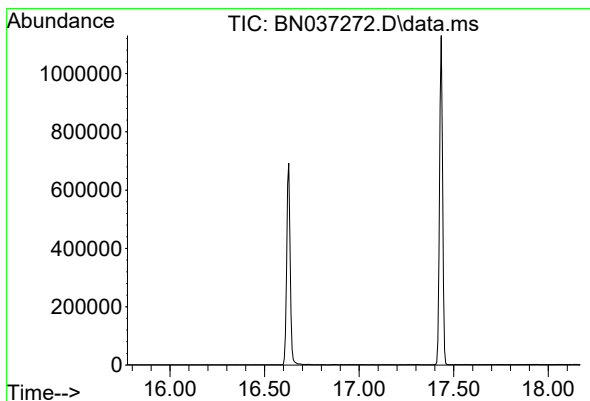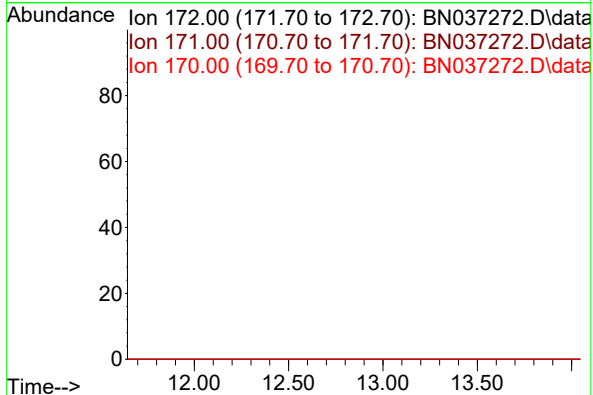


#19
 Phenanthrene-d10
 Concen: 0.000 ng
 Expected RT: 16.97 min
 Lab File: BN037272.D
 Acq: 14 Jun 2025 21:51

Tgt Ion: 188

Sig	Exp Ratio
188	100
94	0.0
80	15.3

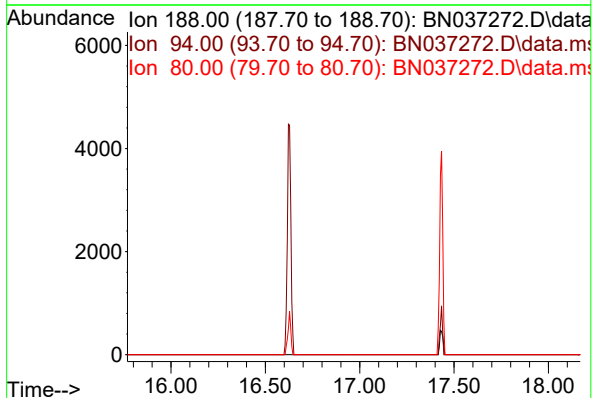


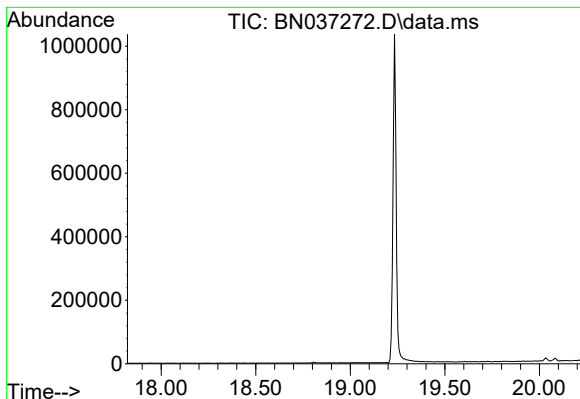


#27
Fluoranthene-d10
Concen: 0.000 ng
Expected RT: 19.02 min

Lab File: BN037272.D
Acq: 14 Jun 2025 21:51

Instrument :
BNA_N
ClientSampleId :
DFTPP


Tgt Ion: 212
Sig Exp Ratio
212 100
106 11.6
104 7.1

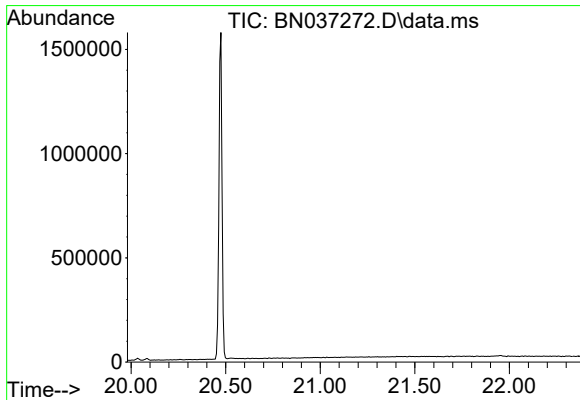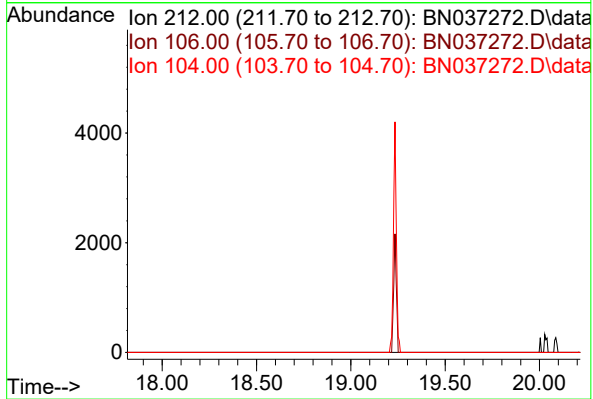


#29
Chrysene-d12
Concen: 0.000 ng
Expected RT: 21.18 min

Lab File: BN037272.D
Acq: 14 Jun 2025 21:51

Tgt Ion: 240
Sig Exp Ratio
240 100
120 14.1
236 30.5

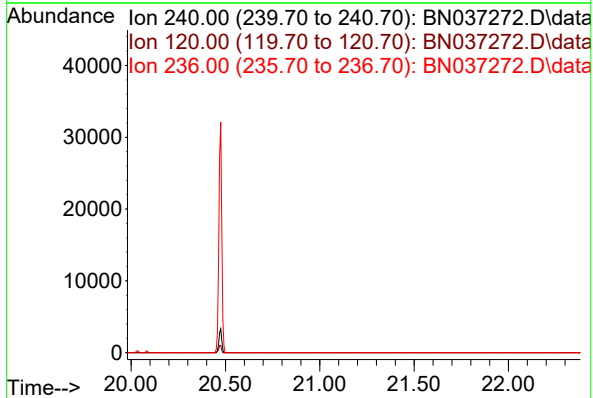


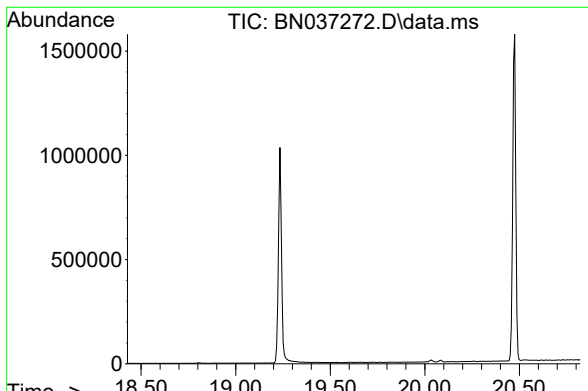


#31
 Terphenyl-d14
 Concen: 0.000 ng
 Expected RT: 19.63 min
 Lab File: BN037272.D
 Acq: 14 Jun 2025 21:51

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 244

Sig	Exp Ratio
244	100
212	15.2
122	17.9

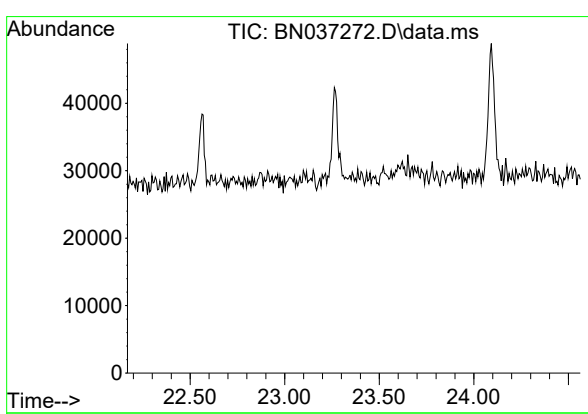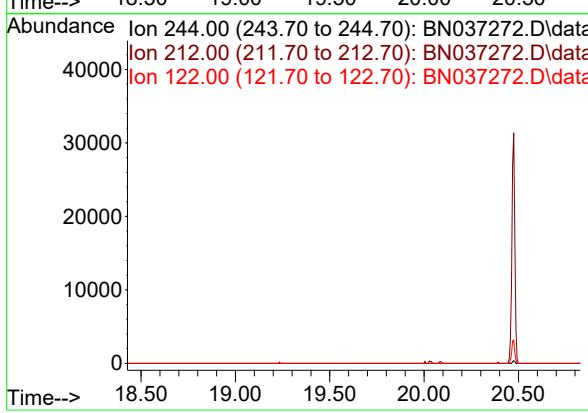

#35
 Perylene-d12
 Concen: 0.000 ng
 Expected RT: 23.37 min
 Lab File: BN037272.D
 Acq: 14 Jun 2025 21:51

Tgt Ion: 264

Sig	Exp Ratio
264	100
260	28.5
265	83.0

