
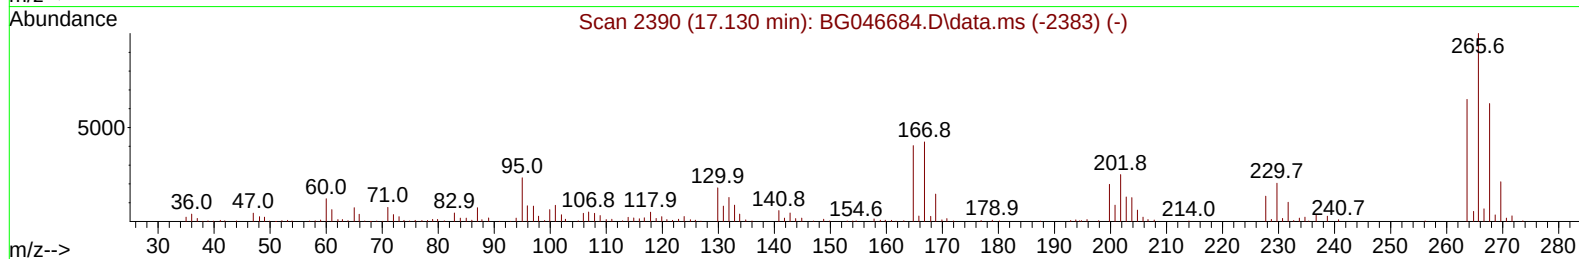
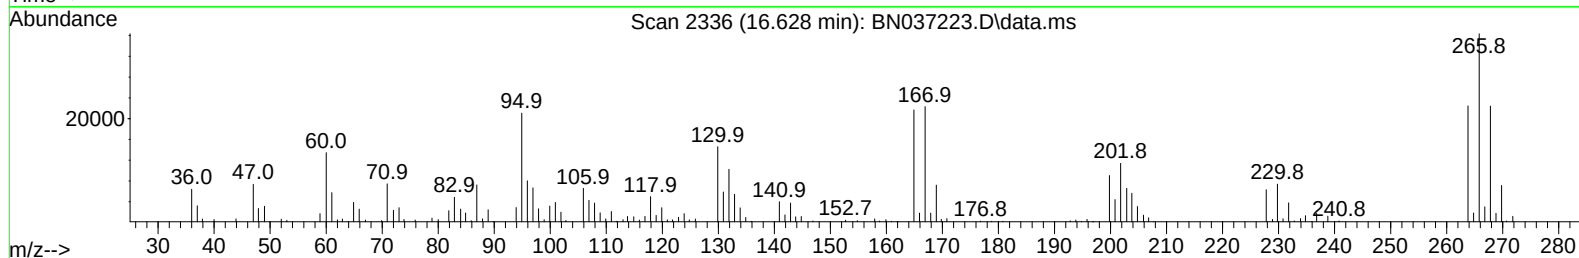


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037223.D
Acq On : 13 Jun 2025 11:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 18:35:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 10 06:01:37 2025
Response via : Initial Calibration

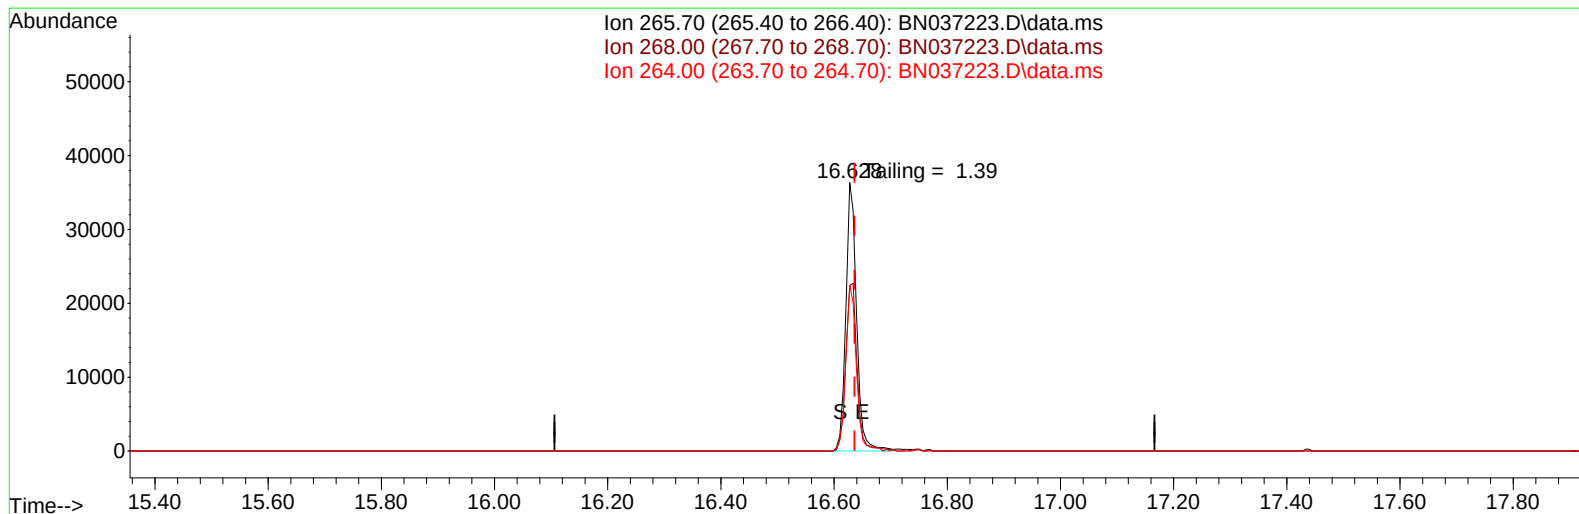

TIC: BN037223.D\data.ms

(70) Pentachlorophenol (C)




16.628min (-0.008) 13765.31 ng

response 48504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.73
264.00	61.60	61.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037223.D
Acq On : 13 Jun 2025 11:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 18:35:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 10 06:01:37 2025
Response via : Initial Calibration

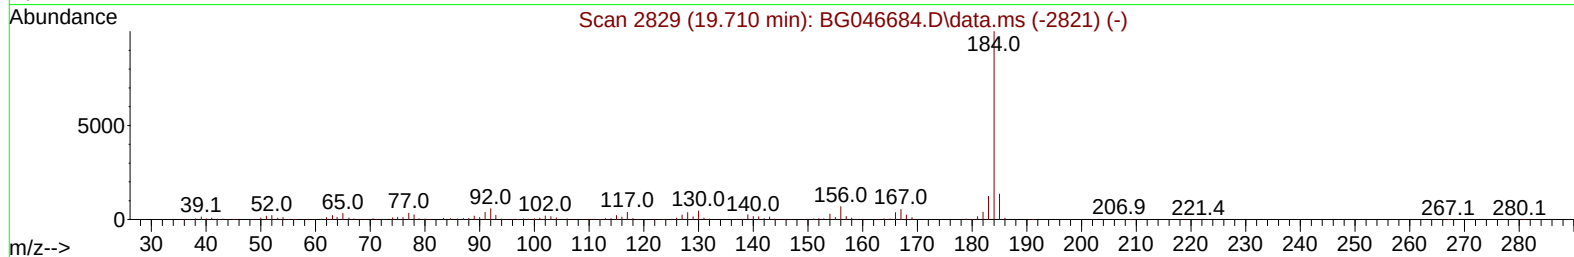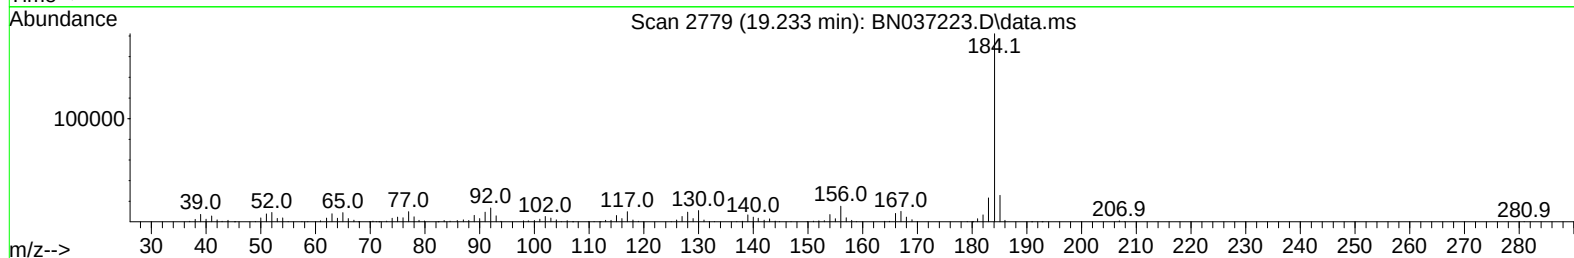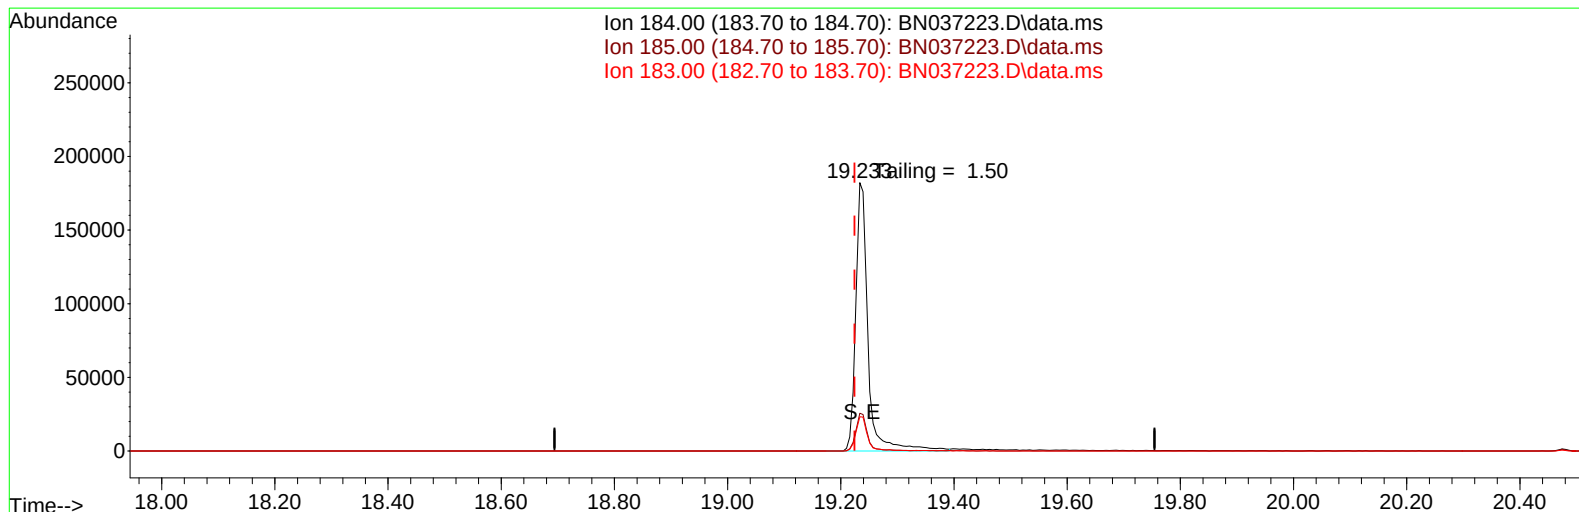

TIC: BN037223.D\data.ms

(77) Benzidine

19.233min (+ 0.009) 0.00 ng

response 272616

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.12
183.00	13.20	12.75
0.00	0.00	0.00