
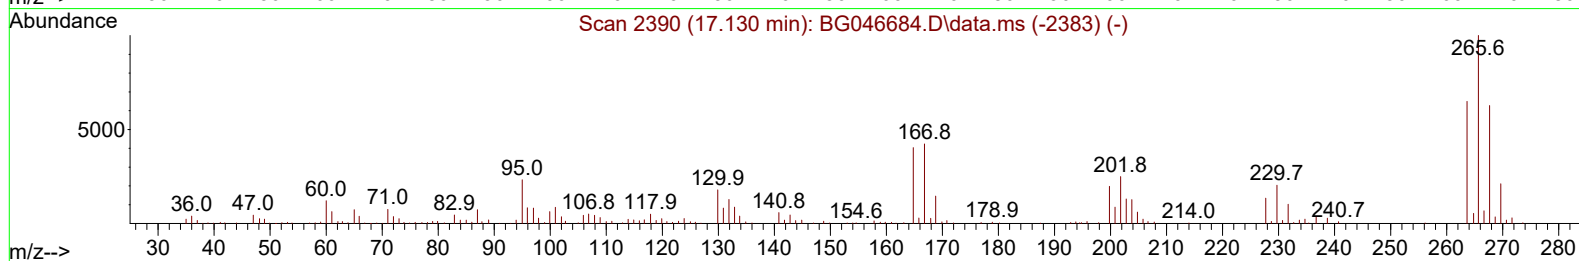
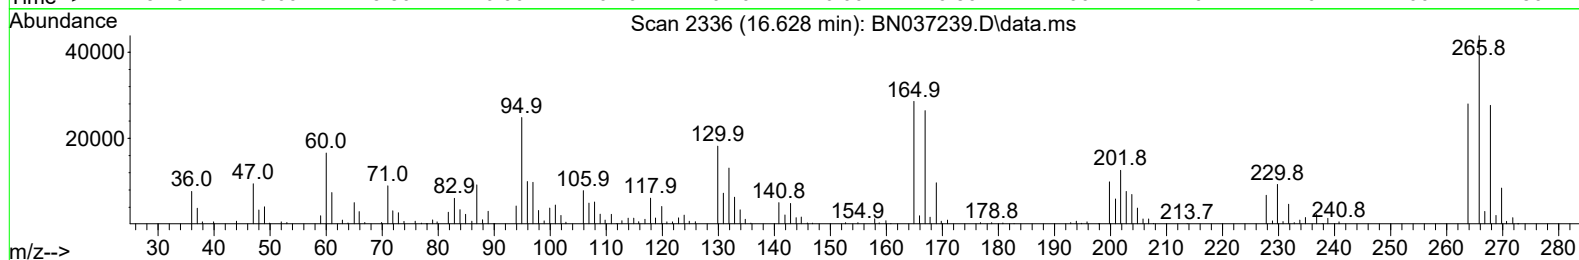


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037239.D
Acq On : 13 Jun 2025 23:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Jun 14 03:28:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 14 03:28:35 2025
Response via : Initial Calibration

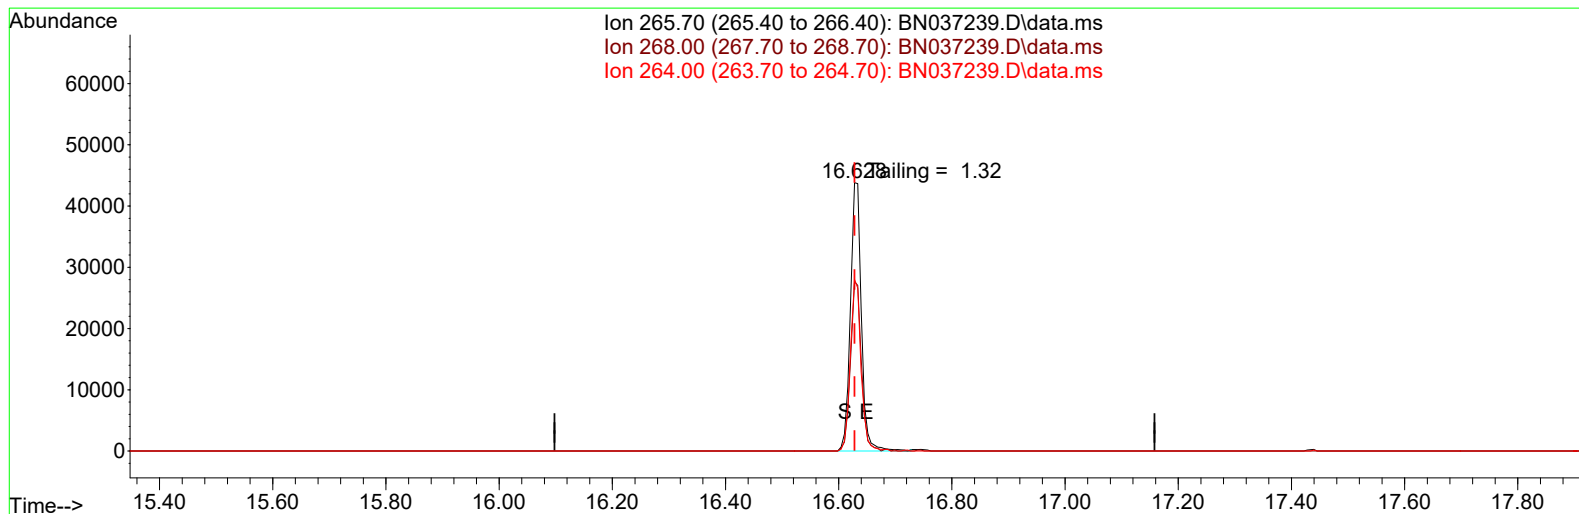

TIC: BN037239.D\data.ms

(70) Pentachlorophenol (C)




16.628min (0.000) 18785.64 ng

response 58970

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.13
264.00	61.60	63.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037239.D
Acq On : 13 Jun 2025 23:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Jun 14 03:28:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 14 03:28:35 2025
Response via : Initial Calibration

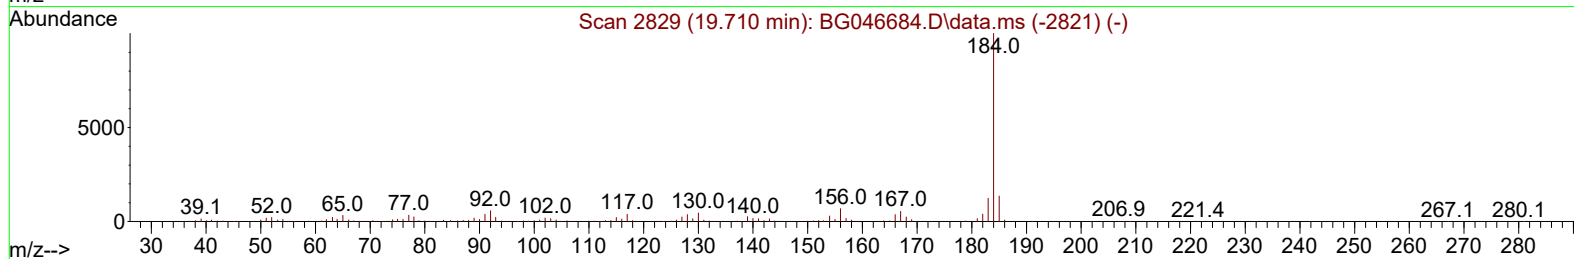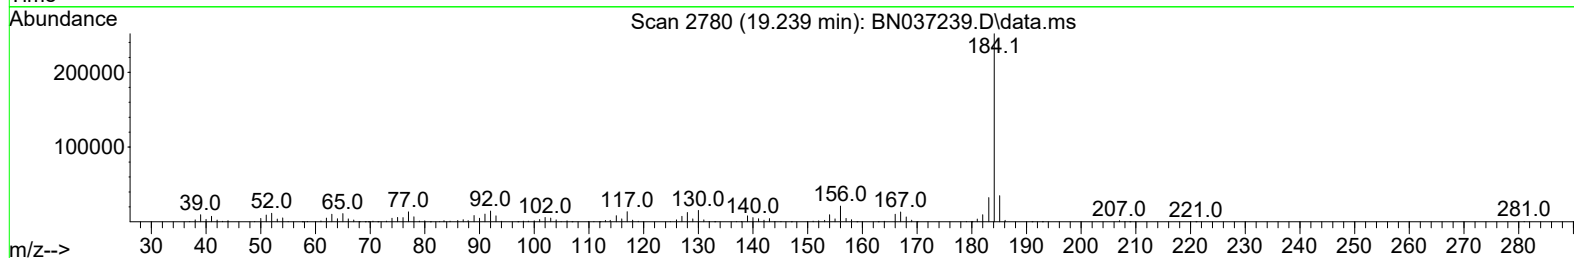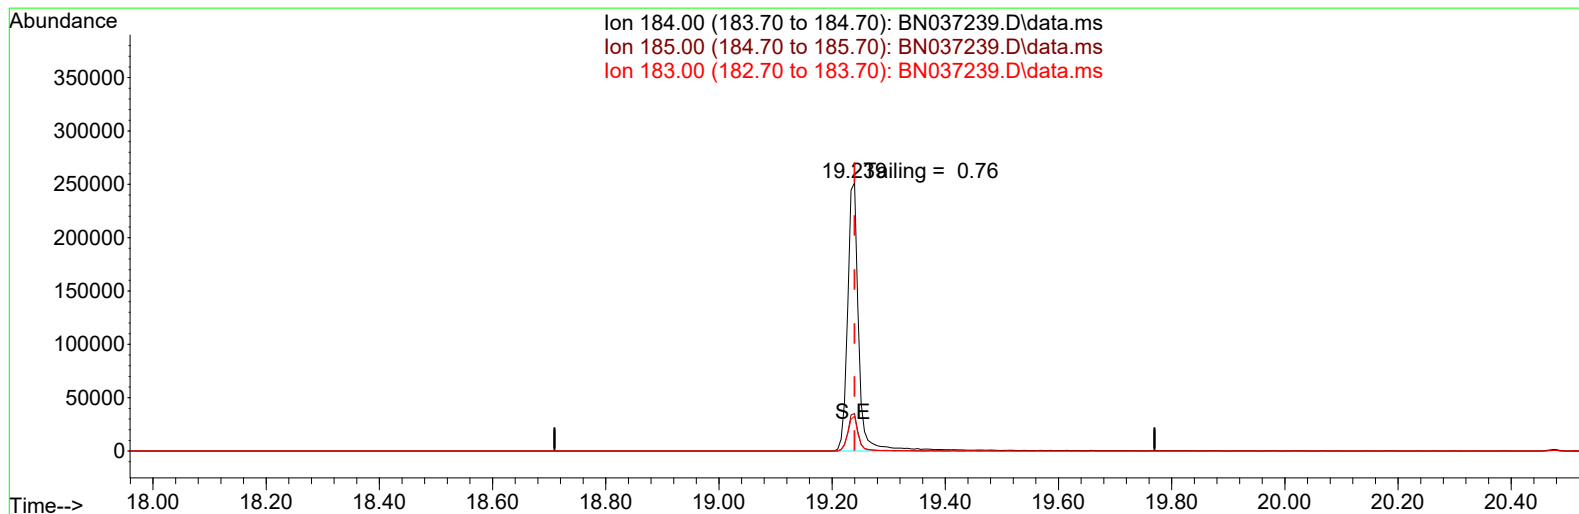

TIC: BN037239.D\data.ms

(77) Benzidine

19.239min (0.000) 0.00 ng

response 344668

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.97
183.00	13.20	12.95
0.00	0.00	0.00