
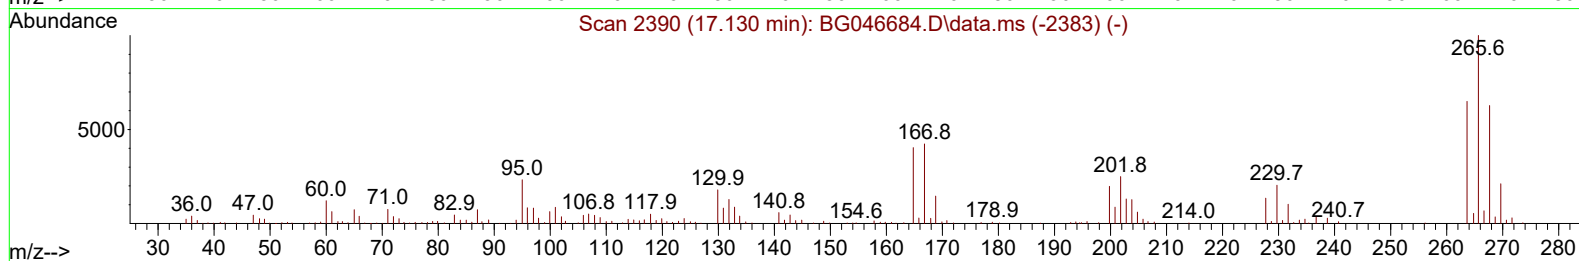
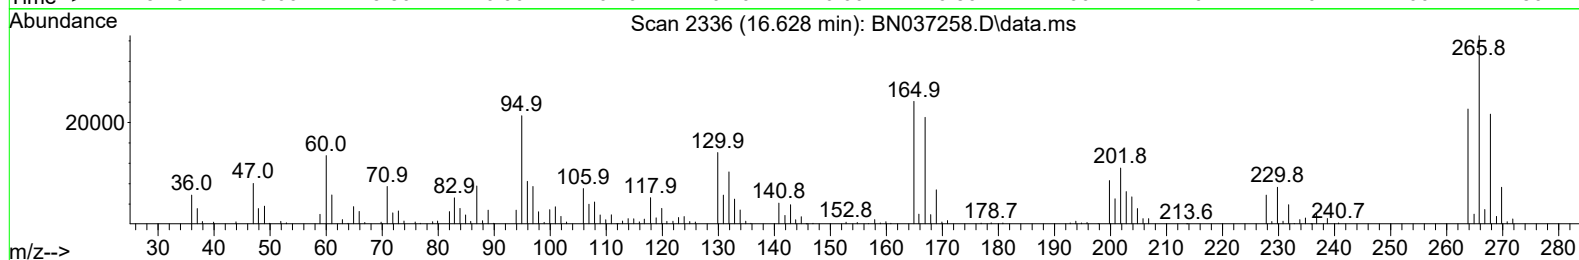


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN061325\  
Data File : BN037258.D  
Acq On : 14 Jun 2025 12:44  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Jun 16 01:30:30 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jun 16 01:30:21 2025  
Response via : Initial Calibration

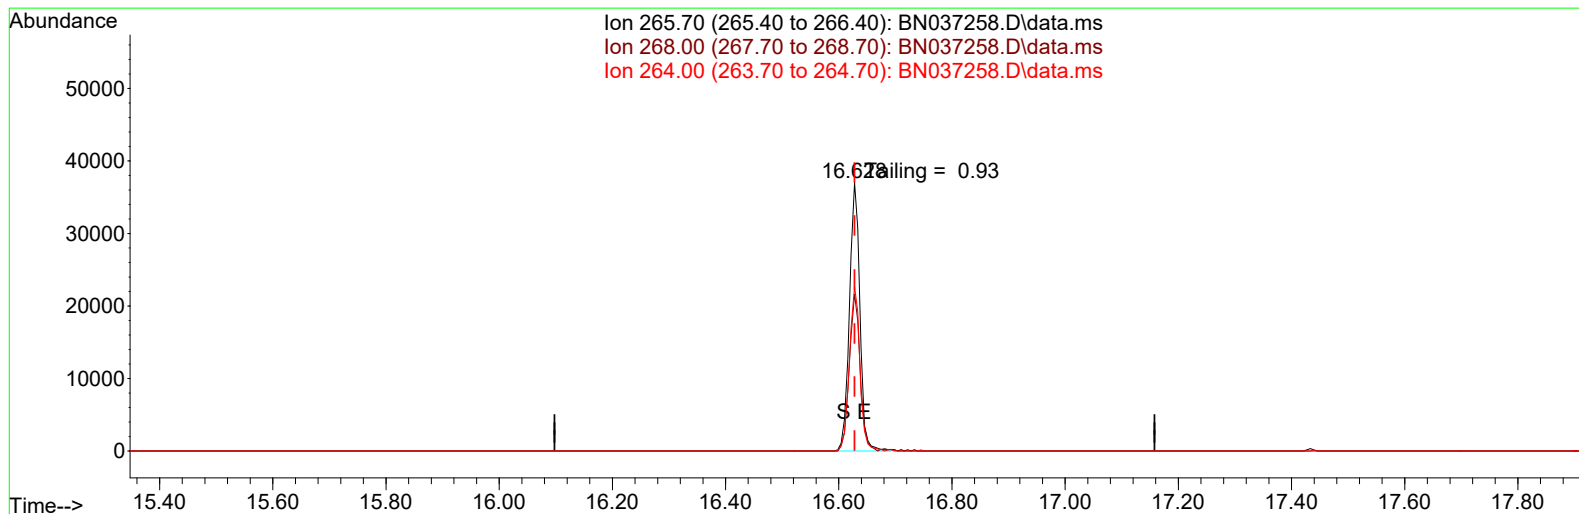

TIC: BN037258.D\data.ms

**(70) Pentachlorophenol (C)**




16.628min ( 0.000) 18255.95 ng

response 47565

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 58.50  |
| 264.00 | 61.60  | 61.21  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN061325\  
Data File : BN037258.D  
Acq On : 14 Jun 2025 12:44  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Jun 16 01:30:30 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jun 16 01:30:21 2025  
Response via : Initial Calibration

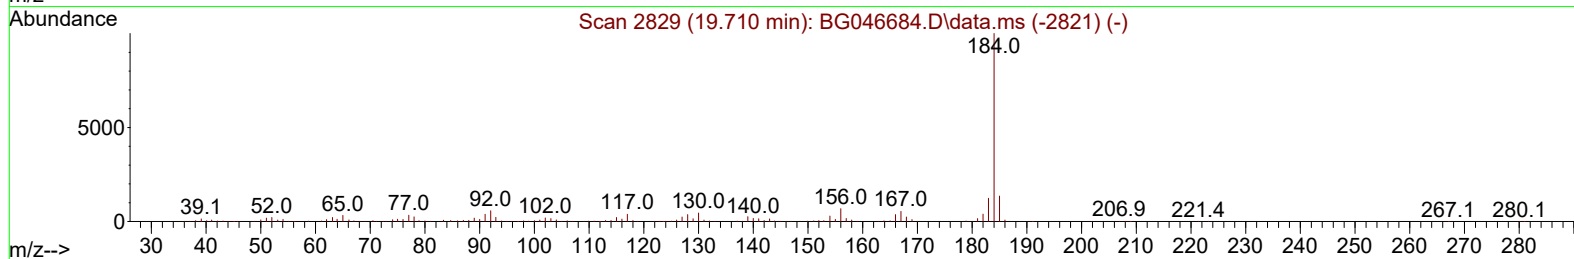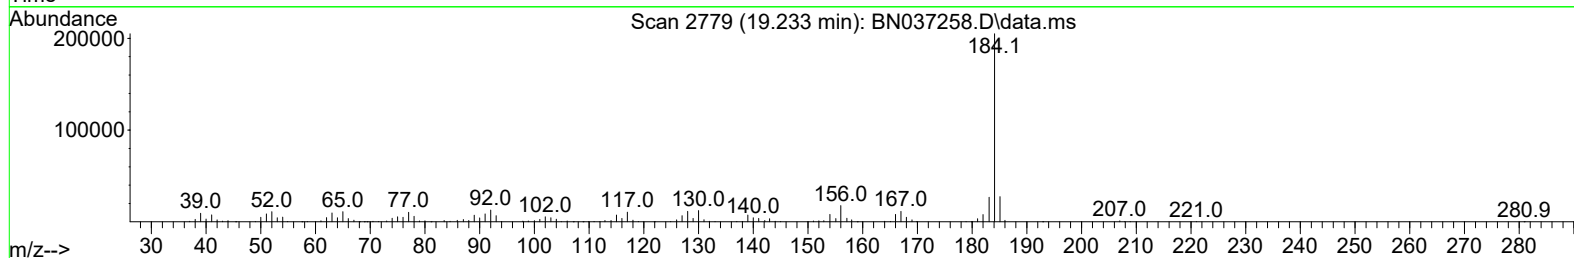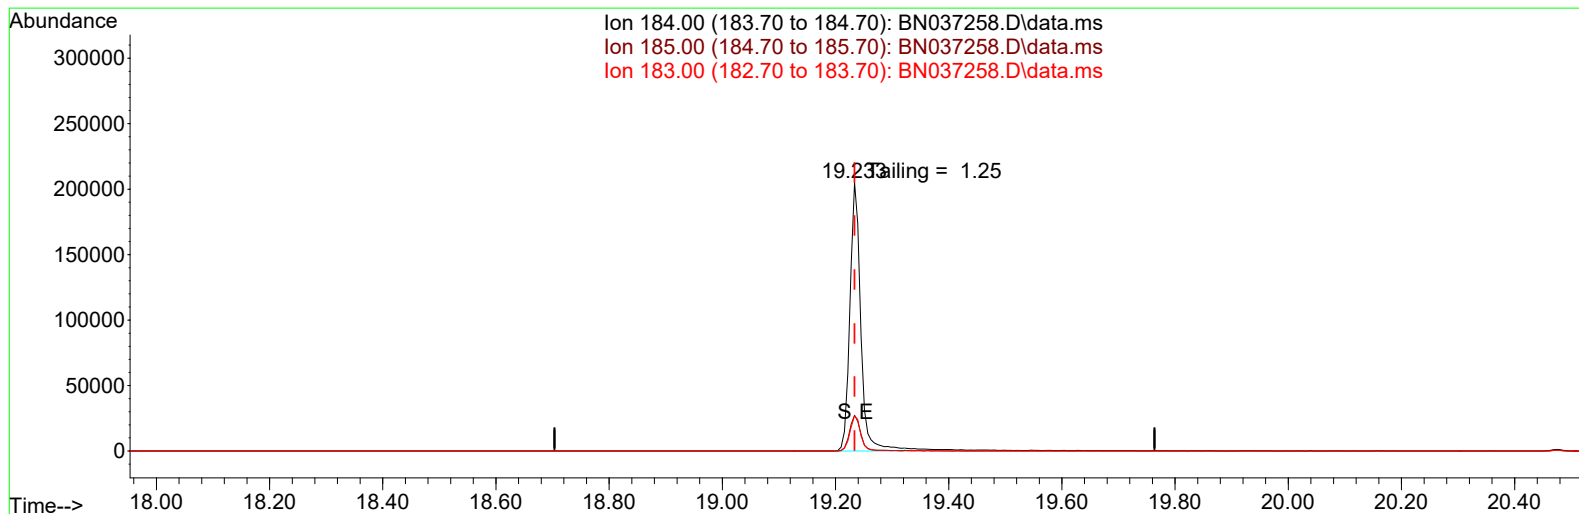

TIC: BN037258.D\data.ms

**(77) Benzidine**

19.233min ( 0.000) 0.00 ng

response 278955

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.39  |
| 183.00 | 13.20  | 13.11  |
| 0.00   | 0.00   | 0.00   |