
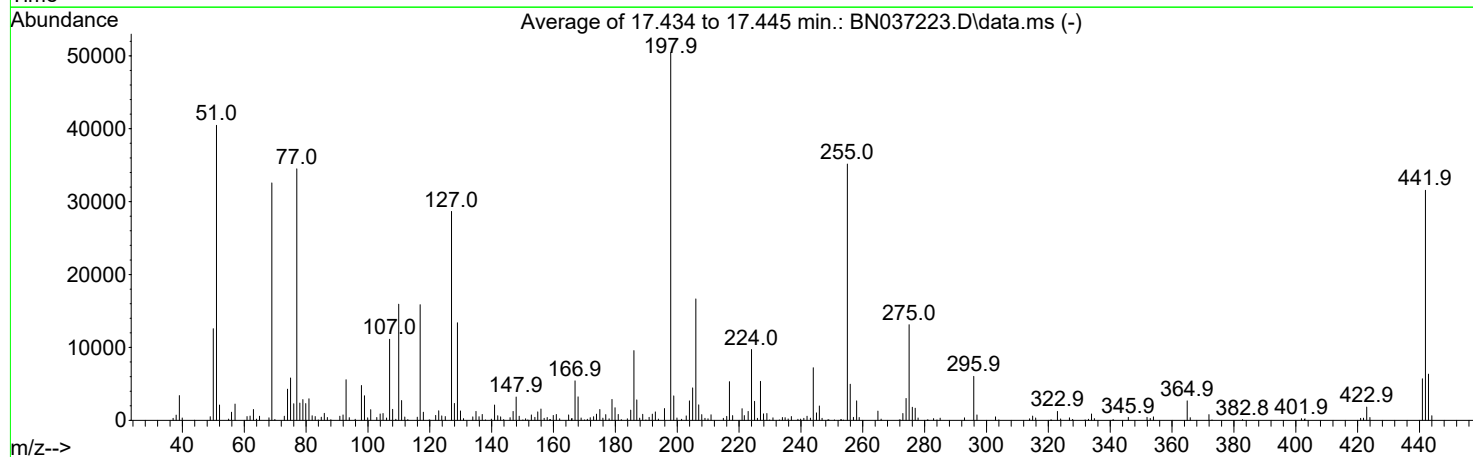


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037223.D
Acq On : 13 Jun 2025 11:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 13 18:43:34 2025

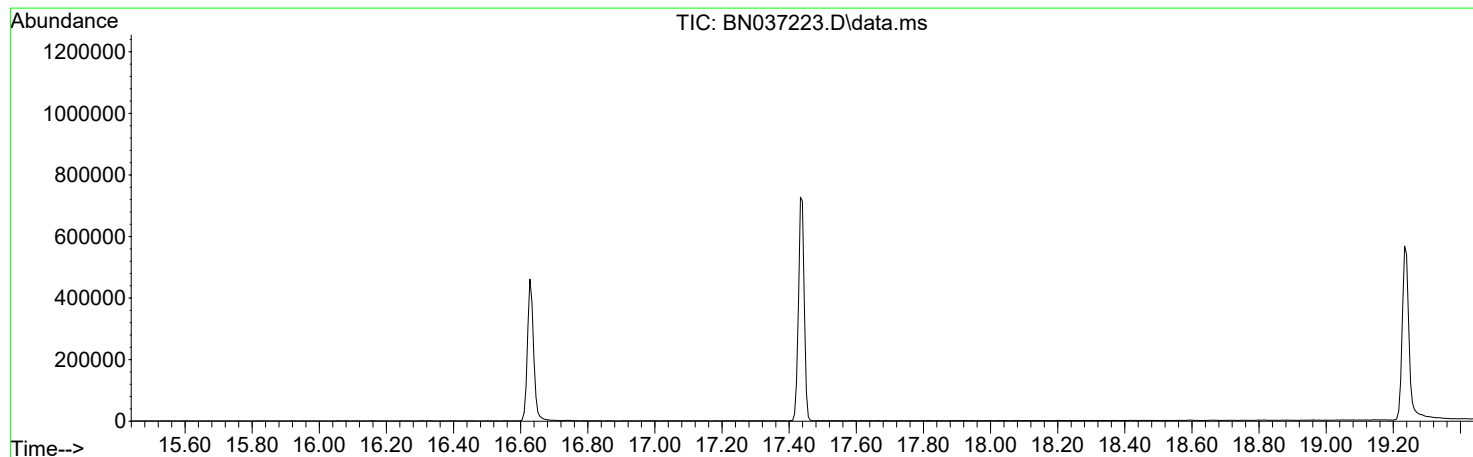

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	80.2	40477	FAIL*
68	69	0.00	2	1.1	362	PASS
69	198	0.00	100	64.6	32573	PASS
70	69	0.00	2	0.4	132	PASS
127	198	10	80	56.8	28661	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50453	PASS
199	198	5	9	6.7	3367	PASS
275	198	10	60	26.0	13127	PASS
365	198	1	100	5.3	2675	PASS
441	198	0.01	100	11.3	5714	PASS
442	442	50	100	100.0	31557	PASS
443	442	15	24	20.1	6344	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/13/2025	BNA_N	<u>BN037223.D</u>
Compound Name	Response	Retention Time
DDT	179828	20.475
DDD	1789	20.086
DDE	62	19.528
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1851	181679	1.02

Instrument :
BNA_N
ClientSampleId :

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037272.D
Acq On : 14 Jun 2025 21:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 16 03:00:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 16 03:00:26 2025
Response via : Initial Calibration

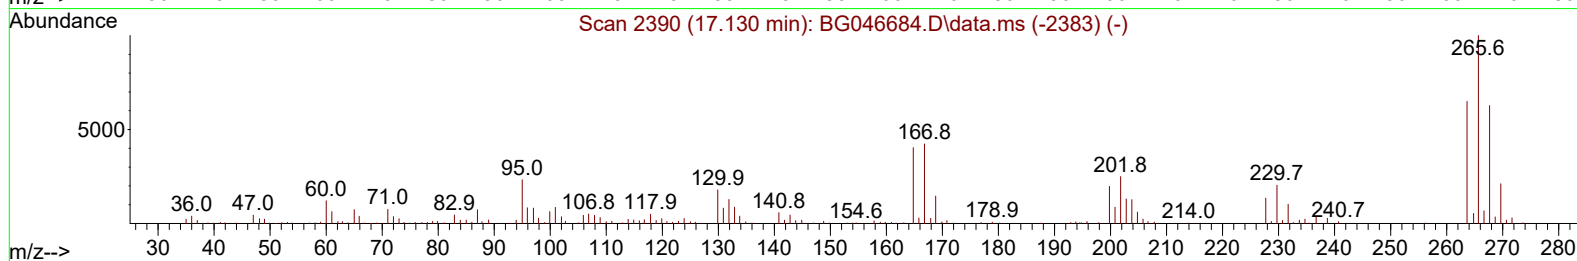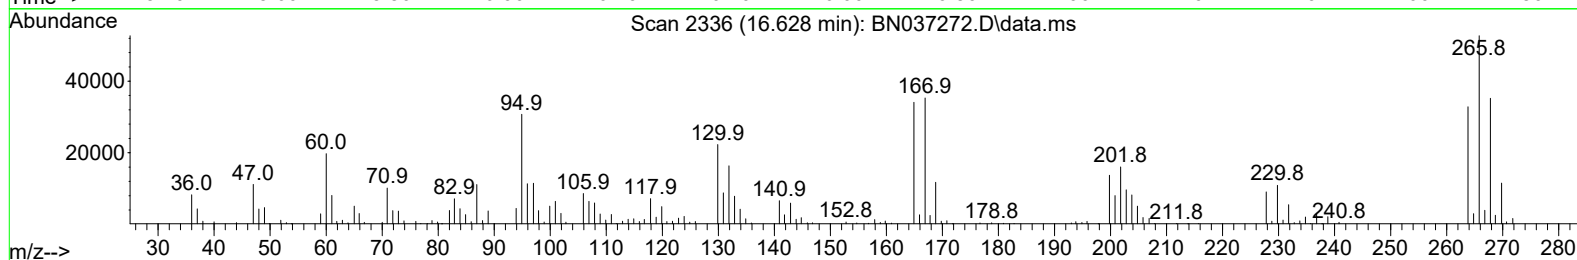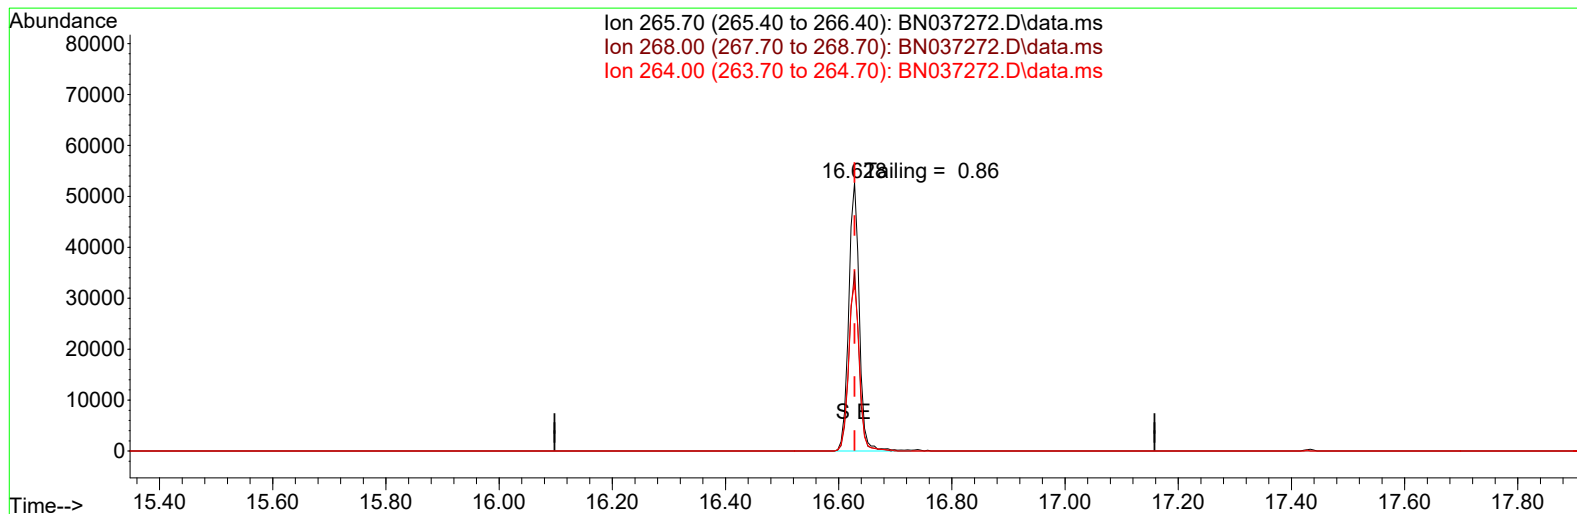

TIC: BN037272.D\data.ms

(70) Pentachlorophenol (C)

16.628min (0.000) 15244.65 ng




response 68073

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.57
264.00	61.60	62.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037272.D
Acq On : 14 Jun 2025 21:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 16 03:00:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 16 03:00:26 2025
Response via : Initial Calibration

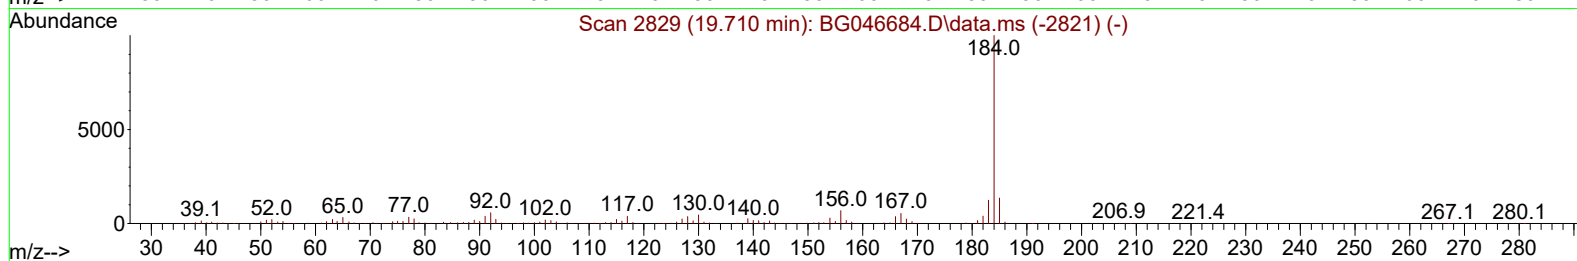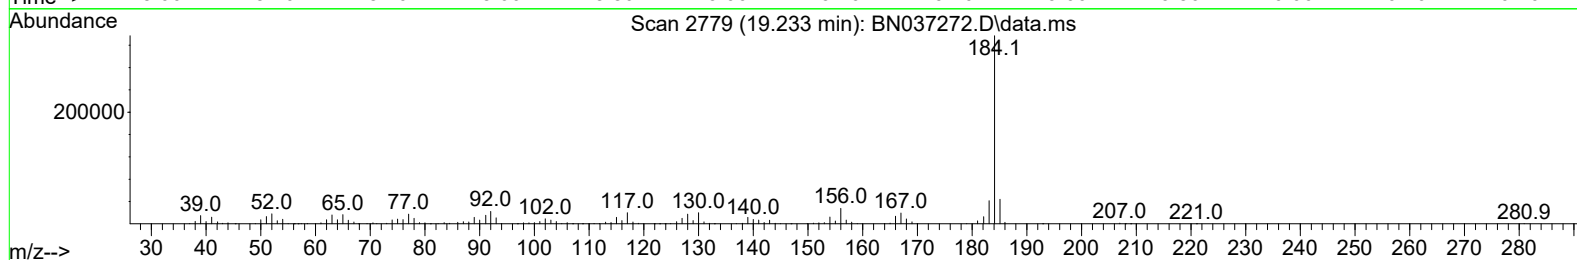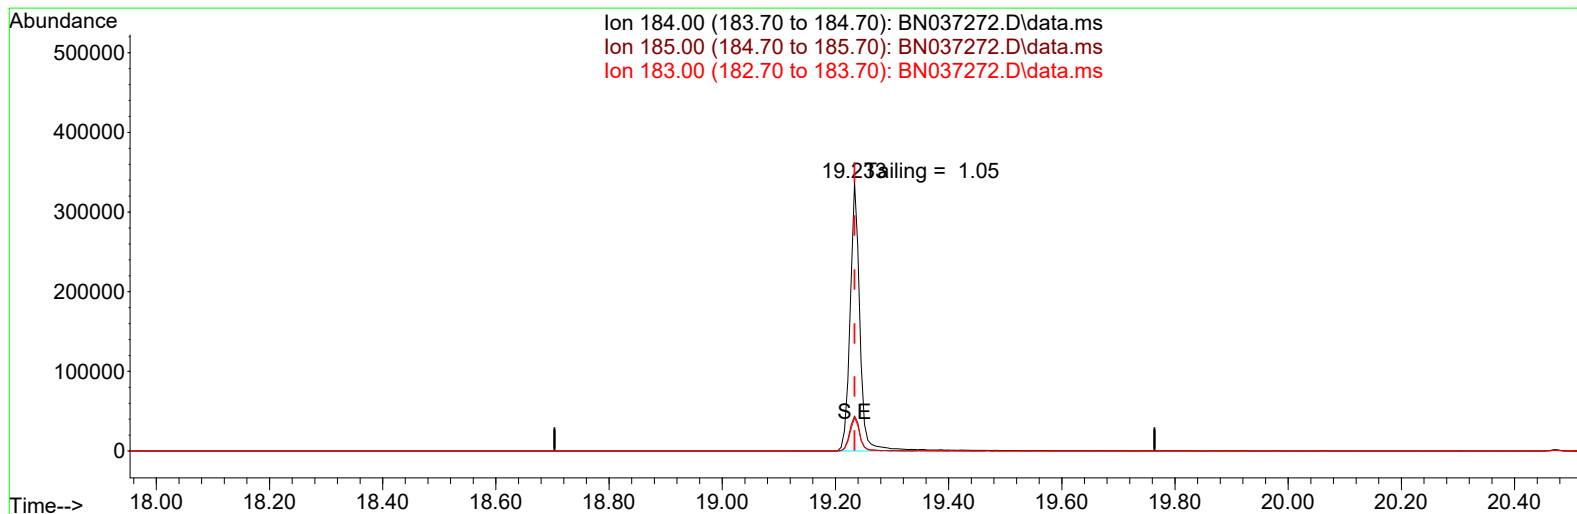

TIC: BN037272.D\data.ms

(77) Benzidine

19.233min (0.000) 0.00 ng

response 404622

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.08
183.00	13.20	12.35
0.00	0.00	0.00