


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037258.D
Acq On : 14 Jun 2025 12:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 19 02:50:12 2025

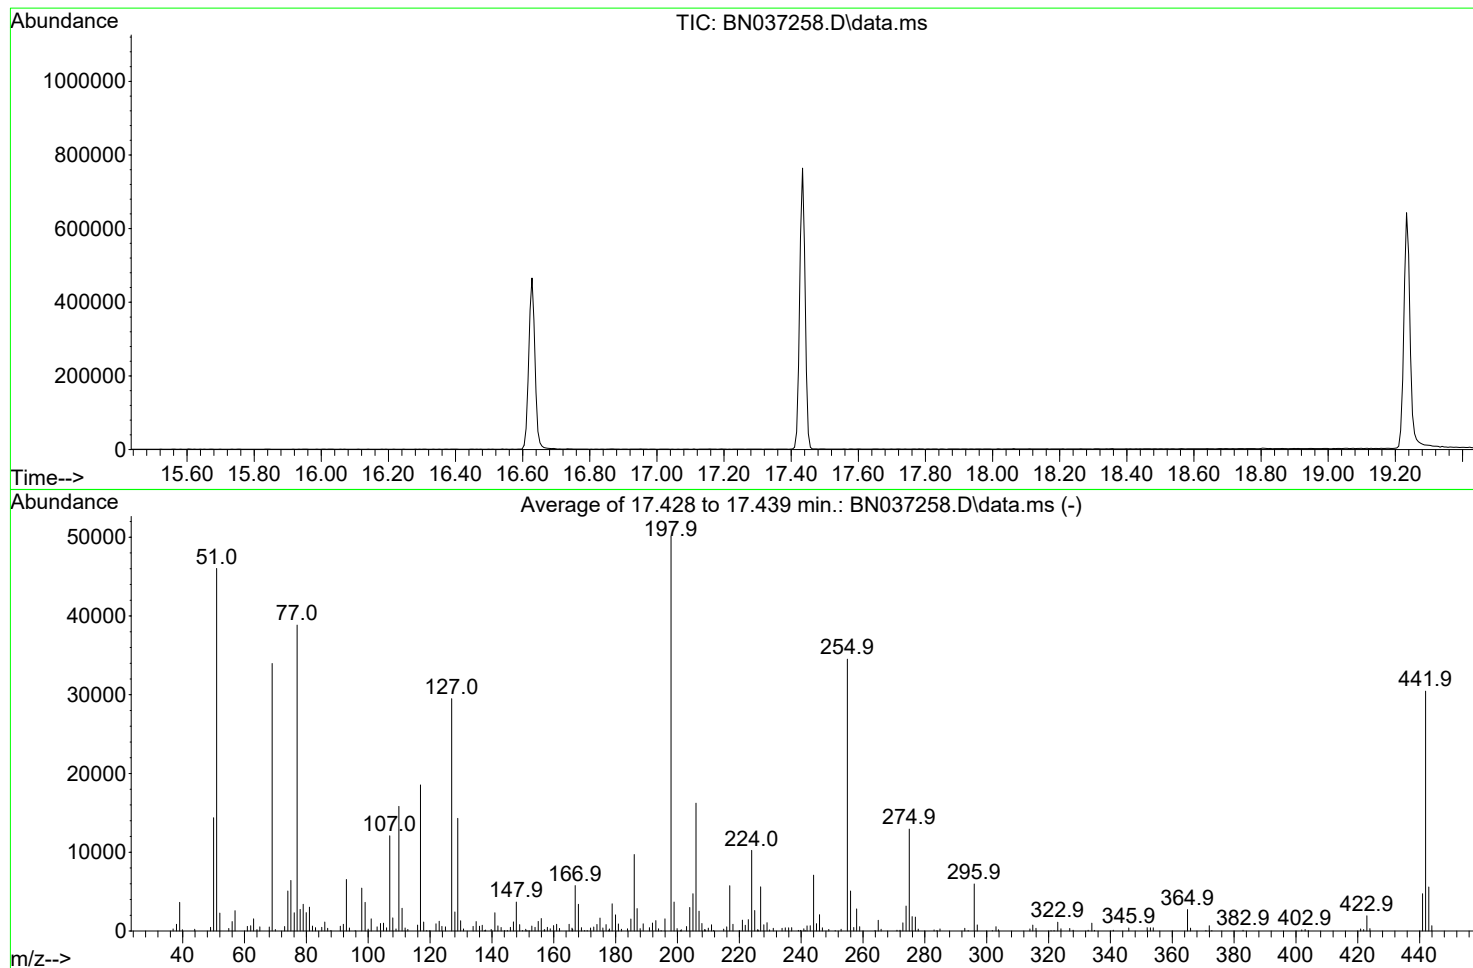

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	513	PASS
69	69	100	100	100.0	33968	PASS
70	69	0.00	2	0.6	187	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50133	PASS
199	198	5	9	7.3	3674	PASS
365	198	1	100	5.4	2731	PASS
441	443	0.01	150	84.6	4726	PASS
442	442	100	100	100.0	30451	PASS
443	442	15	24	18.3	5584	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/13/2025	BNA_N	<u>BN037258.D</u>
Compound Name	Response	Retention Time
DDT	157903	20.475
DDD	2424	20.033
DDE	2656	17.434
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5080	162983	3.12

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037258.D
Acq On : 14 Jun 2025 12:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 16 01:30:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 16 01:30:21 2025
Response via : Initial Calibration

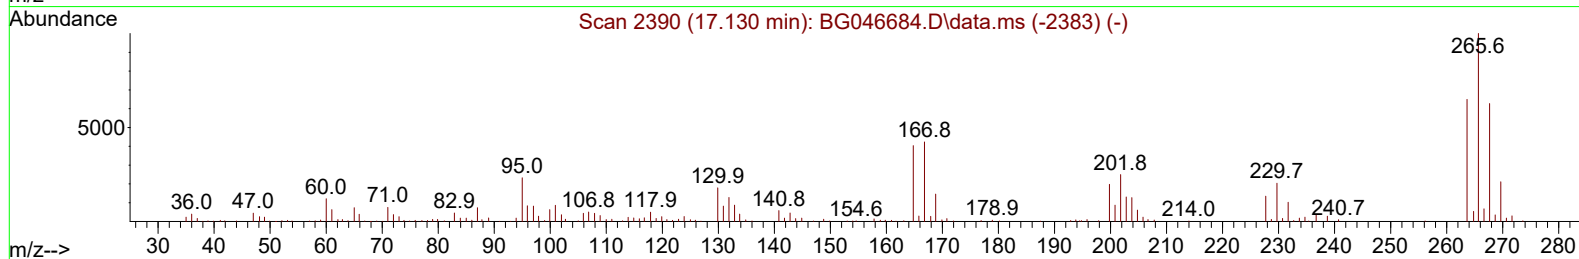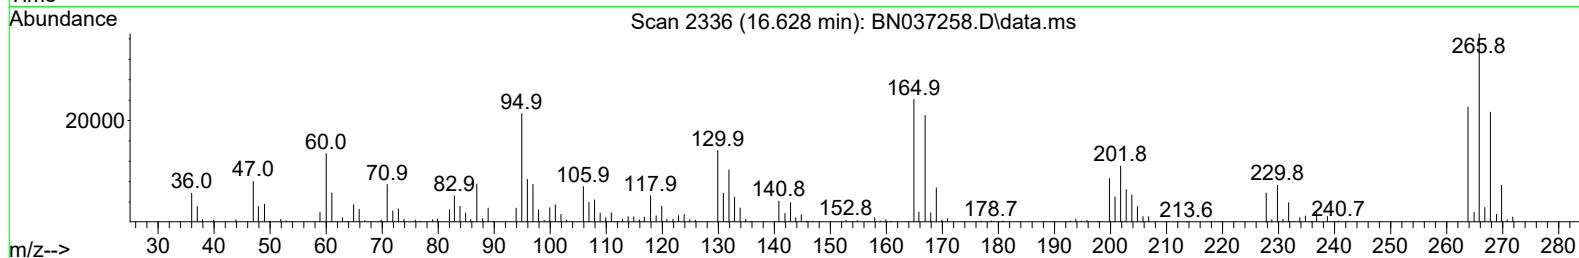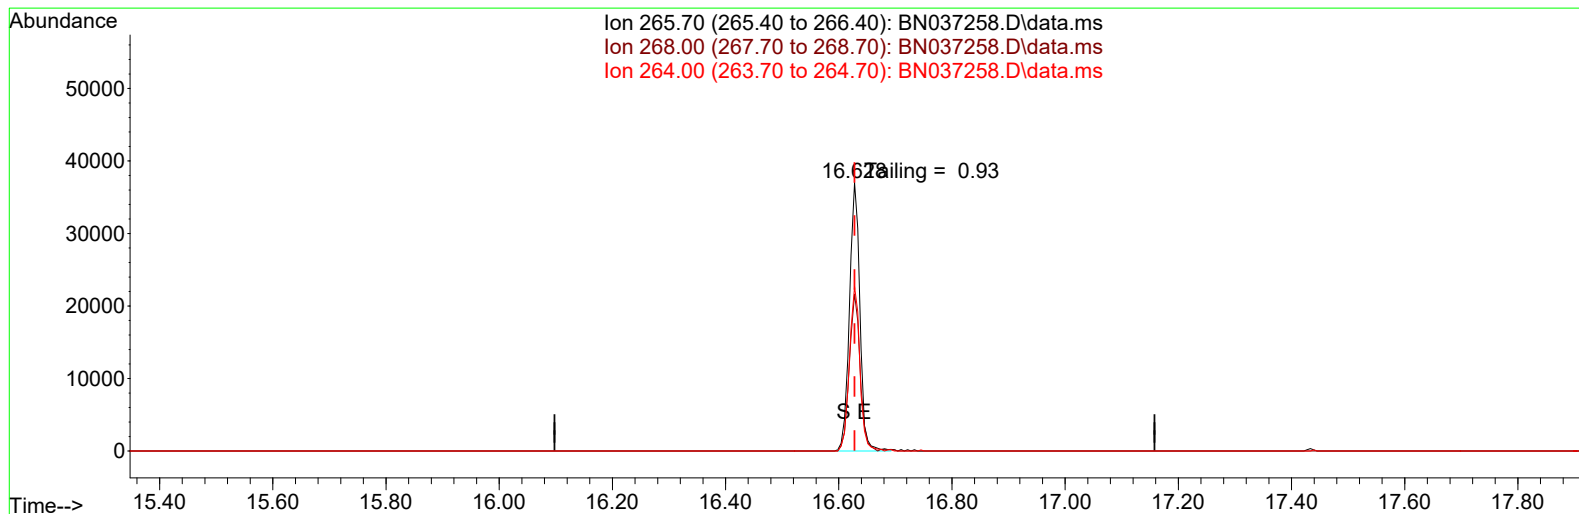

TIC: BN037258.D\data.ms

(70) Pentachlorophenol (C)

16.628min (0.000) 18255.95 ng




response 47565

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.50
264.00	61.60	61.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037258.D
Acq On : 14 Jun 2025 12:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 16 01:30:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 16 01:30:21 2025
Response via : Initial Calibration

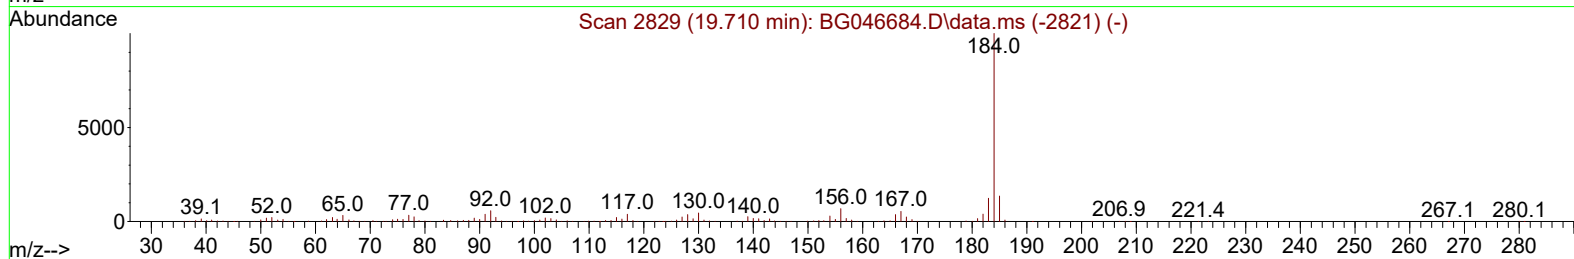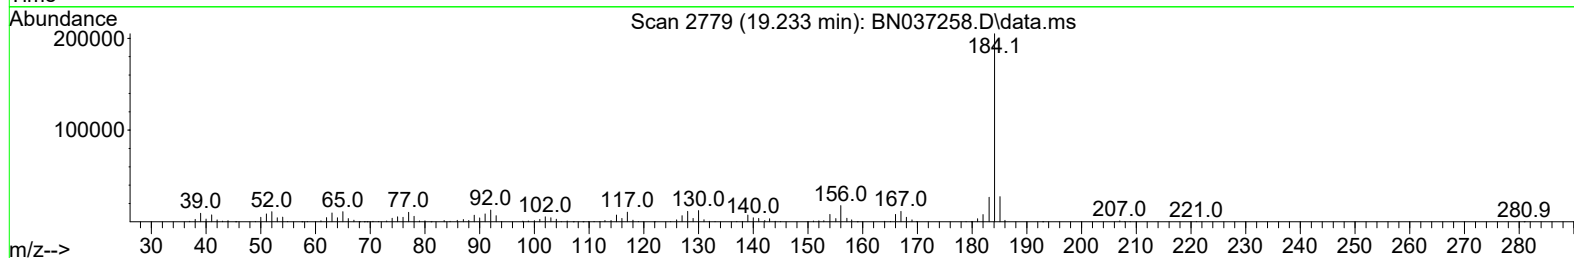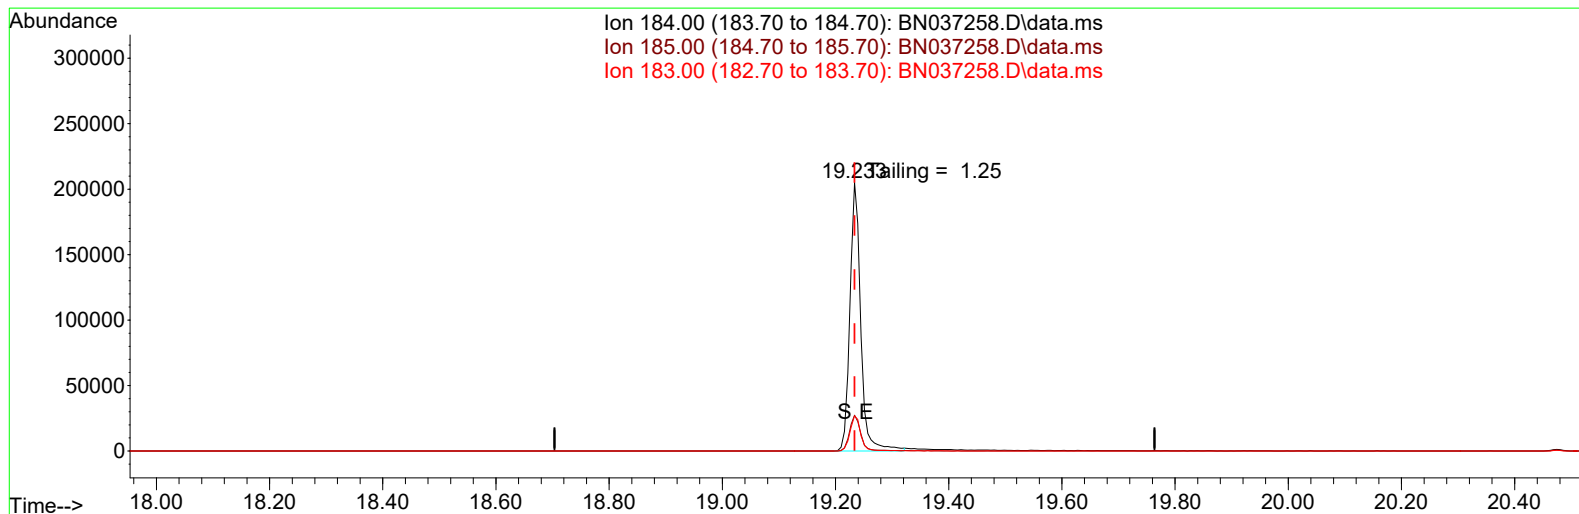

TIC: BN037258.D\data.ms

(77) Benzidine

19.233min (0.000) 0.00 ng

response 278955

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.39
183.00	13.20	13.11
0.00	0.00	0.00