

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014898.D
 Acq On : 14 Jun 2021 09:11
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC020

Manual Integrations
 APPROVED

mohammad
 6/15/2021 2:41:38 PM

Quant Time: Jun 14 10:46:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 14 10:46:06 2021
 Response via : Initial Calibration

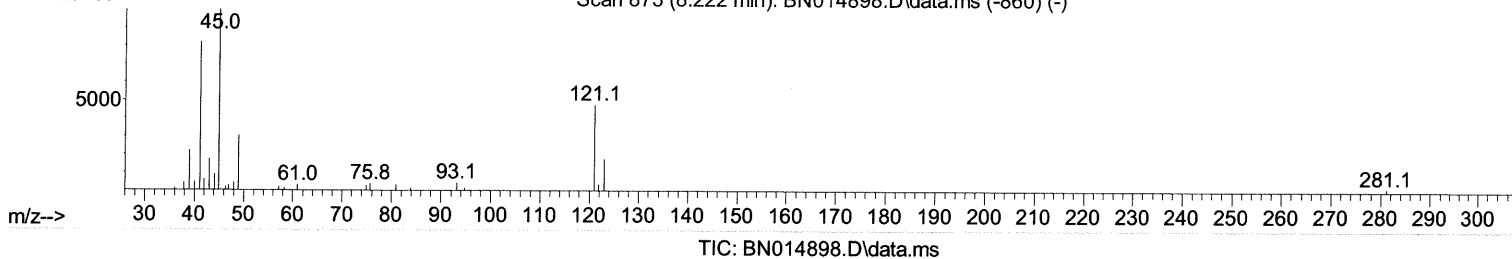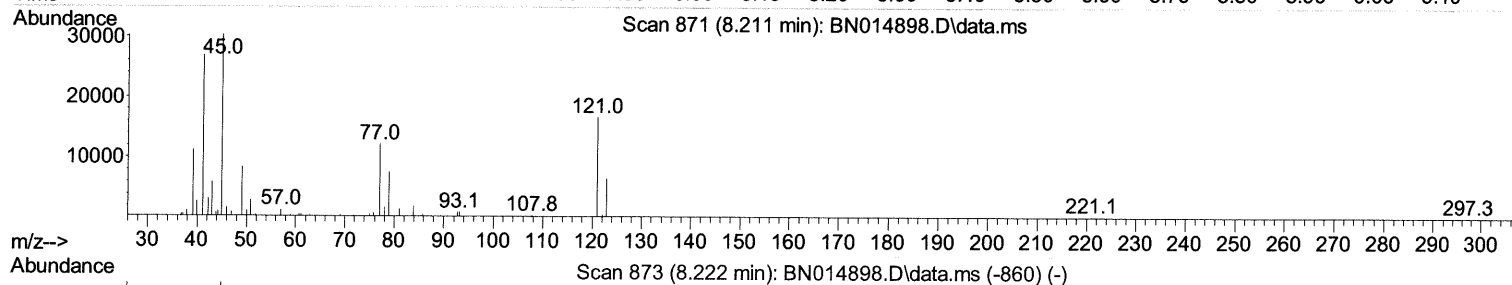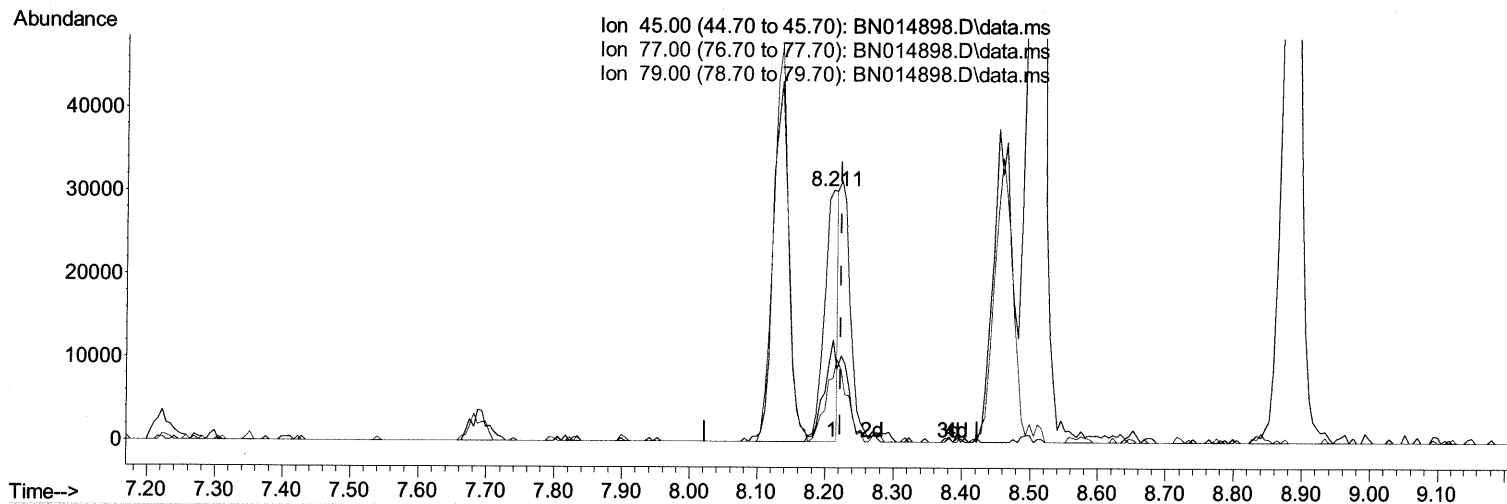

(14) 2,2'-oxybis(1-Chloropropane)

8.211min (-0.012) 10.44 ng/ul

response 43268

Ion	Exp%	Act%
45.00	100.00	100.00
77.00	32.30	40.53#
79.00	26.80	25.06
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014898.D
 Acq On : 14 Jun 2021 09:11
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC020

Manual Integrations
 APPROVED

mohammad
 6/15/2021 2:41:38 PM

Quant Time: Jun 14 10:46:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 14 10:46:06 2021
 Response via : Initial Calibration

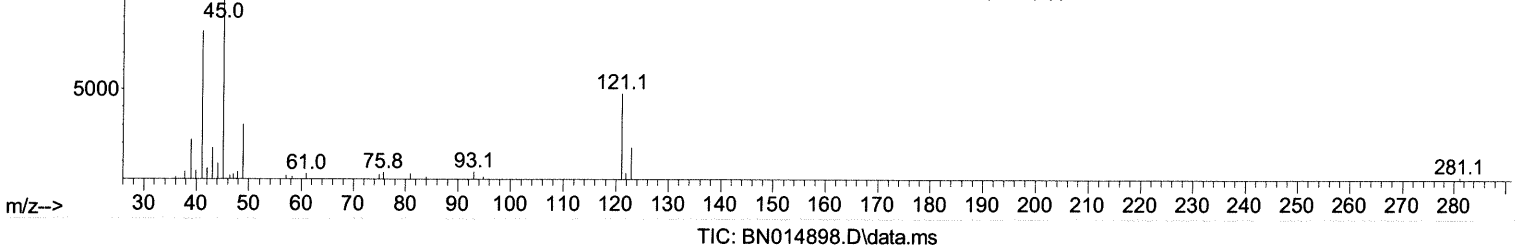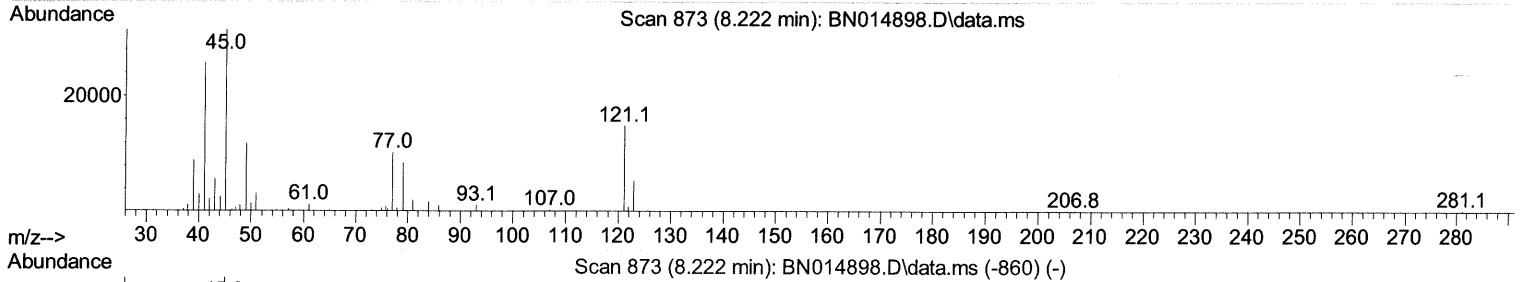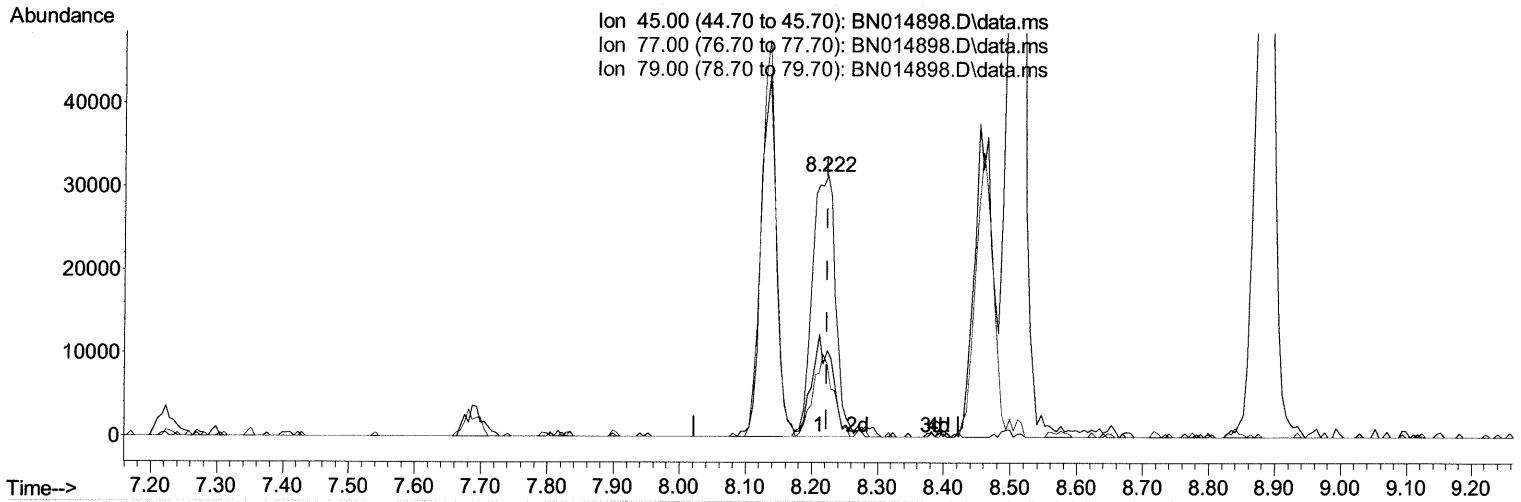

(14) 2,2'-oxybis(1-Chloropropane)

8.222min (0.000) 18.52 ng/ul m 06/16/21 JU

response 76761

Ion	Exp%	Act%
45.00	100.00	100.00
77.00	32.30	33.01
79.00	26.80	27.45
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014898.D
 Acq On : 14 Jun 2021 09:11
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC020

Manual Integrations
 APPROVED

mohammad
 6/15/2021 2:41:38 PM

Quant Time: Jun 14 10:46:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 14 10:46:06 2021
 Response via : Initial Calibration

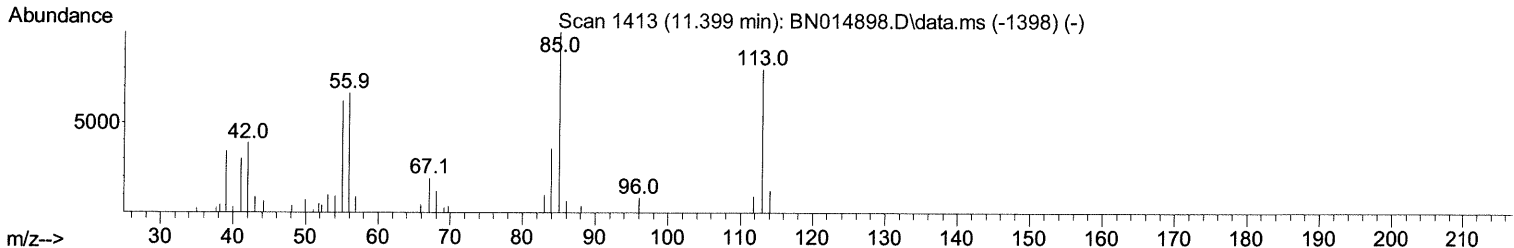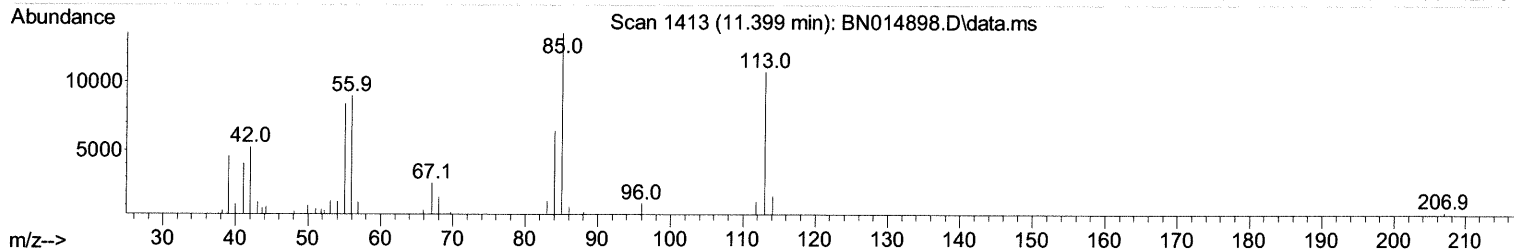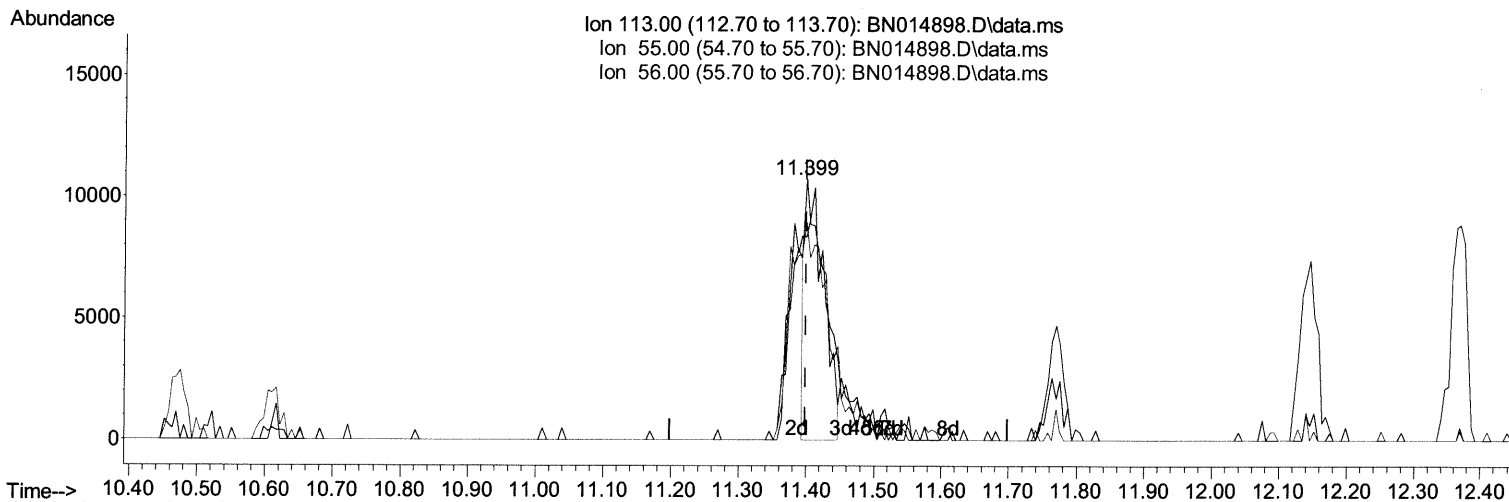

TIC: BN014898.D\data.ms

(34) Caprolactam

11.399min (0.000) 9.96 ng/ul

response 20503

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	118.50	77.97#
56.00	73.20	83.36
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014898.D
 Acq On : 14 Jun 2021 09:11
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC020

Manual Integrations
 APPROVED

mohammad
 6/15/2021 2:41:38 PM

Quant Time: Jun 14 10:46:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 14 10:46:06 2021
 Response via : Initial Calibration

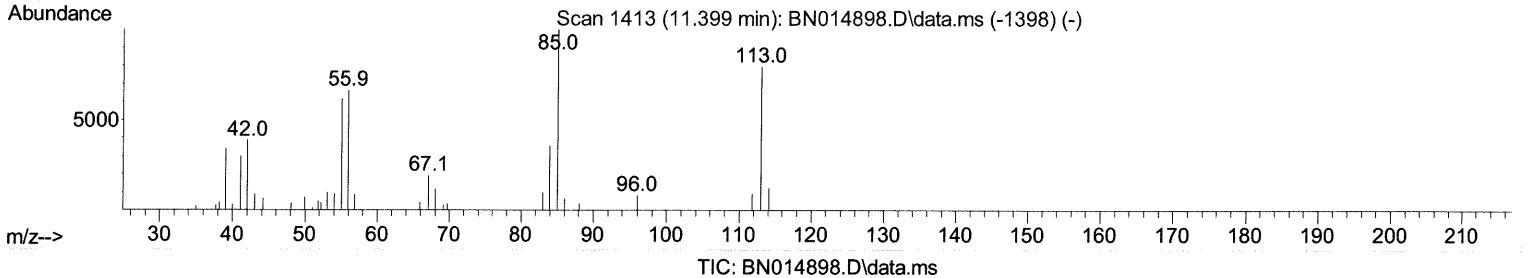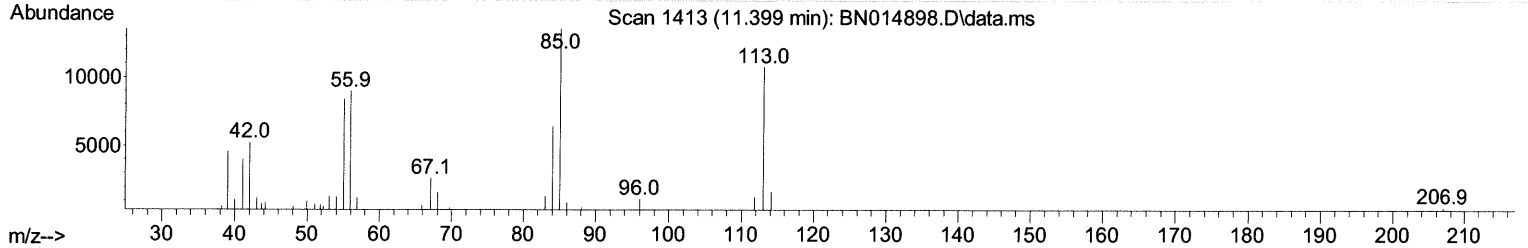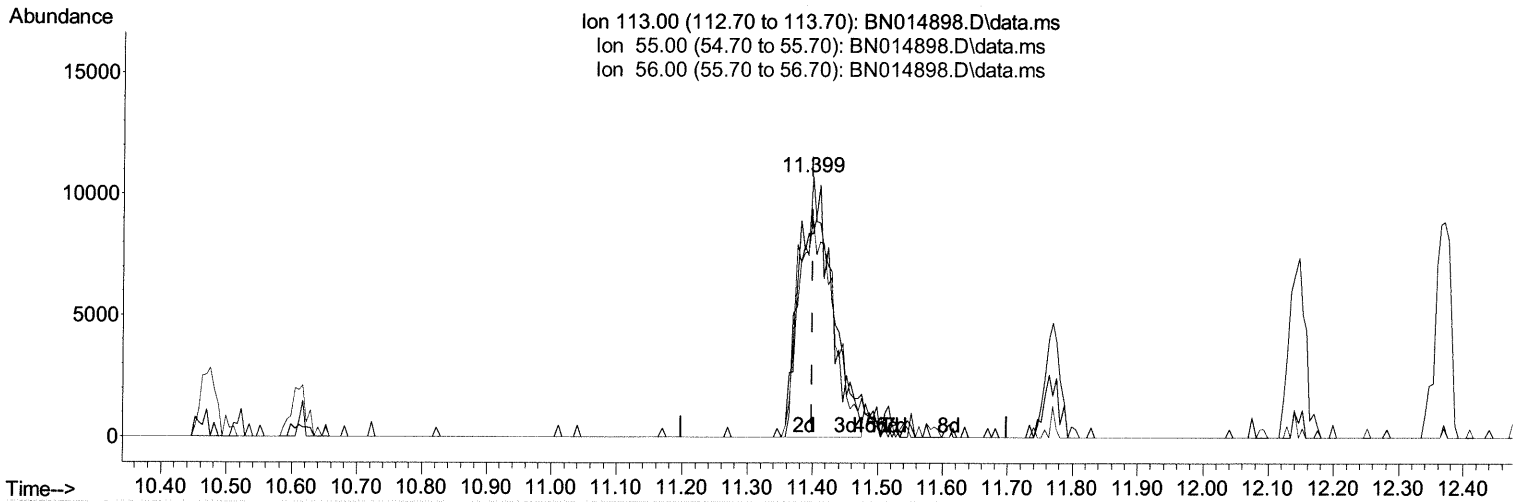

(34) Caprolactam

11.399min (0.000) 17.04 ng/ul m 06/16/21 JU

response 35072

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	118.50	77.97#
56.00	73.20	83.36
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014898.D
 Acq On : 14 Jun 2021 09:11
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC020

Manual Integrations
 APPROVED

mohammad
 6/15/2021 2:41:38 PM

Quant Time: Jun 14 10:46:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 14 10:46:06 2021
 Response via : Initial Calibration

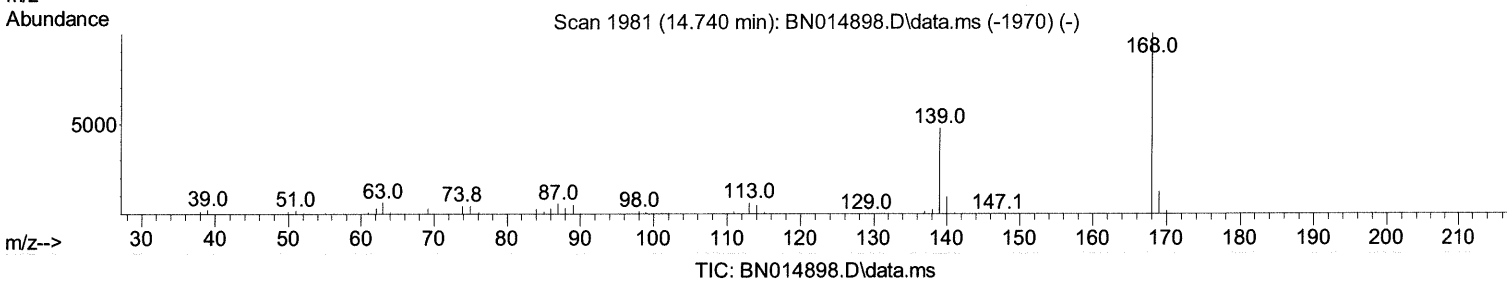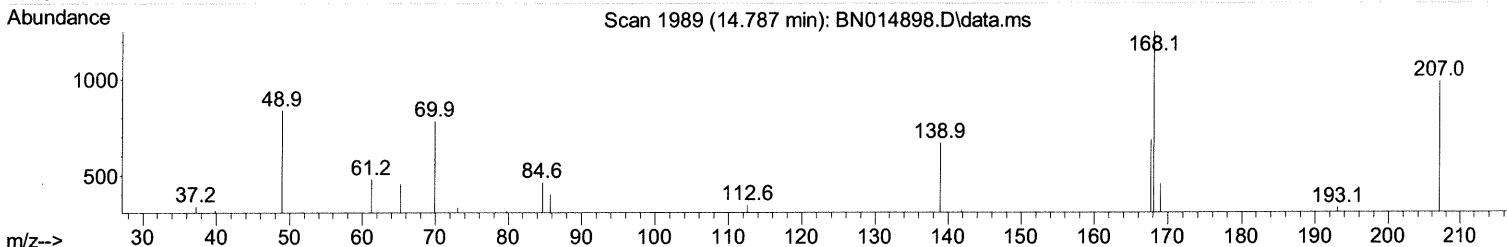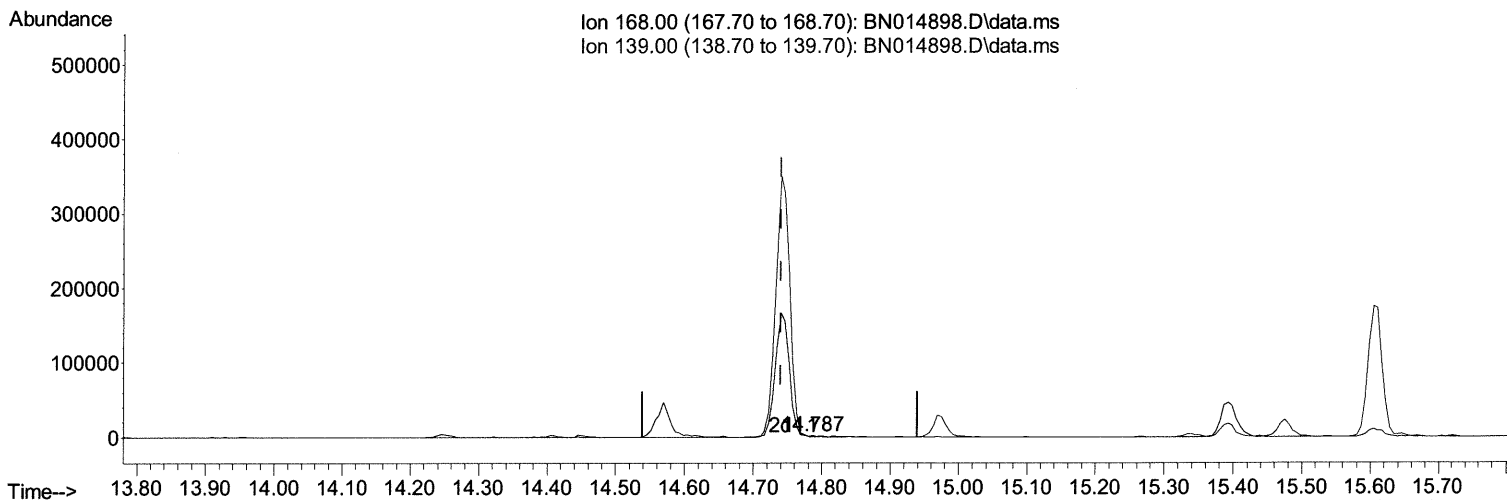

(56) Dibenzofuran

14.787min (+ 0.047) 0.05 ng/ul

response 1379

Ion	Exp%	Act%
168.00	100.00	100.00
139.00	36.90	34.48
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014898.D
 Acq On : 14 Jun 2021 09:11
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC020

Manual Integrations
 APPROVED

mohammad
 6/15/2021 2:41:38 PM

Quant Time: Jun 14 10:46:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 14 10:46:06 2021
 Response via : Initial Calibration

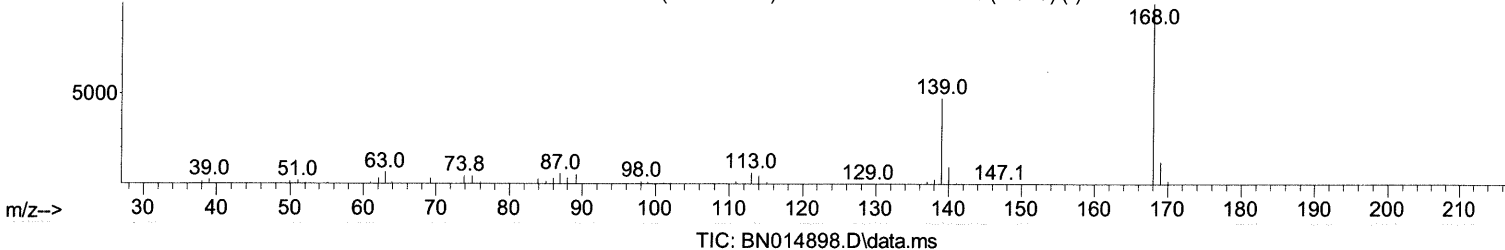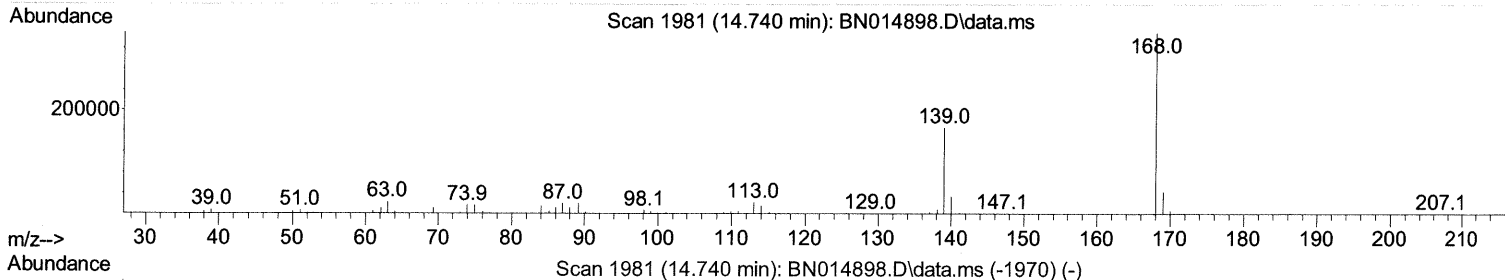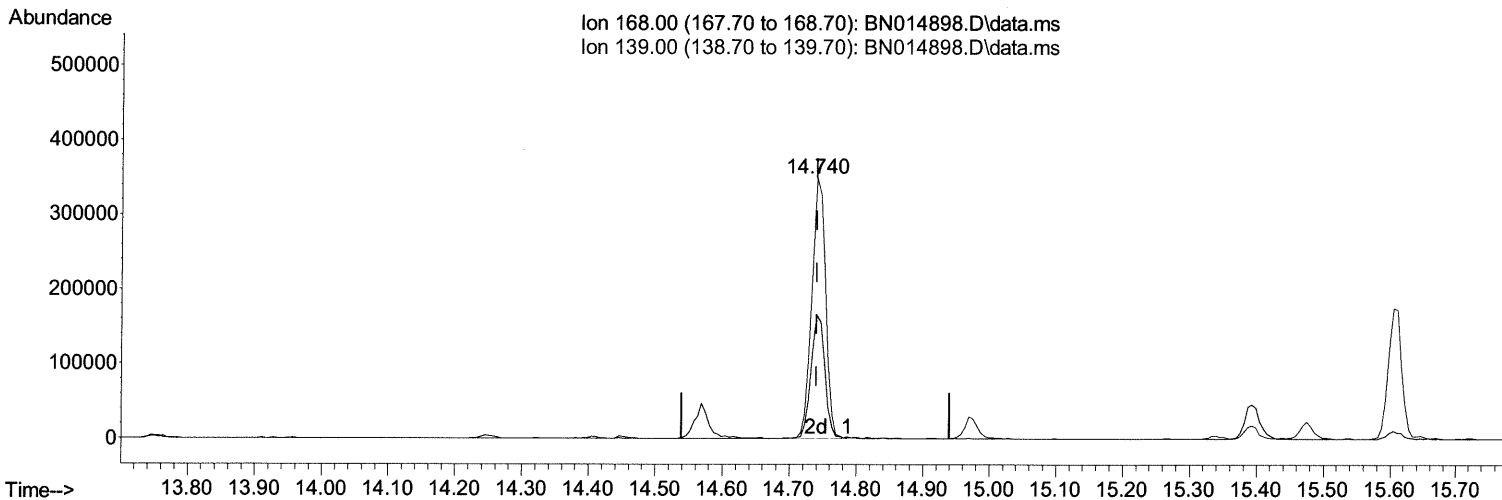

(56) Dibenzofuran

14.740min (0.000) 19.85 ng/ul m 06/16/21 JU

response 503406

Ion	Exp%	Act%
168.00	100.00	100.00
139.00	36.90	47.58#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014898.D
Acq On : 14 Jun 2021 09:11
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC020

Manual Integrations
APPROVED

mohammad
6/15/2021 2:41:38 PM

Quant Time: Jun 14 10:46:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 14 10:46:06 2021
Response via : Initial Calibration

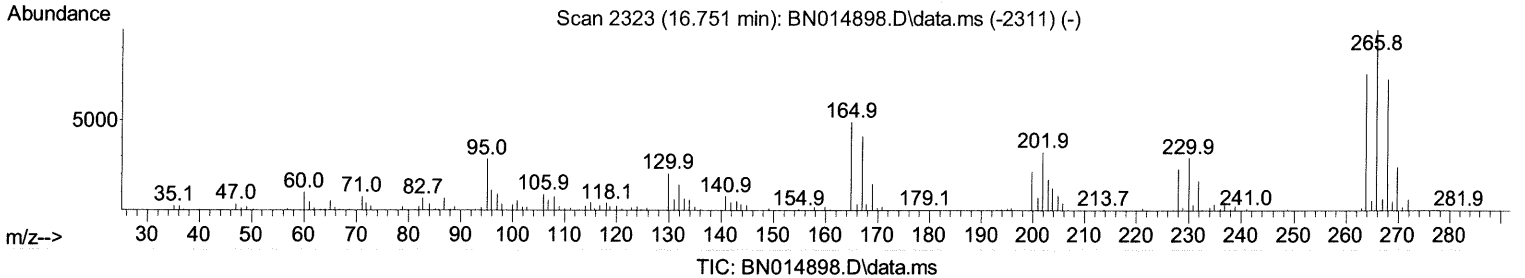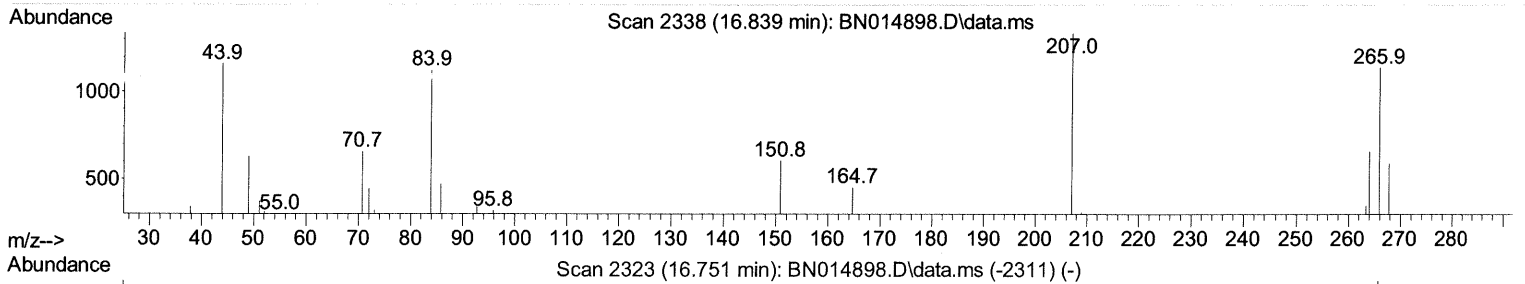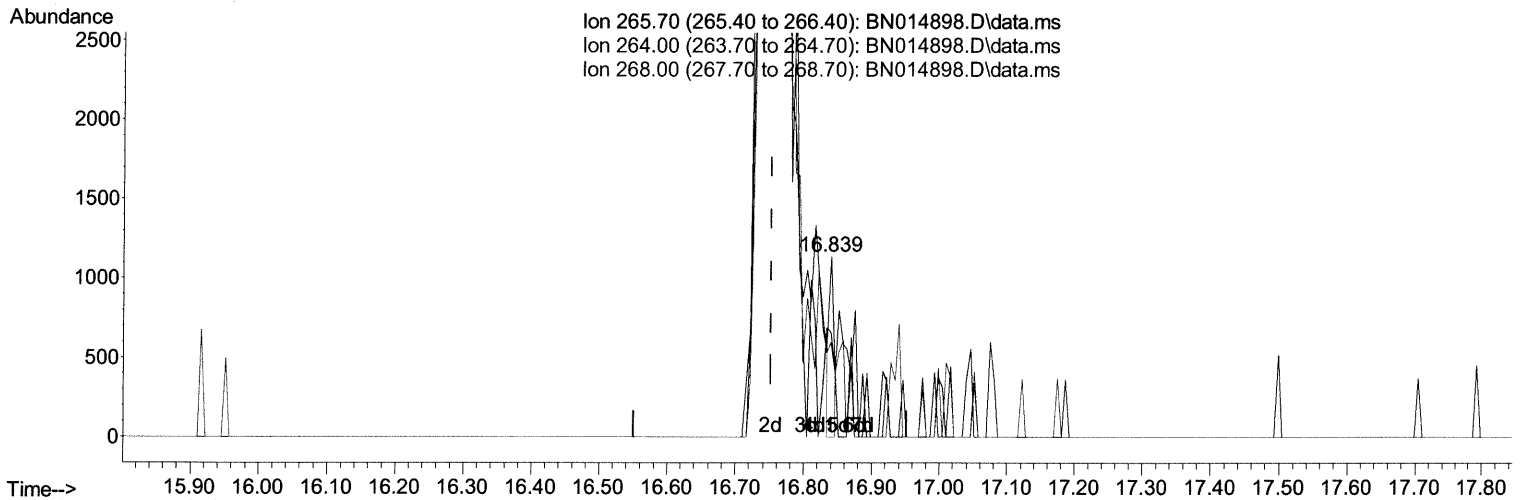

(71) Pentachlorophenol (C)

16.839min (+ 0.088) 0.11 ng/ul

response 545

Ion	Exp%	Act%
265.70	100.00	100.00
264.00	59.70	57.86
268.00	60.50	52.15
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014898.D
Acq On : 14 Jun 2021 09:11
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC020

Manual Integrations
APPROVED

mohammad
6/15/2021 2:41:38 PM

Quant Time: Jun 14 10:46:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 14 10:46:06 2021
Response via : Initial Calibration

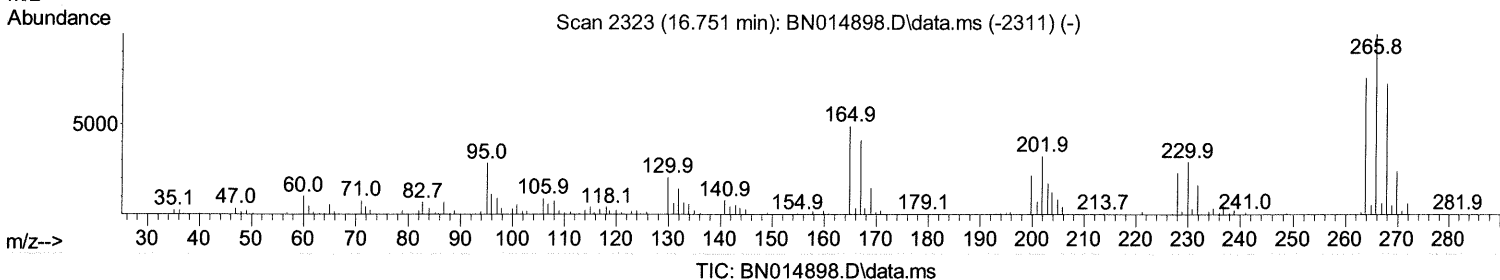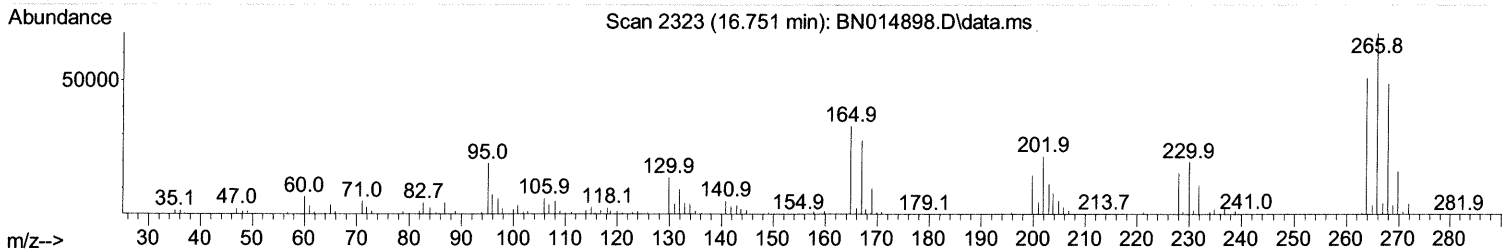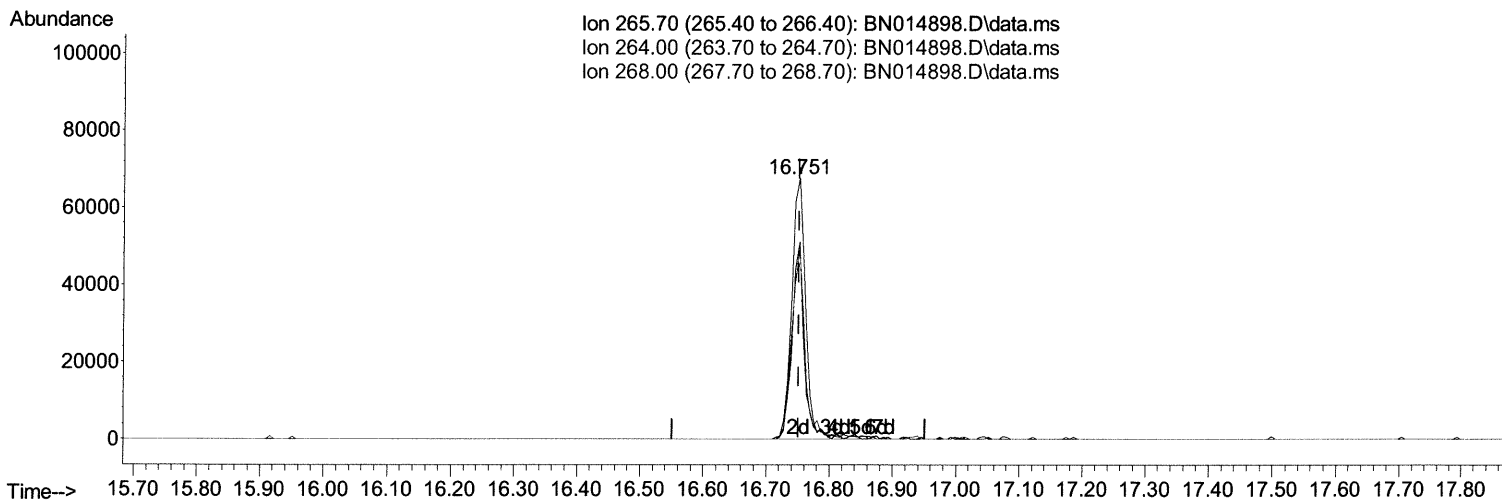

(71) Pentachlorophenol (C)

16.751min (0.000) 20.19 ng/ul m 06/16/21 JU

response 103109

Ion	Exp%	Act%
265.70	100.00	100.00
264.00	59.70	75.46#
268.00	60.50	72.42
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014898.D
Acq On : 14 Jun 2021 09:11
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC020

Manual Integrations
APPROVED

mohammad
6/15/2021 2:41:38 PM

Quant Time: Jun 14 10:46:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 14 10:46:06 2021
Response via : Initial Calibration

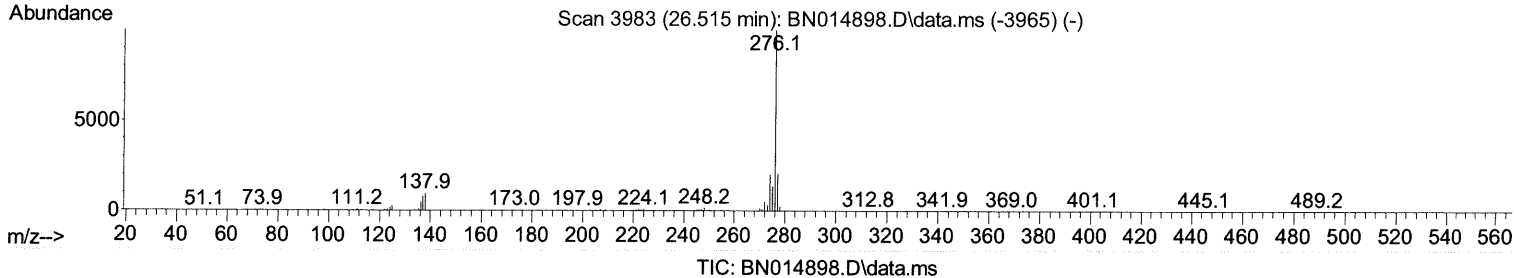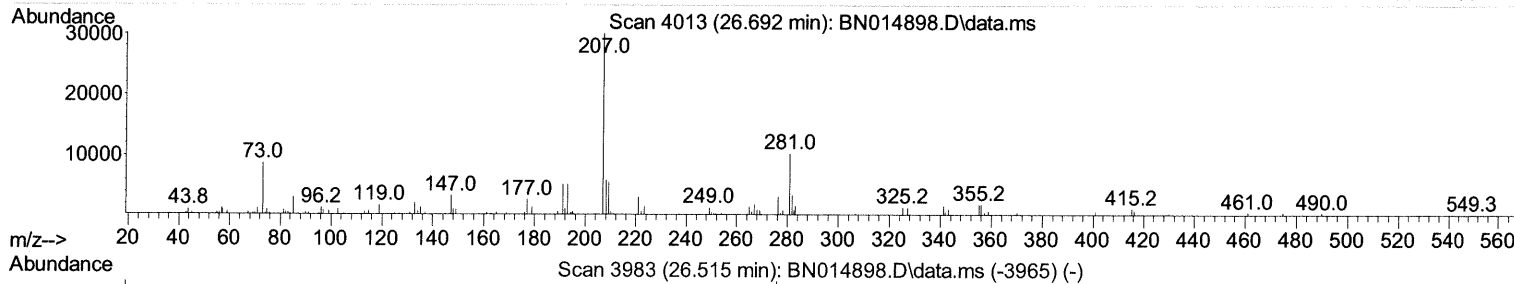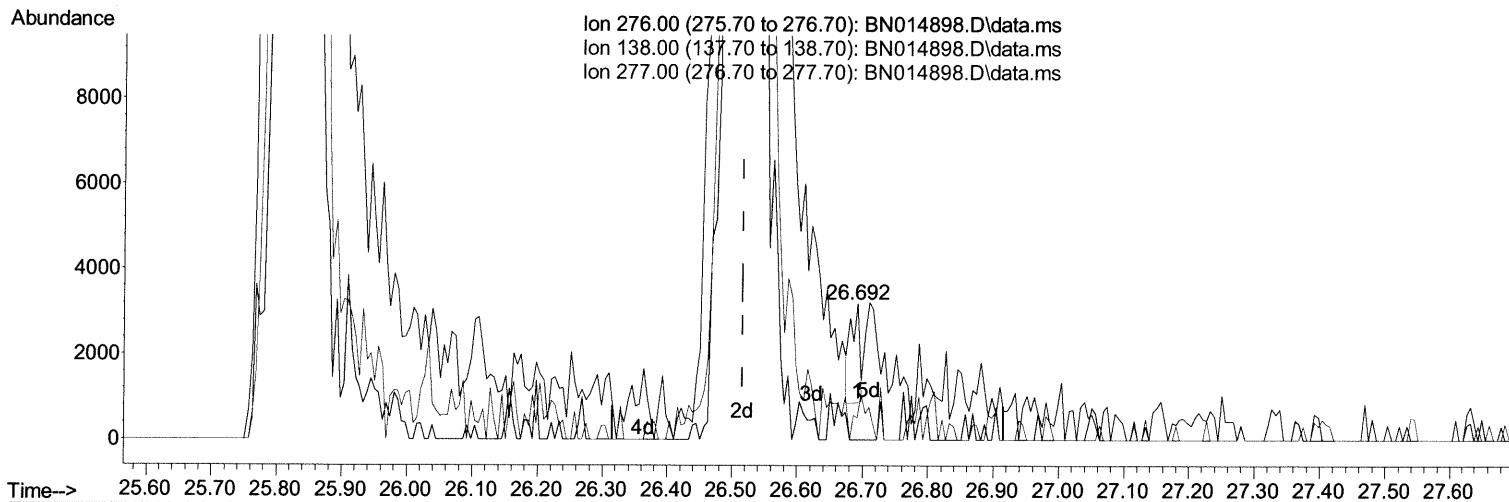

(96) Benzo(g,h,i)perylene

26.692min (+ 0.176) 0.04 ng/ul

response 2225

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	12.80	10.61
277.00	19.60	16.08
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014898.D
Acq On : 14 Jun 2021 09:11
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC020

Manual Integrations
APPROVED

mohammad
6/15/2021 2:41:38 PM

Quant Time: Jun 14 10:46:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 14 10:46:06 2021
Response via : Initial Calibration

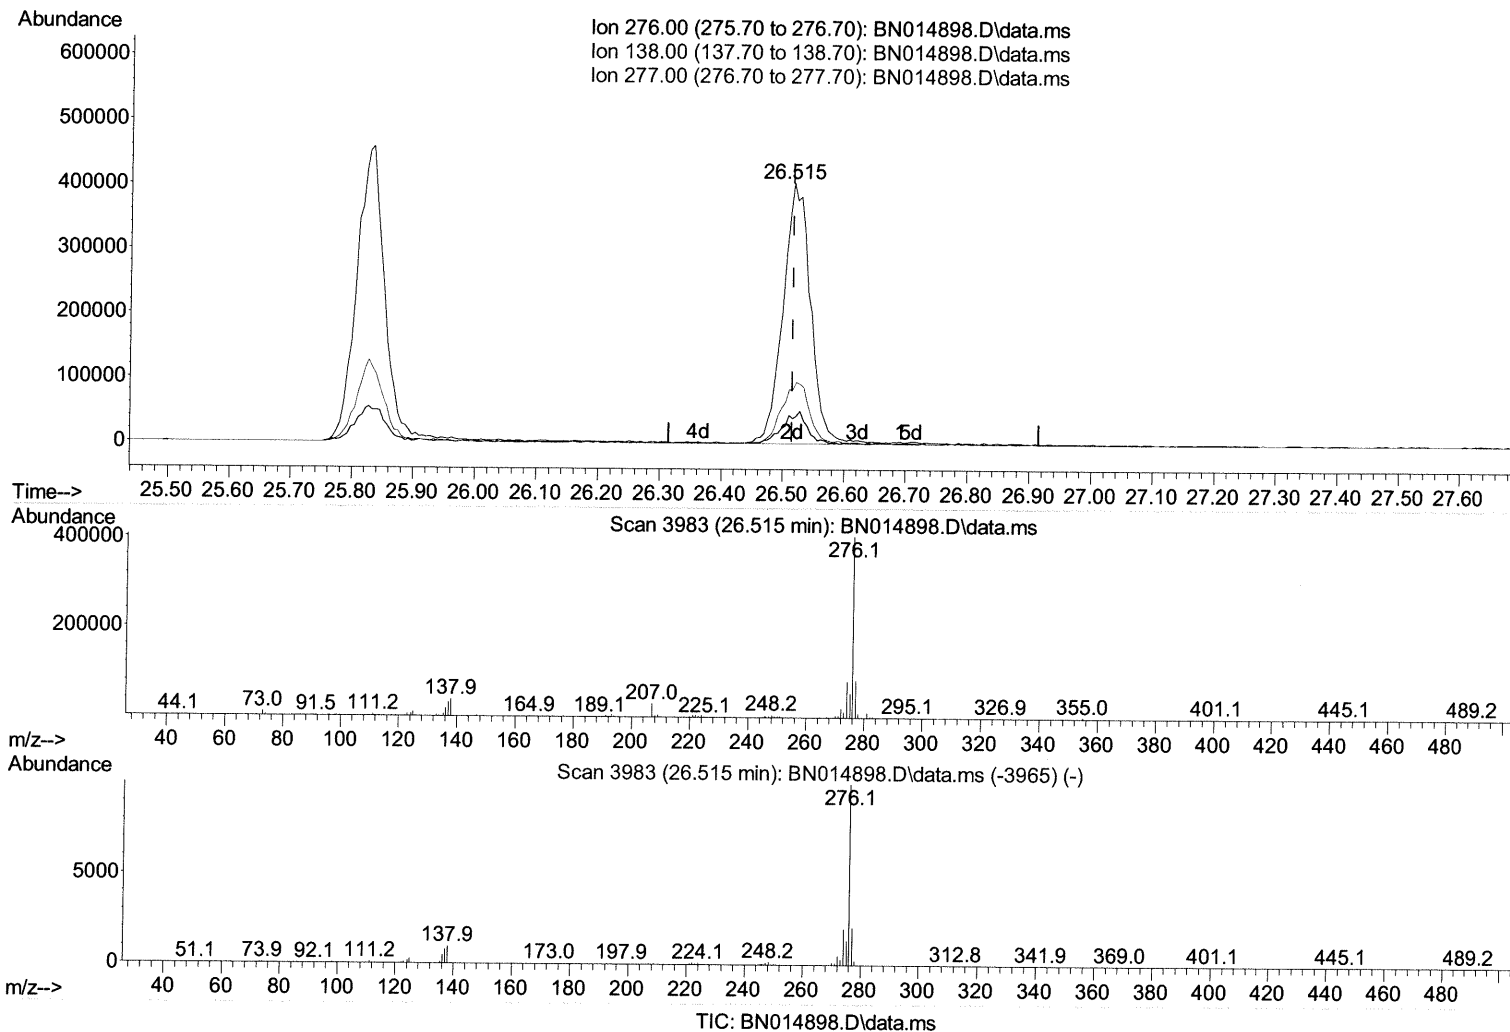

(96) Benzo(g,h,i)perylene

26.515min (0.000) 20.77 ng/ul m 06/16/21 JU

response 1262994

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	12.80	9.52#
277.00	19.60	20.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014898.D
 Acq On : 14 Jun 2021 09:11
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC020

Manual Integrations
 APPROVED

mohammad
 6/15/2021 2:41:38 PM

Quant Time: Jun 14 10:46:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 14 10:46:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.687	152	113610	20.000	ng/ul	0.00
20) Naphthalene-d8	10.475	136	409135	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.340	164	297402	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.098	188	670007	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.298	240	895027	20.000	ng/ul	0.00
88) Perylene-d12	23.551	264	1018494	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	16403	7.678	ng/uL	0.00
4) Pyridine-d5	3.611	84	84792	17.062	ng/ul	0.00
7) Phenol-d5	6.864	99	152732	17.947	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	75725	18.783	ng/ul	0.00
11) 2-Chlorophenol-d4	7.222	132	123269	18.892	ng/ul	0.00
15) 4-Methylphenol-d8	8.399	113	127661	17.603	ng/ul	0.00
21) Nitrobenzene-d5	8.840	128	64587	21.037	ng/ul	0.00
24) 2-Nitrophenol-d4	9.558	143	69742	20.031	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	142358	20.308	ng/ul	0.00
31) 4-Chloroaniline-d4	10.610	131	159710	19.237	ng/ul	0.00
46) Dimethylphthalate-d6	13.751	166	464867	19.662	ng/ul	0.00
49) Acenaphthylene-d8	14.028	160	524113	20.281	ng/ul	0.00
54) 4-Nitrophenol-d4	14.551	143	56462	17.001	ng/ul	0.00
60) Fluorene-d10	15.340	176	393277	20.391	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	75874	18.945	ng/ul	0.00
73) Anthracene-d10	17.192	188	636908	21.005	ng/ul	0.00
81) Pyrene-d10	19.498	212	805774	19.519	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.410	264	1043079	20.492	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.240	88	17531	7.357	ng/ul	90
5) Pyridine	3.628	79	93745	18.187	ng/ul#	79
6) Benzaldehyde	6.834	77	86922	20.324	ng/ul	91
8) Phenol	6.893	94	152642	18.078	ng/ul#	80
10) Bis(2-Chloroethyl)ether	7.116	93	115908	18.192	ng/ul	96
12) 2-Chlorophenol	7.258	128	123213	17.775	ng/ul	92
13) 2-Methylphenol	8.128	108	122910	18.380	ng/ul	94
14) 2,2'-oxybis(1-Chloropr...	8.222	45	76761m	18.516	ng/ul >	06/16/21 JU
16) Acetophenone	8.505	105	225207	19.299	ng/ul	88
17) N-Nitroso-di-n-propyla...	8.493	70	103475	18.761	ng/ul	95
18) 4-Methylphenol	8.463	108	129648	18.021	ng/ul	93
19) Hexachloroethane	8.758	117	63471	17.646	ng/ul	89
22) Nitrobenzene	8.881	77	171221	20.908	ng/ul	96
23) Isophorone	9.405	82	285973	19.362	ng/ul#	93
25) 2-Nitrophenol	9.593	139	68009	19.290	ng/ul#	85
26) 2,4-Dimethylphenol	9.652	107	186393	19.658	ng/ul	91
27) Bis(2-Chloroethoxy)met...	9.893	93	160280	19.841	ng/ul#	93
29) 2,4-Dichlorophenol	10.128	162	138961	20.848	ng/ul	92
30) Naphthalene	10.522	128	401216	19.540	ng/ul	97
32) 4-Chloroaniline	10.634	127	159051	19.402	ng/ul	91
33) Hexachlorobutadiene	10.810	225	142665	21.700	ng/ul	87
34) Caprolactam	11.399	113	35072m	17.040	ng/ul >	06/16/21 JU
35) 4-Chloro-3-methylphenol	11.769	107	174401	20.161	ng/ul	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014898.D
 Acq On : 14 Jun 2021 09:11
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC020

Manual Integrations
 APPROVED

mohammad
 6/15/2021 2:41:38 PM

Quant Time: Jun 14 10:46:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 14 10:46:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
36) 2-Methylnaphthalene	12.146	142	304747	20.242 ng/ul	92
37) 1-Methylnaphthalene	12.363	142	300381	19.762 ng/ul#	97
39) 1,2,4,5-Tetrachloroben...	12.522	216	212294	20.541 ng/ul	96
40) Hexachlorocyclopentadiene	12.499	237	154065	20.109 ng/ul	99
41) 2,4,6-Trichlorophenol	12.763	196	118182	19.706 ng/ul	83
42) 2,4,5-Trichlorophenol	12.840	196	128899	19.542 ng/ul	93
43) 1,1'-Biphenyl	13.169	154	411369	20.136 ng/ul	96
44) 2-Chloronaphthalene	13.204	162	322351	19.757 ng/ul	99
45) 2-Nitroaniline	13.416	65	95860	20.063 ng/ul	97
47) Dimethylphthalate	13.798	163	437618	19.639 ng/ul	96
48) 2,6-Dinitrotoluene	13.916	165	90300	20.917 ng/ul	95
50) Acenaphthylene	14.057	152	464474	19.819 ng/ul	96
51) 3-Nitroaniline	14.246	138	66791	18.709 ng/ul	84
52) Acenaphthene	14.404	153	344212	19.772 ng/ul	96
53) 2,4-Dinitrophenol	14.457	184	42874	18.014 ng/ul	91
55) 4-Nitrophenol	14.569	109	101270	18.276 ng/ul	90
56) Dibenzofuran	14.740	168	503406m	19.847 ng/ul	> 06/16/21 JU
57) 2,4-Dinitrotoluene	14.710	165	144752	21.650 ng/ul	92
58) 2,3,4,6-Tetrachlorophenol	14.969	232	123892	19.892 ng/ul#	94
59) Diethylphthalate	15.175	149	436244	19.264 ng/ul	96
61) Fluorene	15.398	166	410324	20.231 ng/ul	94
62) 4-Chlorophenyl-phenyle...	15.393	204	228514	20.266 ng/ul	89
63) 4-Nitroaniline	15.410	138	64438	18.332 ng/ul	85
66) 4,6-Dinitro-2-methylph...	15.475	198	76329	19.526 ng/ul#	84
67) N-Nitrosodiphenylamine	15.604	169	359922	20.695 ng/ul	98
68) 4-Bromophenyl-phenylether	16.287	248	166068	20.634 ng/ul#	75
69) Hexachlorobenzene	16.404	284	206969	19.856 ng/ul	97
70) Atrazine	16.563	200	160080	20.346 ng/ul	93
71) Pentachlorophenol	16.751	266	103109m	20.191 ng/ul	> 06/16/21 JU
72) Phenanthrene	17.139	178	693829	20.691 ng/ul	98
74) Anthracene	17.228	178	708823	20.951 ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.128	216	208792	20.520 ng/ul	96
76) Pentachlorobenzene	14.663	250	229386	20.479 ng/ul	98
77) Carbazole	17.498	167	588180	20.802 ng/ul	94
78) Di-n-butylphthalate	18.075	149	745607	21.132 ng/ul	97
80) Fluoranthene	19.163	202	920177	19.396 ng/ul#	93
82) Pyrene	19.528	202	970420	19.288 ng/ul#	94
83) Butylbenzylphthalate	20.439	149	354101	19.098 ng/ul	93
84) 3,3'-Dichlorobenzidine	21.222	252	343346	20.933 ng/ul	97
85) Benzo(a)anthracene	21.280	228	1032721	19.699 ng/ul	94
86) Bis(2-ethylhexyl)phtha...	21.222	149	552095	20.212 ng/ul	98
87) Chrysene	21.333	228	1068479	20.566 ng/ul	96
89) Di-n-octyl phthalate	22.104	149	1033209	19.430 ng/ul	100
90) Benzo(b)fluoranthene	22.874	252	1253736	21.185 ng/ul	99
91) Benzo(k)fluoranthene	22.922	252	1186518	20.395 ng/ul	96
93) Benzo(a)pyrene	23.457	252	1107132	20.598 ng/ul	97
94) Indeno(1,2,3-cd)pyrene	25.833	276	1445222	20.875 ng/ul	98
95) Dibenzo(a,h)anthracene	25.839	278	1186476	20.939 ng/ul	99
96) Benzo(g,h,i)perylene	26.515	276	1262994m	20.773 ng/ul	> 06/16/21 JU

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
BNA_N
LabSampleId :
SSTDCCC020

Manual Integrations
APPROVED

mohammad
6/15/2021 2:41:38 PM