

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014908.D
 Acq On : 14 Jun 2021 21:03
 Operator : CG/JU
 Sample : M2649-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 B0AA7

Manual Integrations
 APPROVED

mohammad
 6/15/2021 2:42:13 PM

Quant Time: Jun 15 02:04:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 14 10:46:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.687	152	91218	20.00	ng/ul	0.00
20) Naphthalene-d8	10.475	136	334683	20.00	ng/ul	# 0.00
38) Acenaphthene-d10	14.340	164	234114	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.092	188	575546	20.00	ng/ul	# 0.00
79) Chrysene-d12	21.292	240	733270	20.00	ng/ul	0.00
88) Perylene-d12	23.545	264	811553	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.211	96	9018	5.26	ng/uL	0.00
4) Pyridine-d5	3.623	84	26897m	6.74	ng/ul	0.01
7) Phenol-d5	6.864	99	124751	18.26	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	137023	42.33	ng/ul	0.00
11) 2-Chlorophenol-d4	7.222	132	190684	36.40	ng/ul	0.00
15) 4-Methylphenol-d8	8.393	113	162974	27.99	ng/ul	0.00
21) Nitrobenzene-d5	8.840	128	110077	43.83	ng/ul	0.00
24) 2-Nitrophenol-d4	9.557	143	118782	41.71	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	224688	39.18	ng/ul	0.00
31) 4-Chloroaniline-d4	10.610	131	222087	32.70	ng/ul	0.00
46) Dimethylphthalate-d6	13.751	166	877946	47.17	ng/ul	0.00
49) Acenaphthylene-d8	14.034	160	945751	46.49	ng/ul	0.00
54) 4-Nitrophenol-d4	14.557	143	32247	12.33	ng/ul	0.00
60) Fluorene-d10	15.340	176	711095	46.84	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.463	200	134333	39.05	ng/ul	0.00
73) Anthracene-d10	17.192	188	1197914	45.99	ng/ul	0.00
81) Pyrene-d10	19.498	212	1514373	44.78	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.404	264	1958759	48.29	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.798	163	20436	1.17	ng/ul#	Qvalue 78

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014908.D
Acq On : 14 Jun 2021 21:03
Operator : CG/JU
Sample : M2649-11
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
B0AA7

Manual Integrations
APPROVED

mohammad
6/15/2021 2:42:13 PM

Quant Time: Jun 15 02:04:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 14 10:46:06 2021
Response via : Initial Calibration

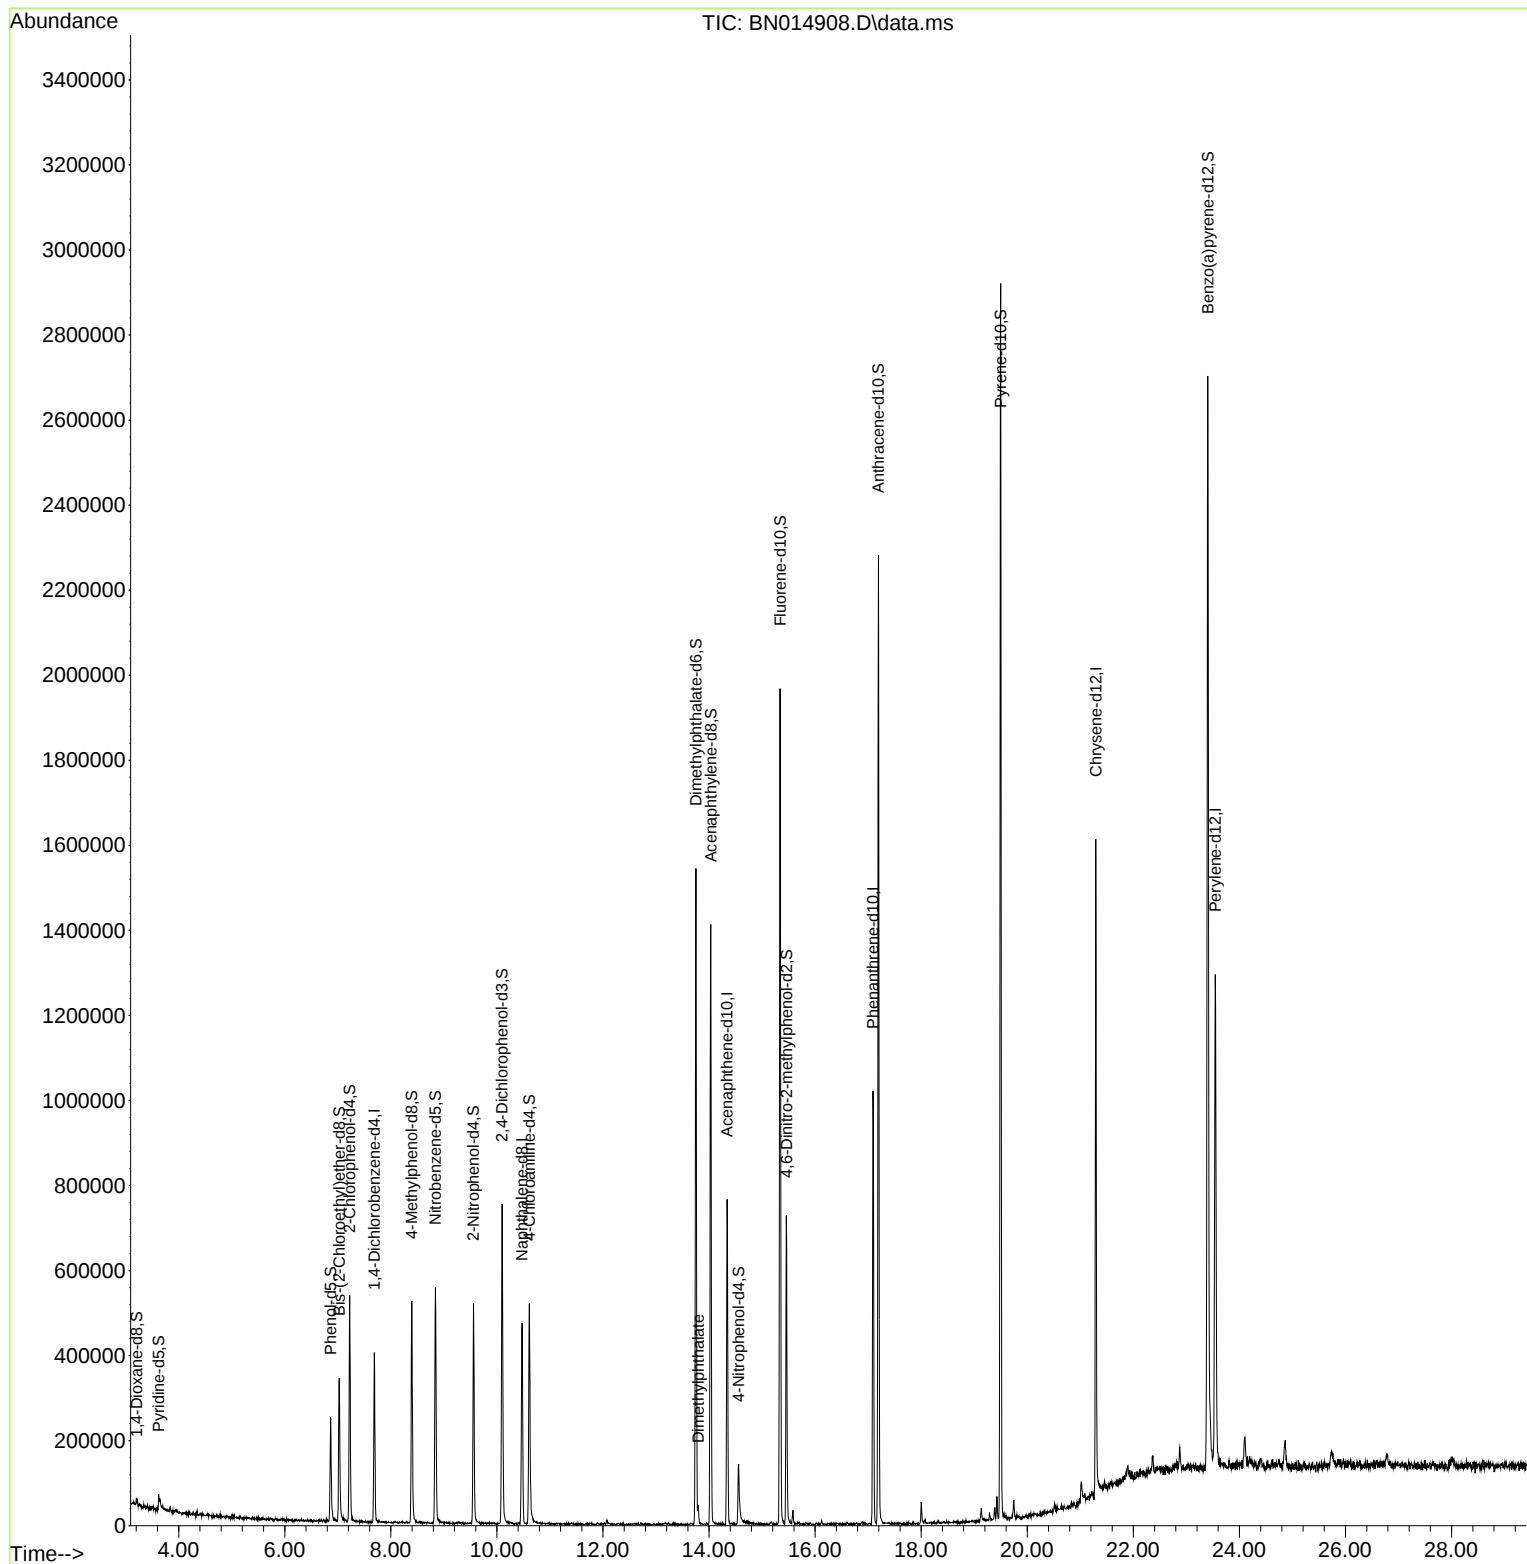

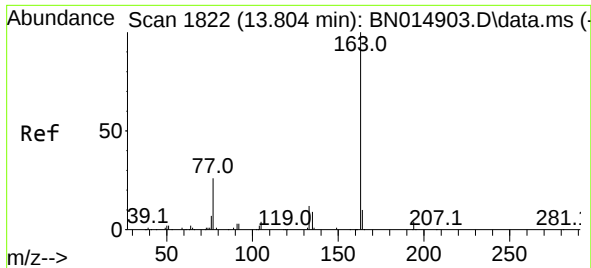

#47
 Dimethylphthalate
 Concen: 1.17 ng/ul
 RT: 13.798 min Scan# 1821
 Delta R.T. -0.000 min
 Lab File: BN014908.D
 Acq: 14 Jun 2021 21:03

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.8	5.8
164	23.1	8.7	13.1#

Instrument :
 BNA_N
 ClientSampleId :
 B0AA7

Manual Integrations
 APPROVED

mohammad
 6/15/2021 2:42:13 PM

