

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014920.D
 Acq On : 15 Jun 2021 10:40
 Operator : CG/JU
 Sample : M2649-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 B0AA9

Manual Integrations
 APPROVED

mohammad
 6/15/2021 2:42:21 PM

Quant Time: Jun 15 11:25:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 14 10:46:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.687	152	107896	20.000	ng/ul	0.00
20) Naphthalene-d8	10.469	136	375404	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.339	164	293260	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.092	188	675840	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.298	240	884153	20.000	ng/ul	0.00
88) Perylene-d12	23.551	264	970143	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.211	96	14106	6.952	ng/uL	0.00
4) Pyridine-d5	3.622	84	38305	8.116	ng/ul	0.01
7) Phenol-d5	6.863	99	95977	11.875	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.022	67	143724	37.538	ng/ul	0.00
11) 2-Chlorophenol-d4	7.222	132	198528	32.037	ng/ul	0.00
15) 4-Methylphenol-d8	8.393	113	162580	23.606	ng/ul	0.00
21) Nitrobenzene-d5	8.840	128	124660	44.253	ng/ul	0.00
24) 2-Nitrophenol-d4	9.563	143	131439	41.144	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	238309	37.050	ng/ul	0.00
31) 4-Chloroaniline-d4	10.610	131	239362	31.422	ng/ul	0.00
46) Dimethylphthalate-d6	13.751	166	921490	39.526	ng/ul	0.00
49) Acenaphthylene-d8	14.028	160	1048754	41.156	ng/ul	0.00
54) 4-Nitrophenol-d4	14.551	143	24662m	7.531	ng/ul	0.00
60) Fluorene-d10	15.339	176	767762	40.370	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	144912	35.871	ng/ul	0.00
73) Anthracene-d10	17.192	188	1268011	41.457	ng/ul	0.00
81) Pyrene-d10	19.498	212	1606601	39.396	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.410	264	1997895	41.207	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.798	163	39960	1.819	ng/ul#	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014920.D
Acq On : 15 Jun 2021 10:40
Operator : CG/JU
Sample : M2649-14
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
B0AA9

Manual Integrations
APPROVED

mohammad
6/15/2021 2:42:21 PM

Quant Time: Jun 15 11:25:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 14 10:46:06 2021
Response via : Initial Calibration

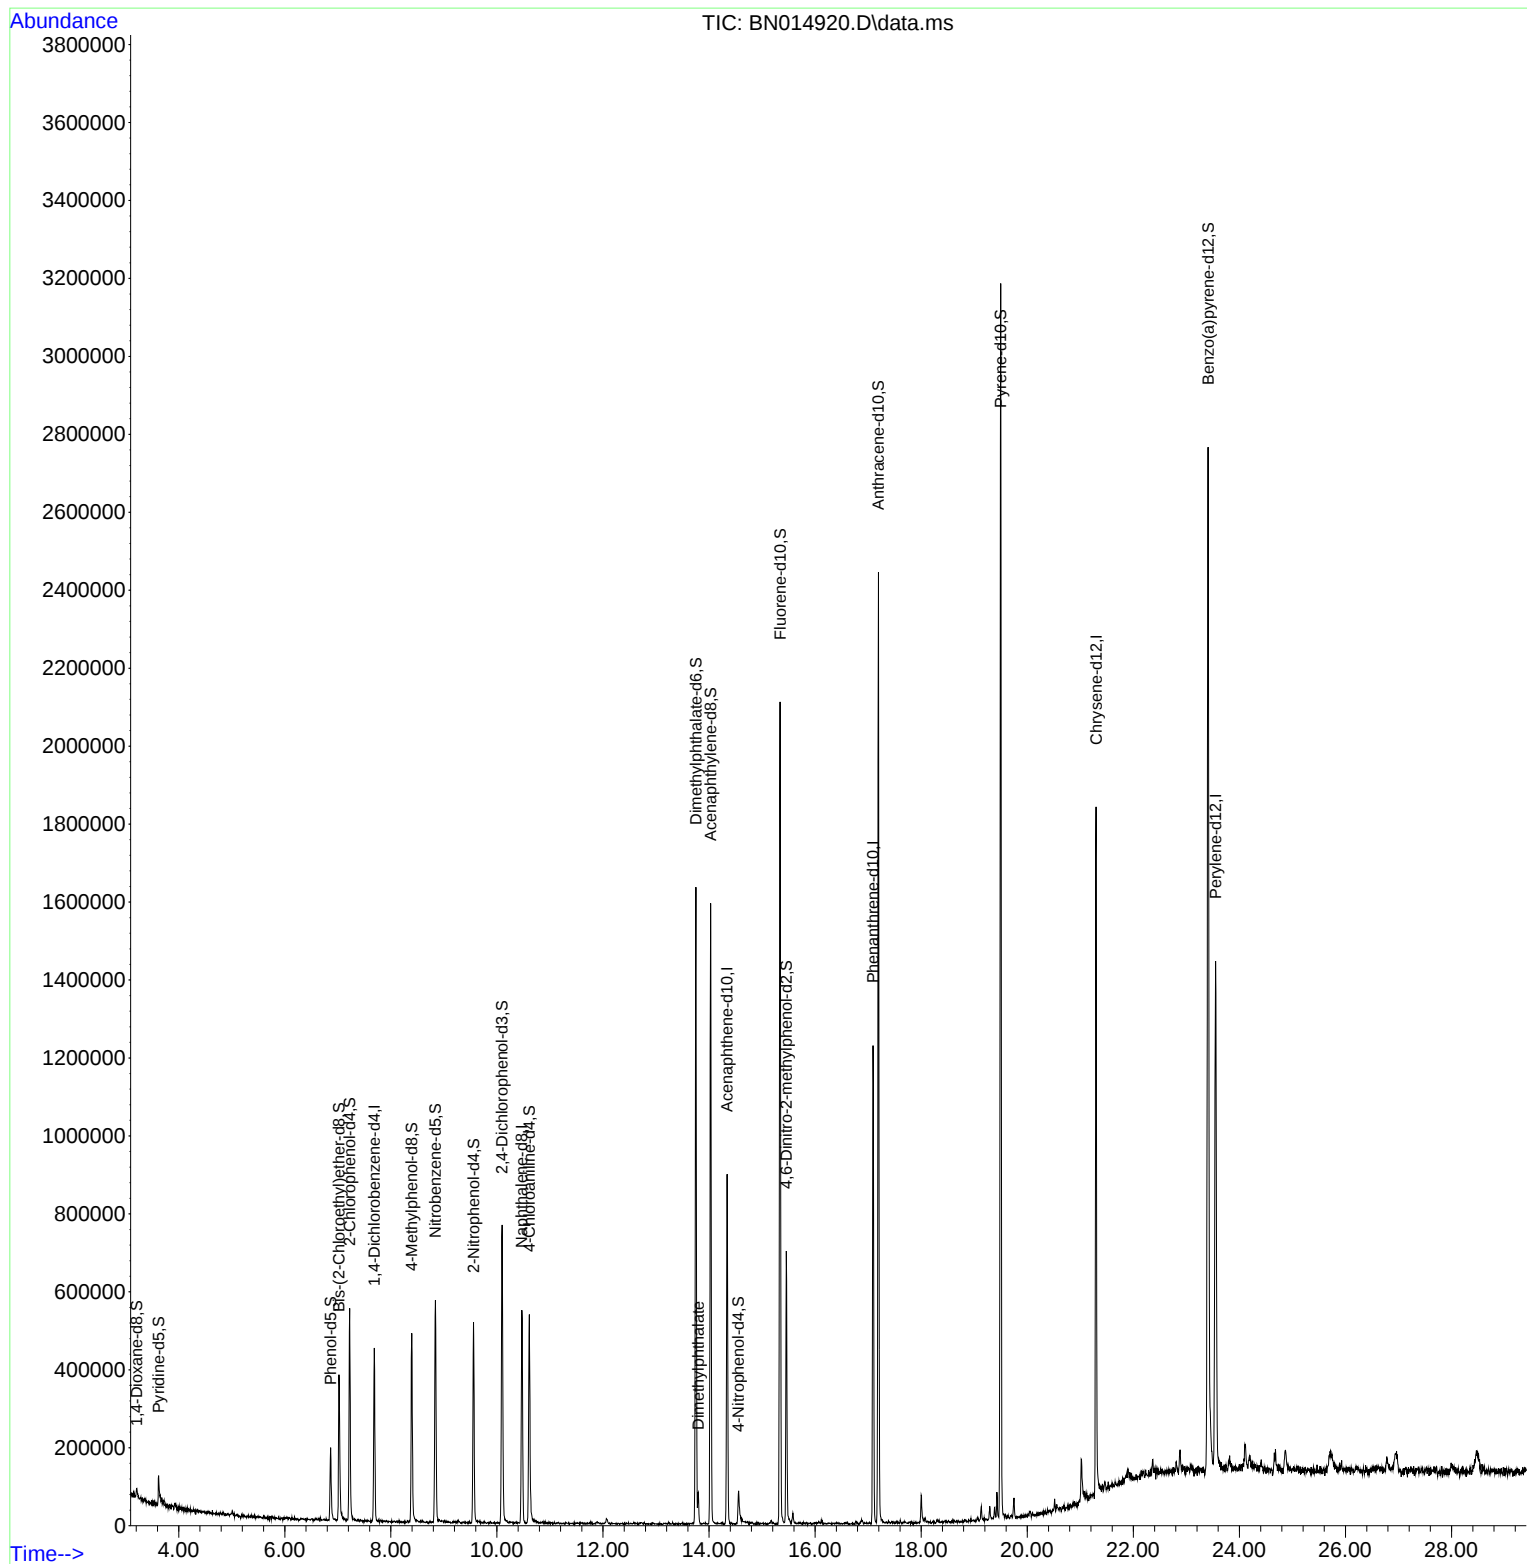

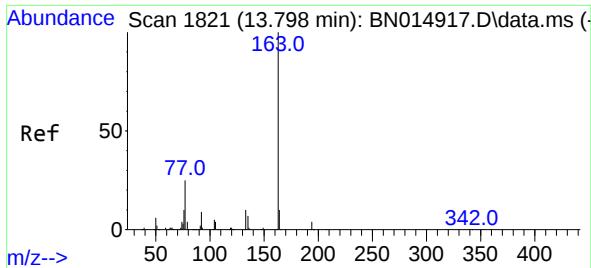

#47
Dimethylphthalate
Concen: 1.819 ng/ul
RT: 13.798 min Scan# 1821
Delta R.T. -0.000 min
Lab File: BN014920.D
Acq: 15 Jun 2021 10:40

Tgt Ion:163 Resp: 39960
Ion Ratio Lower Upper
163 100
194 5.8 3.8 5.8#
164 13.3 8.7 13.1#

Instrument :
BNA_N
ClientSampleId :
B0AA9

Manual Integrations
APPROVED

mohammad
6/15/2021 2:42:21 PM

