

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014899.D
 Acq On : 14 Jun 2021 09:56
 Operator : CG/JU
 Sample : PB137047BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK047

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	10	12	14	rVB3	10005	5896	0.10%	0.012%
2	3.211	17	21	26	rBV6	36774	54535	0.93%	0.115%
3	3.328	38	41	42	rBV2	8869	9645	0.16%	0.020%
4	3.522	72	74	77	rBV3	8942	7630	0.13%	0.016%
5	3.611	85	89	96	rBV	298571	502006	8.52%	1.060%
6	3.799	119	121	123	rVB	9270	6703	0.11%	0.014%
7	3.822	123	125	127	rVB3	8475	6811	0.12%	0.014%
8	4.252	196	198	201	rVB4	10732	9823	0.17%	0.021%
9	4.493	237	239	243	rVB4	6959	7248	0.12%	0.015%
10	4.799	288	291	295	rVB4	8020	11162	0.19%	0.024%
11	5.663	436	438	441	rVB4	6225	6548	0.11%	0.014%
12	5.763	453	455	459	rVB4	4144	5982	0.10%	0.013%
13	6.163	521	523	528	rBV4	6306	8263	0.14%	0.017%
14	6.599	595	597	599	rBV2	5849	6007	0.10%	0.013%
15	6.752	621	623	627	rVB3	6027	6312	0.11%	0.013%
16	6.869	636	643	654	rBV	624165	1042597	17.70%	2.202%
17	7.028	661	670	681	rBV	406268	688300	11.69%	1.454%
18	7.110	683	684	687	rBV2	6162	7302	0.12%	0.015%
19	7.228	698	704	714	rBV	703607	1150316	19.53%	2.430%
20	7.693	775	783	795	rVB2	550856	869588	14.76%	1.837%
21	8.081	846	849	851	rBV3	5870	6364	0.11%	0.013%
22	8.399	896	903	912	rBV2	819615	1373524	23.32%	2.901%
23	8.728	956	959	960	rVB2	7184	5976	0.10%	0.013%
24	8.840	972	978	990	rBV	648010	1125760	19.11%	2.378%
25	8.981	1000	1002	1005	rBV4	4945	6070	0.10%	0.013%
26	9.563	1094	1101	1113	rBV	610270	1011042	17.17%	2.135%
27	10.104	1184	1193	1202	rBV	882252	1544067	26.22%	3.261%
28	10.475	1248	1256	1264	rBV	646529	1087952	18.47%	2.298%
29	10.616	1272	1280	1293	rBV	730960	1385004	23.52%	2.925%
30	10.810	1310	1313	1316	rBV2	4795	6077	0.10%	0.013%
31	12.081	1524	1529	1533	rVV5	15446	26153	0.44%	0.055%
32	12.693	1629	1633	1636	rBV3	6586	7944	0.13%	0.017%
33	13.328	1735	1741	1745	rBV4	3918	6943	0.12%	0.015%
34	13.757	1807	1814	1822	rBV	1709423	2527843	42.92%	5.339%
35	14.034	1853	1861	1873	rBV	1718273	2628714	44.63%	5.552%
36	14.345	1906	1914	1920	rBV	1115660	1573128	26.71%	3.323%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014899.D
 Acq On : 14 Jun 2021 09:56
 Operator : CG/JU
 Sample : PB137047BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK047

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

37	14.557	1943	1950	1963	rBV	610830	1013903	17.22%	2.142%
38	14.834	1993	1997	2001	rBV4	3576	7607	0.13%	0.016%
39	15.339	2076	2083	2091	rBV	2262782	3367728	57.18%	7.113%
40	15.463	2098	2104	2114	rBV2	821749	1138577	19.33%	2.405%
41	15.581	2119	2124	2129	rVV3	34429	50732	0.86%	0.107%
42	15.916	2177	2181	2184	rVB2	4405	8012	0.14%	0.017%
43	16.128	2215	2217	2221	rVB4	12508	13712	0.23%	0.029%
44	16.886	2342	2346	2350	rBV5	8753	15109	0.26%	0.032%
45	17.098	2375	2382	2392	rVV	1481743	2066097	35.08%	4.364%
46	17.198	2392	2399	2412	rVV	2643641	3879762	65.87%	8.195%
47	17.292	2412	2415	2419	rVB5	5814	7464	0.13%	0.016%
48	18.075	2541	2548	2550	rBV4	4802	7092	0.12%	0.015%
49	18.451	2609	2612	2615	rBV4	4863	6879	0.12%	0.015%
50	19.069	2714	2717	2719	rVB3	8078	8131	0.14%	0.017%
51	19.133	2719	2728	2734	rBV6	33614	63239	1.07%	0.134%
52	19.345	2762	2764	2767	rBV3	6804	7884	0.13%	0.017%
53	19.386	2767	2771	2775	rBV2	28350	35050	0.60%	0.074%
54	19.504	2779	2791	2800	rBV2	3362957	4859966	82.52%	10.265%
55	19.669	2817	2819	2822	rVV3	5592	6498	0.11%	0.014%
56	19.698	2822	2824	2826	rVB3	9057	7355	0.12%	0.016%
57	19.733	2826	2830	2832	rBV3	4610	6165	0.10%	0.013%
58	19.839	2847	2848	2851	rBV3	6617	7592	0.13%	0.016%
59	19.951	2866	2867	2871	rVB4	7000	6969	0.12%	0.015%
60	20.110	2891	2894	2897	rBV5	8352	10620	0.18%	0.022%
61	20.186	2906	2907	2913	rBV6	6592	7973	0.14%	0.017%
62	20.233	2913	2915	2918	rVB2	9728	9669	0.16%	0.020%
63	20.263	2918	2920	2922	rBV3	8388	9858	0.17%	0.021%
64	20.280	2922	2923	2926	rBV3	9198	6024	0.10%	0.013%
65	20.333	2930	2932	2938	rVB6	7759	13077	0.22%	0.028%
66	20.422	2944	2947	2949	rBV3	6430	7936	0.13%	0.017%
67	20.510	2960	2962	2966	rBV4	8129	9250	0.16%	0.020%
68	20.786	3007	3009	3010	rBV	8789	7264	0.12%	0.015%
69	20.821	3014	3015	3018	rBV3	11597	11470	0.19%	0.024%
70	21.033	3049	3051	3052	rVB2	15691	8090	0.14%	0.017%
71	21.086	3058	3060	3061	rBV2	15756	9104	0.15%	0.019%
72	21.298	3091	3096	3108	rBV2	1916920	2834821	48.13%	5.988%
73	21.751	3171	3173	3174	rBV2	16046	8543	0.15%	0.018%
74	23.415	3448	3456	3470	rBV2	2907837	5889648	100.00%	12.440%
75	23.557	3473	3480	3492	rVB	1509664	3096941	52.58%	6.541%
76	24.862	3700	3702	3705	rBV4	31041	34798	0.59%	0.073%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014899.D
Acq On : 14 Jun 2021 09:56
Operator : CG/JU
Sample : PB137047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK047

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Title : SVOA CALIBRATION

77	28.950	4395	4397	4399	rBV3	22669	20115	0.34%	0.042%
78	29.086	4418	4420	4422	rBV3	26427	23077	0.39%	0.049%




Sum of corrected areas: 47345036

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014899.D
Acq On : 14 Jun 2021 09:56
Operator : CG/JU
Sample : PB137047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK047

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

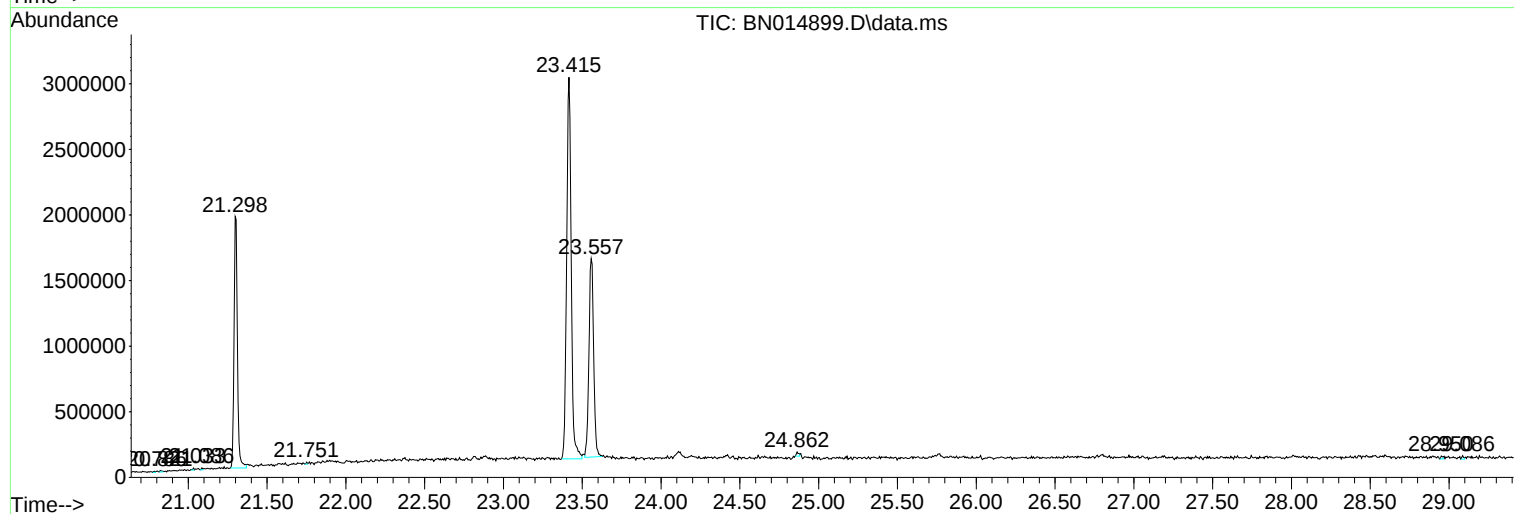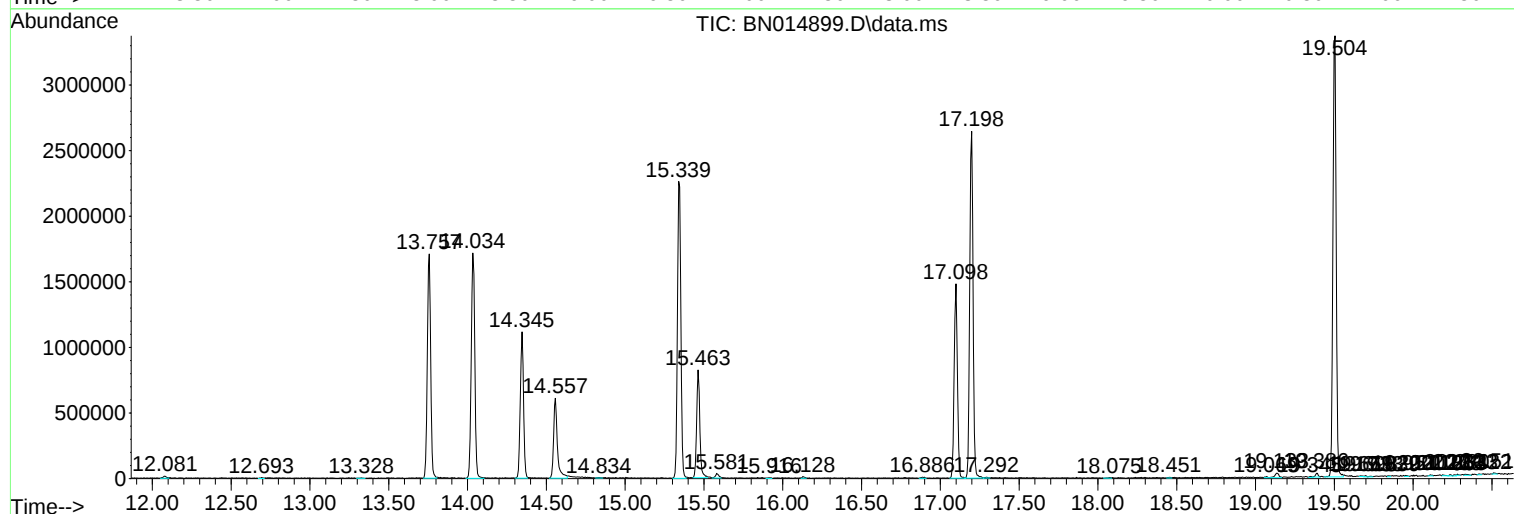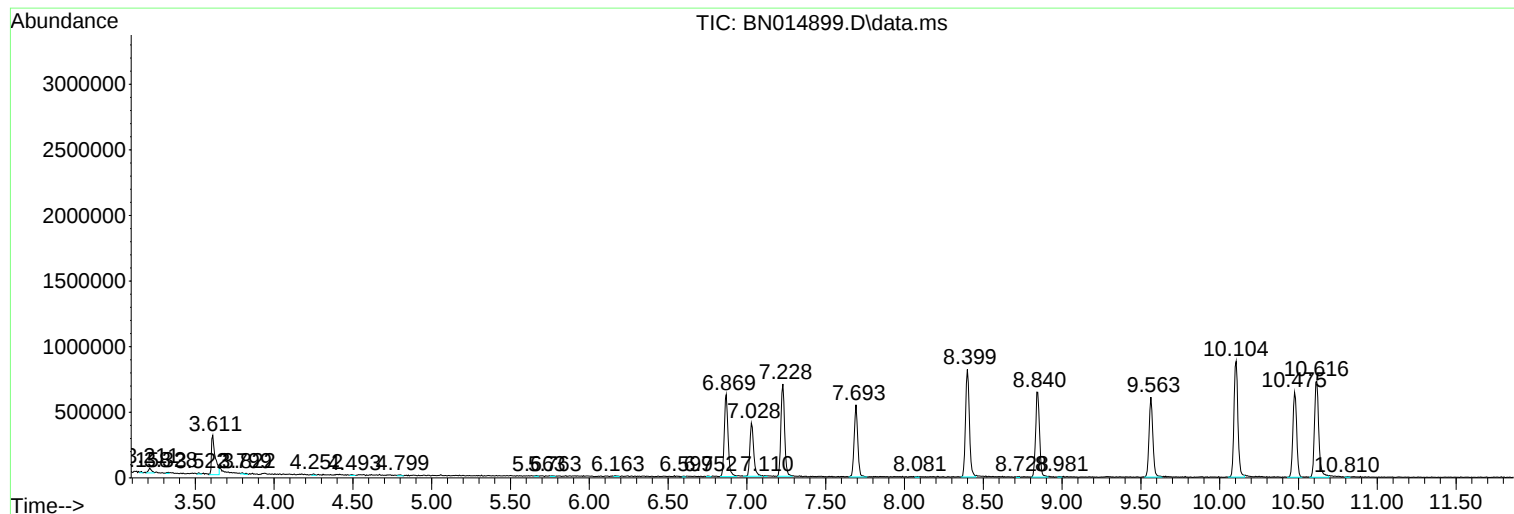

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014899.D
Acq On : 14 Jun 2021 09:56
Operator : CG/JU
Sample : PB137047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK047

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014899.D
Acq On : 14 Jun 2021 09:56
Operator : CG/JU
Sample : PB137047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK047

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
