

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014904.D
 Acq On : 14 Jun 2021 18:39
 Operator : CG/JU
 Sample : PB137065BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK065

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.605	85	88	102	rBV	189763	342415	8.47%	1.064%
2	4.328	209	211	212	rBV2	8282	4748	0.12%	0.015%
3	4.605	256	258	260	rBV3	8262	8512	0.21%	0.026%
4	5.540	414	417	420	rVB4	7997	10471	0.26%	0.033%
5	5.916	478	481	482	rBV2	5839	6100	0.15%	0.019%
6	6.193	526	528	530	rVB3	6116	4782	0.12%	0.015%
7	6.863	637	642	650	rBV	428996	667178	16.51%	2.072%
8	7.028	664	670	681	rVB	265078	454562	11.25%	1.412%
9	7.222	697	703	712	rVV	478388	785273	19.43%	2.439%
10	7.287	712	714	718	rVB4	6106	6465	0.16%	0.020%
11	7.687	776	782	789	rBV	397800	649288	16.07%	2.017%
12	8.028	837	840	844	rVB4	4371	6472	0.16%	0.020%
13	8.393	896	902	918	rBV	547389	917418	22.70%	2.850%
14	8.534	924	926	930	rVB4	4743	4469	0.11%	0.014%
15	8.769	963	966	971	rVB4	5104	7755	0.19%	0.024%
16	8.840	971	978	987	rBV	448726	758442	18.77%	2.356%
17	9.110	1022	1024	1027	rVB2	4507	4668	0.12%	0.014%
18	9.157	1027	1032	1033	rBV3	3380	5042	0.12%	0.016%
19	9.557	1093	1100	1115	rBV2	393796	681187	16.86%	2.116%
20	9.793	1137	1140	1144	rVB2	3710	5522	0.14%	0.017%
21	10.099	1186	1192	1202	rBV2	580507	997342	24.68%	3.098%
22	10.475	1249	1256	1263	rBV	474380	811742	20.09%	2.521%
23	10.610	1273	1279	1289	rBV	514523	918864	22.74%	2.854%
24	10.828	1315	1316	1320	rVB2	3979	4887	0.12%	0.015%
25	11.040	1348	1352	1355	rVB4	3096	4492	0.11%	0.014%
26	11.416	1414	1416	1421	rBV3	3881	5487	0.14%	0.017%
27	12.075	1524	1528	1531	rBV3	5717	8304	0.21%	0.026%
28	13.304	1734	1737	1740	rVB2	3547	4572	0.11%	0.014%
29	13.751	1806	1813	1826	rBV	1160881	1666086	41.23%	5.175%
30	14.034	1854	1861	1873	rBV	1190908	1750235	43.31%	5.437%
31	14.340	1906	1913	1920	rBV	776321	1132606	28.03%	3.518%
32	14.410	1923	1925	1929	rVB2	5129	4803	0.12%	0.015%
33	14.551	1943	1949	1966	rBV	314157	593438	14.69%	1.843%
34	14.663	1966	1968	1973	rVV3	10835	16675	0.41%	0.052%
35	14.704	1973	1975	1977	rVB2	6338	5221	0.13%	0.016%
36	14.869	1999	2003	2004	rBV3	5068	4767	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014904.D
 Acq On : 14 Jun 2021 18:39
 Operator : CG/JU
 Sample : PB137065BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK065

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

37	14.898	2004	2008	2011	rVB3	3401	5179	0.13%	0.016%
38	15.340	2077	2083	2091	rBV	1531781	2230908	55.21%	6.930%
39	15.457	2097	2103	2113	rBV	490531	702567	17.39%	2.182%
40	15.587	2121	2125	2129	rVB4	22933	30160	0.75%	0.094%
41	15.728	2146	2149	2151	rVB2	4842	4531	0.11%	0.014%
42	15.751	2151	2153	2156	rVB2	4040	4451	0.11%	0.014%
43	15.798	2156	2161	2163	rBV	4886	6162	0.15%	0.019%
44	16.128	2212	2217	2221	rVB3	8224	15049	0.37%	0.047%
45	16.257	2236	2239	2243	rBV3	3586	5087	0.13%	0.016%
46	16.369	2256	2258	2261	rBV2	4425	4884	0.12%	0.015%
47	16.763	2324	2325	2330	rBV	5445	5440	0.13%	0.017%
48	16.886	2342	2346	2349	rBV3	6284	7484	0.19%	0.023%
49	16.986	2356	2363	2364	rBV2	3478	6292	0.16%	0.020%
50	17.092	2375	2381	2388	rBV2	1019999	1518759	37.58%	4.718%
51	17.192	2392	2398	2412	rVB	1722916	2537934	62.80%	7.883%
52	18.045	2542	2543	2545	rBV	6185	4537	0.11%	0.014%
53	18.175	2560	2565	2566	rBV2	4694	5392	0.13%	0.017%
54	18.222	2569	2573	2576	rVV2	4483	5567	0.14%	0.017%
55	18.692	2650	2653	2654	rBV2	6536	5439	0.13%	0.017%
56	18.775	2663	2667	2669	rBV4	7885	8444	0.21%	0.026%
57	18.845	2674	2679	2682	rVB4	5042	6132	0.15%	0.019%
58	18.869	2682	2683	2686	rBV	4515	4827	0.12%	0.015%
59	19.033	2708	2711	2712	rBV3	5097	4669	0.12%	0.015%
60	19.086	2718	2720	2724	rVB4	4295	4791	0.12%	0.015%
61	19.128	2724	2727	2732	rBV3	25412	40478	1.00%	0.126%
62	19.204	2737	2740	2741	rBV2	4940	4514	0.11%	0.014%
63	19.380	2766	2770	2774	rBV5	17661	24652	0.61%	0.077%
64	19.498	2784	2790	2801	rBV	2322286	3253225	80.50%	10.105%
65	19.616	2809	2810	2817	rVB4	8693	13566	0.34%	0.042%
66	19.816	2843	2844	2848	rBV2	8233	6685	0.17%	0.021%
67	20.010	2876	2877	2879	rBV2	9155	5186	0.13%	0.016%
68	20.033	2879	2881	2884	rVV3	6028	5455	0.13%	0.017%
69	21.292	3090	3095	3109	rBV	1520289	2148168	53.16%	6.673%
70	23.404	3447	3454	3468	rBV2	2044488	4041077	100.00%	12.552%
71	23.551	3472	3479	3488	rVB3	1161208	2255764	55.82%	7.007%




Sum of corrected areas: 32193745

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014904.D
Acq On : 14 Jun 2021 18:39
Operator : CG/JU
Sample : PB137065BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK065

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

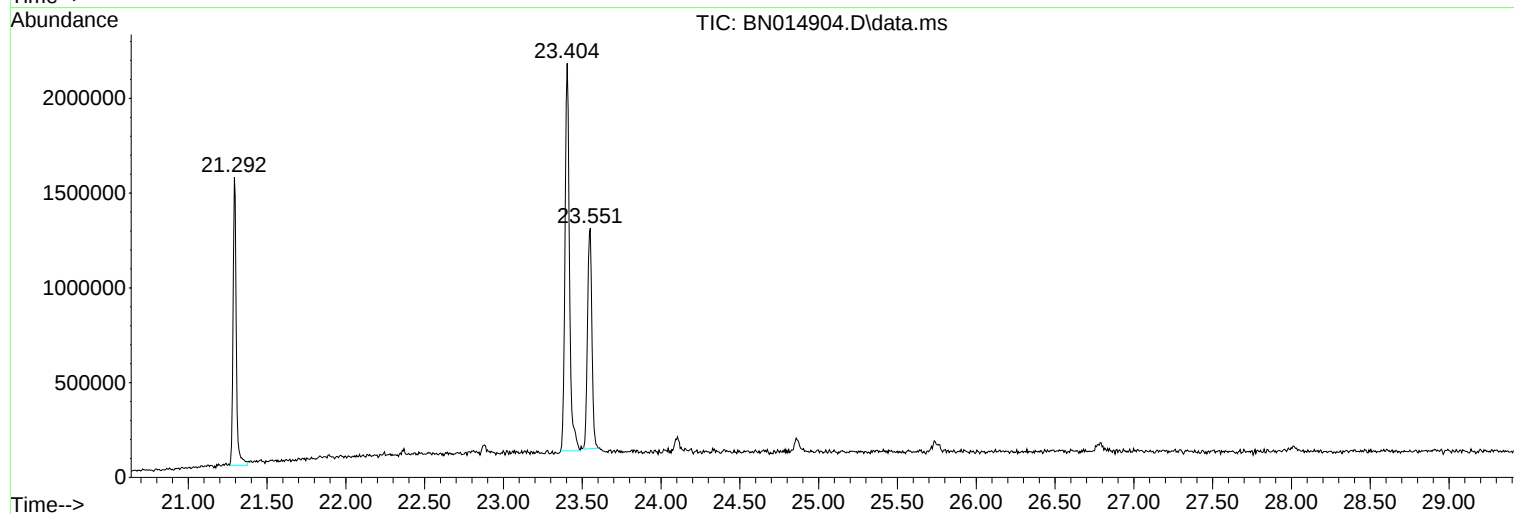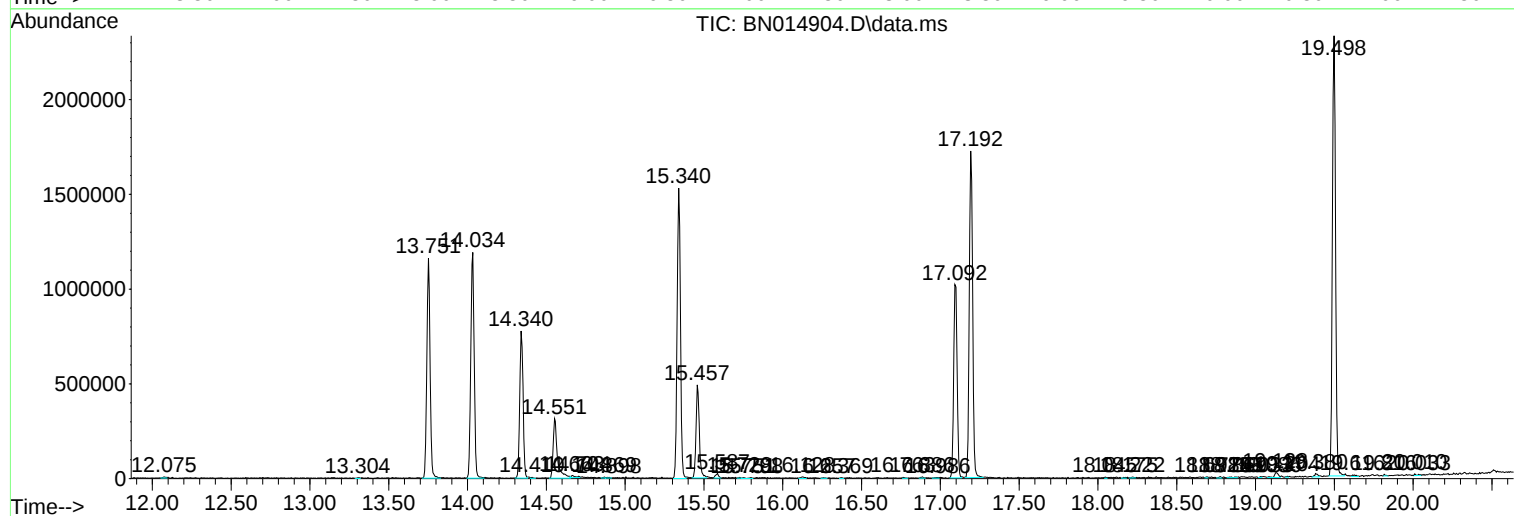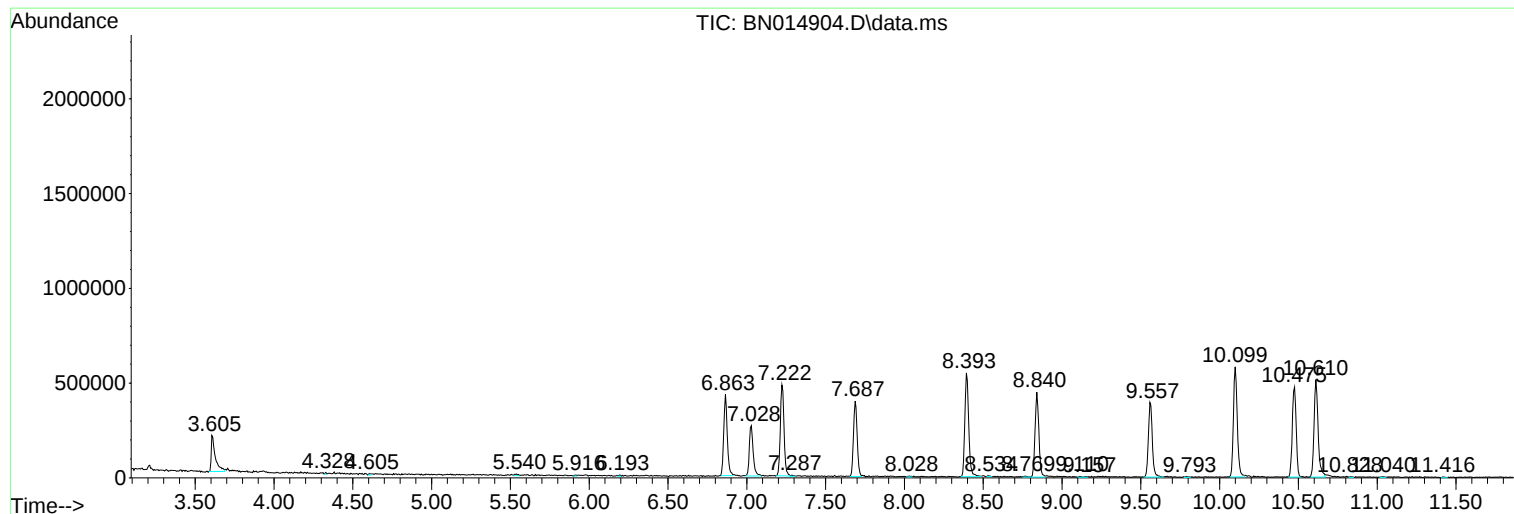

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014904.D
Acq On : 14 Jun 2021 18:39
Operator : CG/JU
Sample : PB137065BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK065

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014904.D
Acq On : 14 Jun 2021 18:39
Operator : CG/JU
Sample : PB137065BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK065

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
