

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014908.D
 Acq On : 14 Jun 2021 21:03
 Operator : CG/JU
 Sample : M2649-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 B0AA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.623	89	91	100	rBV4	36076	73217	1.42%	0.198%
2	4.352	213	215	218	rVB4	9739	5620	0.11%	0.015%
3	5.393	390	392	395	rBV3	6674	7468	0.14%	0.020%
4	5.505	410	411	414	rBV2	7413	6319	0.12%	0.017%
5	5.734	446	450	452	rBV4	5993	7795	0.15%	0.021%
6	6.864	637	642	652	rBV2	244023	397085	7.68%	1.073%
7	7.028	664	670	681	rBV	336532	584557	11.31%	1.579%
8	7.134	686	688	693	rVB4	5924	6611	0.13%	0.018%
9	7.222	695	703	711	rBV2	533794	868548	16.81%	2.347%
10	7.558	758	760	763	rVB2	5211	5866	0.11%	0.016%
11	7.687	776	782	791	rBV2	400367	626223	12.12%	1.692%
12	8.393	895	902	915	rBV	522100	851411	16.48%	2.300%
13	8.687	950	952	957	rBV3	4464	6102	0.12%	0.016%
14	8.840	971	978	986	rBV	554764	939998	18.19%	2.540%
15	9.016	1007	1008	1013	rBV3	5755	8175	0.16%	0.022%
16	9.275	1050	1052	1055	rBV3	4530	5713	0.11%	0.015%
17	9.557	1094	1100	1109	rBV2	517749	844003	16.33%	2.280%
18	10.099	1184	1192	1204	rBV	751058	1249924	24.19%	3.377%
19	10.475	1249	1256	1266	rBV	472900	808784	15.65%	2.185%
20	10.610	1272	1279	1293	rBV	517415	978480	18.94%	2.644%
21	12.075	1523	1528	1531	rBV5	11486	18105	0.35%	0.049%
22	13.175	1712	1715	1721	rVB4	4235	5581	0.11%	0.015%
23	13.751	1804	1813	1818	rBV	1544097	2156239	41.73%	5.826%
24	13.793	1818	1820	1825	rVB2	42496	60138	1.16%	0.162%
25	14.034	1853	1861	1872	rBV	1411611	2219175	42.95%	5.996%
26	14.340	1907	1913	1923	rBV3	765481	1145537	22.17%	3.095%
27	14.451	1930	1932	1936	rBV2	4933	5866	0.11%	0.016%
28	14.557	1944	1950	1964	rBV2	140613	291793	5.65%	0.788%
29	15.175	2053	2055	2058	rVB	5524	6300	0.12%	0.017%
30	15.340	2076	2083	2096	rVB	1964523	2873714	55.61%	7.764%
31	15.457	2098	2103	2114	rBV	724266	1013708	19.62%	2.739%
32	15.581	2120	2124	2128	rBV2	30937	37064	0.72%	0.100%
33	15.698	2140	2144	2145	rVB	5122	5698	0.11%	0.015%
34	15.828	2163	2166	2169	rBV2	4492	6195	0.12%	0.017%
35	15.910	2176	2180	2183	rVB4	4237	6223	0.12%	0.017%
36	16.122	2210	2216	2221	rBV4	10348	18338	0.35%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014908.D
 Acq On : 14 Jun 2021 21:03
 Operator : CG/JU
 Sample : M2649-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 B0AA7

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

37	16.239	2233	2236	2240	rBV2	3886	5581	0.11%	0.015%
38	16.410	2261	2265	2268	rBV3	4947	8755	0.17%	0.024%
39	16.598	2295	2297	2301	rBV4	5406	6442	0.12%	0.017%
40	16.887	2341	2346	2348	rBV2	6762	9151	0.18%	0.025%
41	17.092	2375	2381	2391	rBV	1019332	1502580	29.08%	4.060%
42	17.192	2391	2398	2412	rBV	2278459	3371325	65.24%	9.108%
43	17.998	2531	2535	2544	rBV5	49948	69451	1.34%	0.188%
44	18.063	2544	2546	2547	rBV2	5727	5755	0.11%	0.016%
45	18.245	2574	2577	2580	rVB2	6934	7162	0.14%	0.019%
46	19.133	2721	2728	2732	rBV4	34700	58097	1.12%	0.157%
47	19.286	2752	2754	2759	rVB5	18738	22861	0.44%	0.062%
48	19.386	2767	2771	2774	rBV	26706	28331	0.55%	0.077%
49	19.428	2774	2778	2783	rBV	52180	65628	1.27%	0.177%
50	19.498	2783	2790	2798	rBV	2903864	4213185	81.54%	11.383%
51	19.598	2805	2807	2809	rVB2	8846	5760	0.11%	0.016%
52	19.692	2819	2823	2825	rBV4	6315	9903	0.19%	0.027%
53	19.745	2825	2832	2837	rVV5	43947	70986	1.37%	0.192%
54	19.963	2867	2869	2873	rBV4	6340	7293	0.14%	0.020%
55	21.022	3045	3049	3053	rBV7	48547	92036	1.78%	0.249%
56	21.292	3090	3095	3103	rBV2	1540594	2029035	39.27%	5.482%
57	23.404	3446	3454	3466	rBV	2568401	5167178	100.00%	13.960%
58	23.545	3472	3478	3485	rBV	1128188	2105220	40.74%	5.688%


Sum of corrected areas: 37013288

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014908.D
Acq On : 14 Jun 2021 21:03
Operator : CG/JU
Sample : M2649-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
B0AA7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

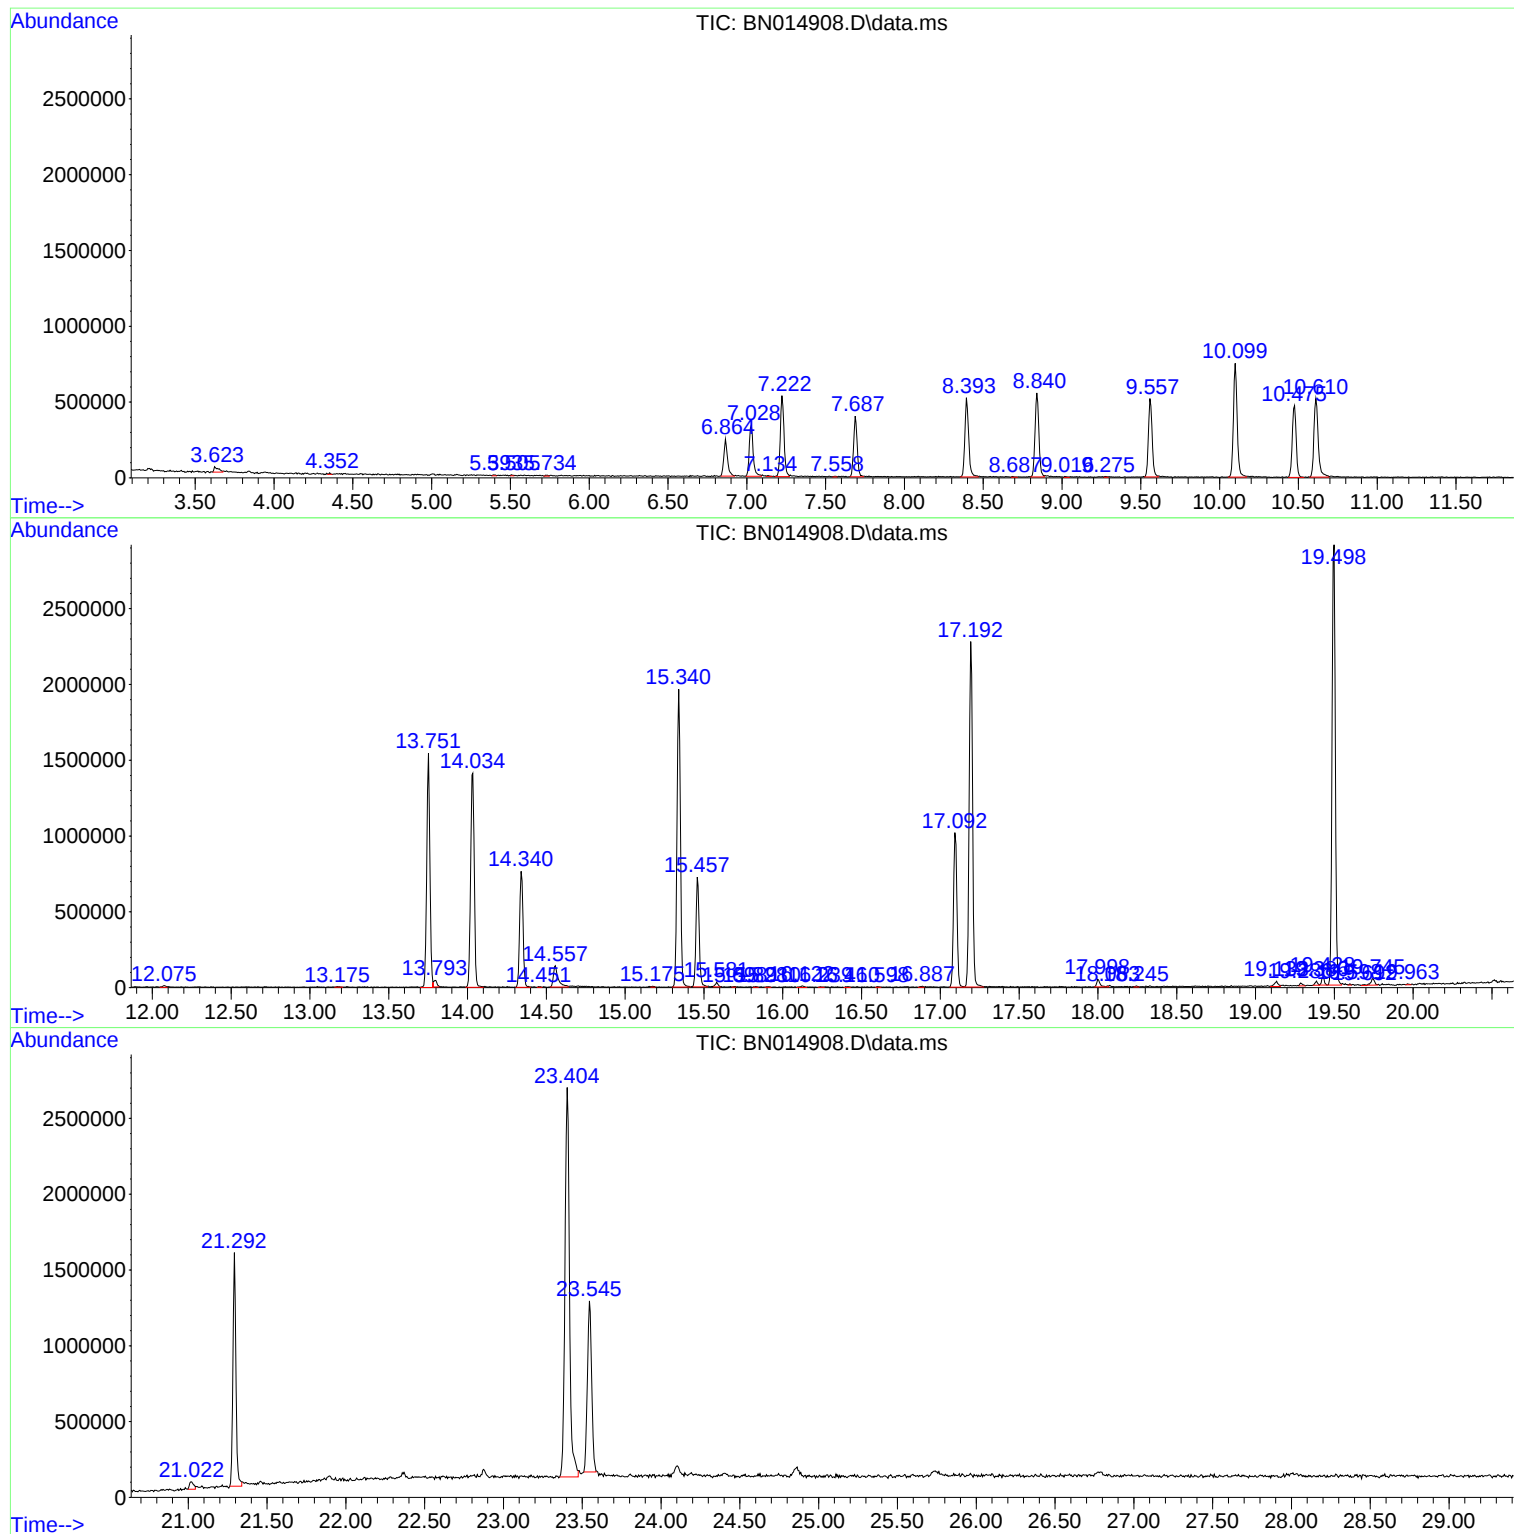

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014908.D
Acq On : 14 Jun 2021 21:03
Operator : CG/JU
Sample : M2649-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
B0AA7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014908.D
Acq On : 14 Jun 2021 21:03
Operator : CG/JU
Sample : M2649-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
B0AA7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
