

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014909.D
 Acq On : 14 Jun 2021 21:39
 Operator : CG/JU
 Sample : M2649-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 B0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	18	20	23	rVB3	19492	20106	0.32%	0.045%
2	3.234	23	25	27	rVB3	11860	7636	0.12%	0.017%
3	3.405	52	54	56	rBV3	6431	6292	0.10%	0.014%
4	3.475	62	66	67	rBV4	6680	8704	0.14%	0.019%
5	3.622	87	91	93	rBV2	65380	87018	1.39%	0.194%
6	3.793	119	120	122	rBV2	10275	6574	0.10%	0.015%
7	3.905	138	139	141	rBV	8932	8310	0.13%	0.019%
8	4.016	156	158	160	rBV3	5735	7029	0.11%	0.016%
9	4.293	202	205	206	rBV3	11638	9095	0.14%	0.020%
10	4.311	206	208	211	rVV4	7417	6878	0.11%	0.015%
11	4.493	237	239	242	rVB4	7370	7229	0.12%	0.016%
12	4.663	265	268	272	rBV6	10294	14097	0.22%	0.031%
13	4.728	277	279	281	rVB3	8922	7795	0.12%	0.017%
14	4.816	292	294	299	rVB4	6169	7643	0.12%	0.017%
15	5.011	323	327	330	rBV5	9340	14213	0.23%	0.032%
16	5.063	335	336	338	rBV2	10137	6817	0.11%	0.015%
17	5.646	431	435	438	rBV5	7215	8417	0.13%	0.019%
18	6.205	526	530	533	rBV5	3635	6576	0.10%	0.015%
19	6.652	603	606	609	rBV2	6719	6611	0.11%	0.015%
20	6.775	625	627	632	rBV5	4748	8427	0.13%	0.019%
21	6.863	635	642	652	rBV	301939	527547	8.41%	1.175%
22	7.022	664	669	681	rBV	414142	712669	11.36%	1.587%
23	7.222	697	703	717	rBV	670237	1076592	17.16%	2.397%
24	7.687	775	782	788	rBV2	407731	649290	10.35%	1.446%
25	7.757	791	794	796	rBV3	6565	6390	0.10%	0.014%
26	8.393	896	902	913	rBV	670780	1078388	17.18%	2.401%
27	8.840	972	978	986	rBV	693811	1159087	18.47%	2.581%
28	9.210	1038	1041	1043	rBV3	6036	6420	0.10%	0.014%
29	9.287	1050	1054	1056	rVB3	4342	6833	0.11%	0.015%
30	9.557	1094	1100	1111	rVV2	634085	1098524	17.51%	2.446%
31	10.098	1186	1192	1202	rBV	916936	1593106	25.39%	3.547%
32	10.204	1209	1210	1216	rVB3	6300	8349	0.13%	0.019%
33	10.475	1248	1256	1263	rVV	467792	816380	13.01%	1.818%
34	10.610	1270	1279	1292	rBV	717104	1269038	20.22%	2.826%
35	11.887	1492	1496	1498	rBV3	4478	6975	0.11%	0.016%
36	12.081	1523	1529	1533	rVB2	11736	20360	0.32%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014909.D
 Acq On : 14 Jun 2021 21:39
 Operator : CG/JU
 Sample : M2649-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 B0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

37	13.239	1722	1726	1729	rVB5	3989	6506	0.10%	0.014%
38	13.751	1806	1813	1818	rBV	1924736	2603305	41.48%	5.797%
39	13.798	1818	1821	1829	rVB	77297	108400	1.73%	0.241%
40	14.034	1853	1861	1872	rBV	1842670	2802178	44.65%	6.239%
41	14.339	1906	1913	1922	rBV	795512	1160750	18.50%	2.585%
42	14.551	1944	1949	1958	rBV2	221324	394499	6.29%	0.878%
43	14.704	1973	1975	1982	rVB4	7948	11952	0.19%	0.027%
44	14.757	1982	1984	1989	rBV3	6837	7518	0.12%	0.017%
45	15.169	2050	2054	2055	rBV4	14563	9440	0.15%	0.021%
46	15.339	2076	2083	2090	rBV	2437933	3496526	55.72%	7.785%
47	15.457	2097	2103	2113	rBV	910152	1270956	20.25%	2.830%
48	15.581	2119	2124	2127	rVV4	30879	50610	0.81%	0.113%
49	16.128	2214	2217	2220	rVB2	14239	17280	0.28%	0.038%
50	16.580	2289	2294	2296	rBV2	4876	6815	0.11%	0.015%
51	16.869	2339	2343	2347	rBV4	7576	13704	0.22%	0.031%
52	17.092	2374	2381	2387	rVV	1062290	1534265	24.45%	3.416%
53	17.192	2391	2398	2410	rVV2	2708110	4005434	63.83%	8.919%
54	17.775	2495	2497	2501	rVB2	8011	7854	0.13%	0.017%
55	17.886	2513	2516	2519	rVB3	5459	6951	0.11%	0.015%
56	17.945	2523	2526	2529	rVV2	4993	8458	0.13%	0.019%
57	18.004	2529	2536	2544	rVV5	70017	123140	1.96%	0.274%
58	18.069	2546	2547	2554	rVV5	16774	22343	0.36%	0.050%
59	18.304	2585	2587	2591	rVB4	6501	7842	0.12%	0.017%
60	19.051	2711	2714	2718	rBV6	9138	13722	0.22%	0.031%
61	19.133	2723	2728	2731	rVV	36883	51766	0.82%	0.115%
62	19.186	2735	2737	2739	rVV3	9576	8453	0.13%	0.019%
63	19.286	2751	2754	2758	rVV6	30549	34928	0.56%	0.078%
64	19.316	2758	2759	2764	rVB4	9696	9755	0.16%	0.022%
65	19.380	2764	2770	2775	rBV3	28638	48397	0.77%	0.108%
66	19.427	2775	2778	2783	rVV	61010	73280	1.17%	0.163%
67	19.498	2783	2790	2800	rVV	3572120	5067839	80.76%	11.284%
68	19.745	2827	2832	2837	rVB3	54182	77739	1.24%	0.173%
69	19.904	2858	2859	2862	rVB3	9616	8690	0.14%	0.019%
70	19.939	2862	2865	2867	rBV4	5796	8586	0.14%	0.019%
71	20.057	2882	2885	2887	rVB4	12664	11017	0.18%	0.025%
72	20.163	2902	2903	2906	rBV2	6240	7384	0.12%	0.016%
73	20.192	2906	2908	2911	rVV4	9411	10390	0.17%	0.023%
74	20.233	2911	2915	2917	rVV4	9657	13845	0.22%	0.031%
75	20.269	2919	2921	2924	rVV4	7739	8832	0.14%	0.020%
76	20.316	2924	2929	2930	rVB3	11894	13150	0.21%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014909.D
 Acq On : 14 Jun 2021 21:39
 Operator : CG/JU
 Sample : M2649-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 B0AA9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

77	20.327	2930	2931	2934	rBV3	11181	11243	0.18%	0.025%
78	20.374	2937	2939	2941	rBV2	11074	7612	0.12%	0.017%
79	20.516	2959	2963	2965	rVV5	27125	26691	0.43%	0.059%
80	20.551	2967	2969	2972	rVB4	12280	12011	0.19%	0.027%
81	20.598	2976	2977	2979	rBV2	8880	6878	0.11%	0.015%
82	20.669	2987	2989	2990	rVB2	9412	6450	0.10%	0.014%
83	20.798	3008	3011	3012	rBV3	9288	10537	0.17%	0.023%
84	20.880	3021	3025	3028	rBV6	14431	21319	0.34%	0.047%
85	21.016	3044	3048	3058	rBV8	125514	250703	4.00%	0.558%
86	21.163	3071	3073	3076	rBV4	12804	14475	0.23%	0.032%
87	21.292	3090	3095	3101	rBV	1589747	2065712	32.92%	4.600%
88	21.374	3108	3109	3111	rBV2	16717	15186	0.24%	0.034%
89	21.692	3162	3163	3164	rBV	16633	7183	0.11%	0.016%
90	21.798	3178	3181	3183	rBV4	25662	31947	0.51%	0.071%
91	22.357	3274	3276	3280	rVB4	40945	46388	0.74%	0.103%
92	22.874	3361	3364	3368	rVB6	55904	84721	1.35%	0.189%
93	23.404	3446	3454	3469	rBV	3011405	6275293	100.00%	13.973%
94	23.545	3471	3478	3488	rVB2	1199190	2352050	37.48%	5.237%
95	24.857	3696	3701	3709	rVB10	70432	139099	2.22%	0.310%
96	25.739	3849	3851	3856	rVB6	48820	67903	1.08%	0.151%
97	28.545	4327	4328	4330	rBV2	28338	21957	0.35%	0.049%


Sum of corrected areas: 44911272

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014909.D
Acq On : 14 Jun 2021 21:39
Operator : CG/JU
Sample : M2649-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
B0AA9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

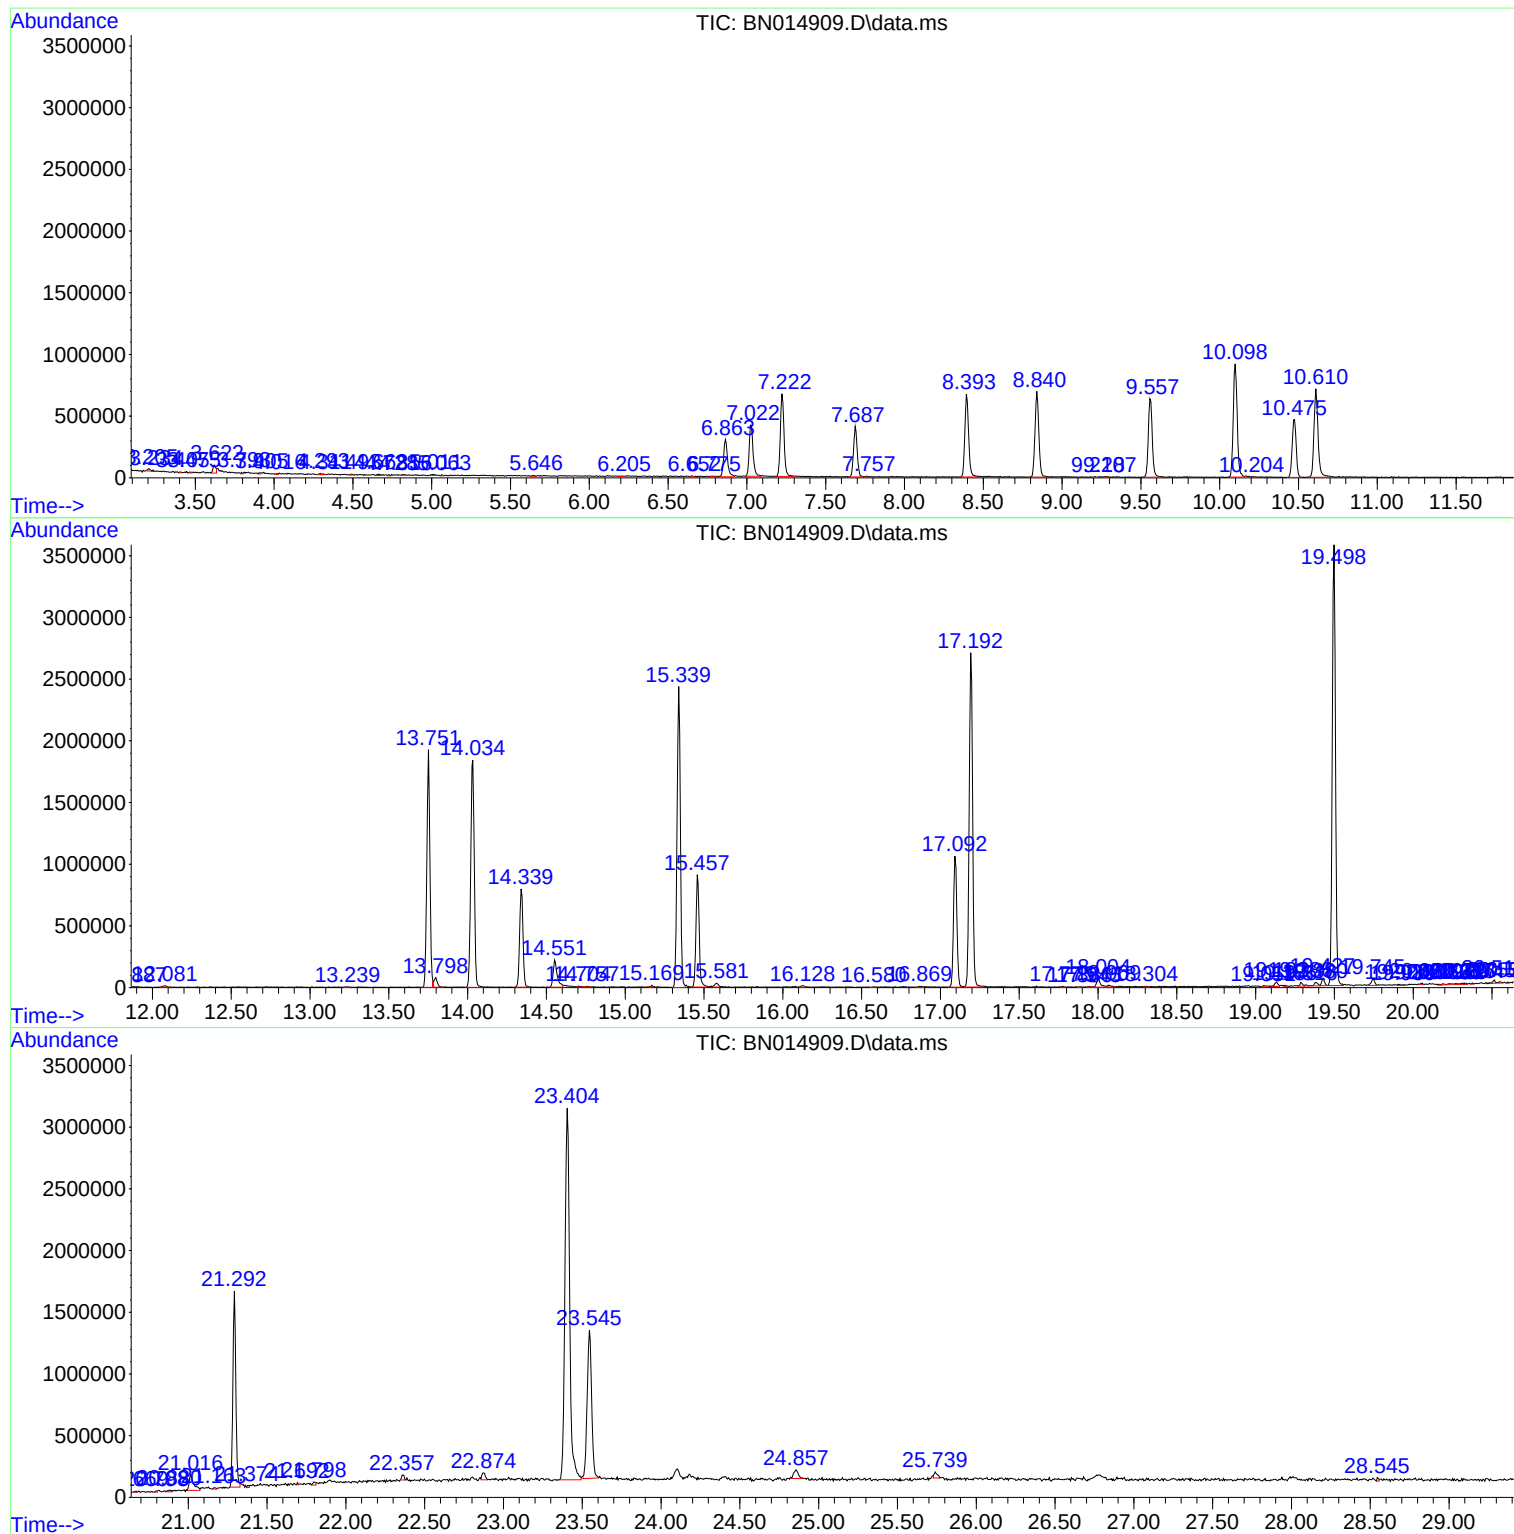

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014909.D
Acq On : 14 Jun 2021 21:39
Operator : CG/JU
Sample : M2649-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
B0AA9










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Nonadecyl trifluoroacetate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.016	2.43 ng/ul	250703	Chrysene-d12	21.292

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Nonadecyl trifluoroacetate	380	C21H39F3O2	1000351-76-3	90
2			2- Chloropropionic acid, pentade...	318	C18H35ClO2	1000292-44-1	74
3			Bacteriochlorophyll-c-stearyl	841	C52H72MgN4O4	1000164-49-7	72
4			Heptafluorobutyric acid, n-octad...	466	C22H37F7O2	000400-57-7	70
5			1-Nonadecene	266	C19H38	018435-45-5	70

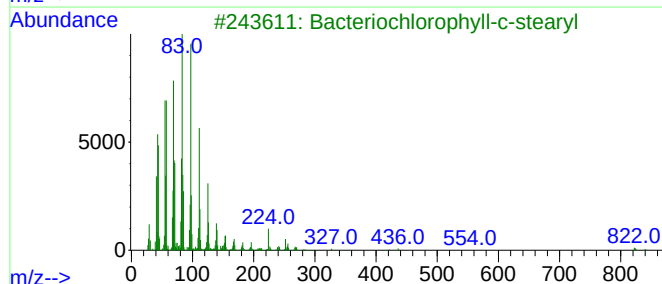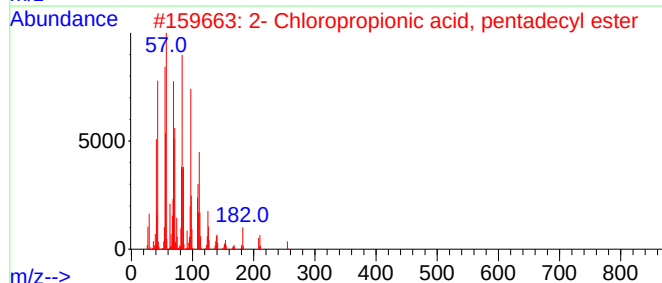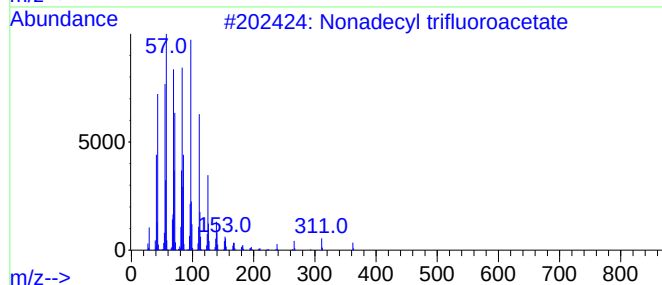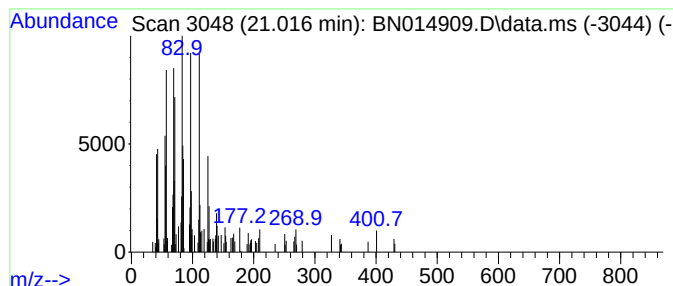

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014909.D
Acq On : 14 Jun 2021 21:39
Operator : CG/JU
Sample : M2649-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
B0AA9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Nonadecyl trifl...	21.016	2.4	ng/u1	250703	5	21.292	2065710	20.0