

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014913.D
 Acq On : 15 Jun 2021 00:02
 Operator : CG/JU
 Sample : PB137031BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK031

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014913.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	16	rVB	552106	561243	27.67%	5.907%
2	3.457	61	63	68	rVB6	18131	20318	1.00%	0.214%
3	4.751	282	283	285	rBV2	6021	3570	0.18%	0.038%
4	5.146	348	350	353	rVB2	4951	4146	0.20%	0.044%
5	5.299	374	376	381	rBV3	4980	8905	0.44%	0.094%
6	5.340	381	383	385	rVV3	5387	3293	0.16%	0.035%
7	5.551	417	419	423	rVB3	5874	4619	0.23%	0.049%
8	5.757	451	454	455	rBV2	6730	6258	0.31%	0.066%
9	5.828	464	466	468	rBV2	4264	4030	0.20%	0.042%
10	5.946	484	486	490	rBV3	4035	5126	0.25%	0.054%
11	6.069	505	507	511	rVV3	5443	4808	0.24%	0.051%
12	6.104	511	513	515	rVB4	6166	3945	0.19%	0.042%
13	6.534	584	586	588	rBV	6231	6705	0.33%	0.071%
14	6.628	600	602	605	rVB3	4891	3941	0.19%	0.041%
15	6.804	628	632	634	rBV3	6841	8515	0.42%	0.090%
16	6.875	641	644	646	rVB3	3751	4661	0.23%	0.049%
17	7.169	690	694	696	rBV3	4688	4613	0.23%	0.049%
18	7.310	717	718	721	rVB3	4450	3181	0.16%	0.033%
19	7.481	745	747	749	rVB2	5162	4070	0.20%	0.043%
20	7.498	749	750	754	rBV	4099	5309	0.26%	0.056%
21	7.687	775	782	789	rBV	493382	790001	38.95%	8.315%
22	7.892	813	817	821	rVB4	4486	7793	0.38%	0.082%
23	8.069	845	847	853	rVB	2753	3798	0.19%	0.040%
24	8.210	869	871	874	rVB3	3819	4690	0.23%	0.049%
25	8.240	874	876	878	rBV2	3628	3890	0.19%	0.041%
26	8.340	889	893	895	rBV2	3967	4237	0.21%	0.045%
27	8.604	936	938	940	rBV2	3770	3471	0.17%	0.037%
28	8.704	953	955	957	rVB3	4043	3301	0.16%	0.035%
29	8.728	957	959	961	rBV	3243	3173	0.16%	0.033%
30	8.792	966	970	973	rVB3	4536	6004	0.30%	0.063%
31	8.822	973	975	977	rBV2	3735	3223	0.16%	0.034%
32	8.845	977	979	984	rVV4	3619	4451	0.22%	0.047%
33	8.951	994	997	1000	rVB2	3075	3428	0.17%	0.036%
34	9.263	1043	1050	1052	rVV4	4643	9013	0.44%	0.095%
35	10.322	1228	1230	1233	rVB2	3688	3333	0.16%	0.035%
36	10.345	1233	1234	1237	rBV2	4030	3534	0.17%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014913.D
 Acq On : 15 Jun 2021 00:02
 Operator : CG/JU
 Sample : PB137031BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK031

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

37	10.469	1249	1255	1263	rBV	510089	912743	45.00%	9.607%
38	10.581	1272	1274	1277	rVB2	6249	4656	0.23%	0.049%
39	10.710	1293	1296	1298	rVB2	3344	3892	0.19%	0.041%
40	10.745	1301	1302	1306	rVV2	3175	3810	0.19%	0.040%
41	10.775	1306	1307	1311	rVB2	3560	3650	0.18%	0.038%
42	10.916	1330	1331	1336	rVB	3144	4215	0.21%	0.044%
43	11.092	1359	1361	1364	rBV	2696	3204	0.16%	0.034%
44	11.651	1454	1456	1459	rVB2	3217	3393	0.17%	0.036%
45	11.698	1462	1464	1468	rVB	2733	3493	0.17%	0.037%
46	11.769	1470	1476	1477	rBV3	4347	5240	0.26%	0.055%
47	11.904	1496	1499	1501	rBV	3164	3486	0.17%	0.037%
48	11.922	1501	1502	1506	rVB	3403	4010	0.20%	0.042%
49	11.957	1506	1508	1511	rBV2	2864	3836	0.19%	0.040%
50	12.228	1548	1554	1556	rVB	3987	4679	0.23%	0.049%
51	12.275	1559	1562	1564	rBV3	4033	3430	0.17%	0.036%
52	12.798	1647	1651	1653	rVB	3429	3223	0.16%	0.034%
53	12.875	1661	1664	1667	rVB	4186	4640	0.23%	0.049%
54	13.163	1712	1713	1718	rVB2	3165	3197	0.16%	0.034%
55	13.516	1771	1773	1776	rVB2	3043	3216	0.16%	0.034%
56	14.339	1906	1913	1922	rBV	804353	1205005	59.41%	12.683%
57	14.539	1944	1947	1950	rVB	3512	3488	0.17%	0.037%
58	14.633	1960	1963	1967	rVB3	3592	3832	0.19%	0.040%
59	14.769	1985	1986	1991	rBV2	2788	3232	0.16%	0.034%
60	14.945	2011	2016	2020	rBV3	1981	4206	0.21%	0.044%
61	14.992	2022	2024	2031	rBV2	2046	3623	0.18%	0.038%
62	15.104	2039	2043	2044	rBV	4212	3657	0.18%	0.038%
63	15.180	2052	2056	2059	rVB2	2982	3953	0.19%	0.042%
64	15.345	2081	2084	2088	rBV2	2220	3644	0.18%	0.038%
65	15.674	2136	2140	2144	rBV	2740	3388	0.17%	0.036%
66	16.804	2328	2332	2333	rBV2	3739	3484	0.17%	0.037%
67	16.892	2344	2347	2349	rVB2	4152	3447	0.17%	0.036%
68	16.957	2356	2358	2360	rBV	3046	3218	0.16%	0.034%
69	16.980	2360	2362	2366	rVB2	3155	3550	0.18%	0.037%
70	17.092	2374	2381	2394	rBV	1009255	1551611	76.50%	16.331%
71	17.433	2435	2439	2442	rBV2	4019	5582	0.28%	0.059%
72	17.821	2502	2505	2506	rVB	4059	3304	0.16%	0.035%
73	17.963	2526	2529	2530	rVB2	2723	3389	0.17%	0.036%
74	18.163	2562	2563	2566	rBV	3568	3281	0.16%	0.035%
75	18.286	2582	2584	2586	rBV	2765	3523	0.17%	0.037%
76	18.445	2605	2611	2614	rVB2	5027	6806	0.34%	0.072%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014913.D
 Acq On : 15 Jun 2021 00:02
 Operator : CG/JU
 Sample : PB137031BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK031

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

77	18.474	2614	2616	2618	rBV2	6223	5916	0.29%	0.062%
78	18.521	2622	2624	2629	rVB3	3211	5035	0.25%	0.053%
79	18.568	2629	2632	2635	rBV3	3135	4248	0.21%	0.045%
80	18.627	2638	2642	2645	rBV3	4364	6080	0.30%	0.064%
81	18.686	2650	2652	2657	rVB4	4751	6443	0.32%	0.068%
82	18.727	2657	2659	2662	rBV3	5326	7277	0.36%	0.077%
83	18.980	2700	2702	2705	rVB2	5280	5306	0.26%	0.056%
84	19.021	2706	2709	2711	rBV3	5377	3529	0.17%	0.037%
85	19.127	2725	2727	2730	rBV4	5911	5807	0.29%	0.061%
86	19.157	2730	2732	2734	rVB2	7739	4747	0.23%	0.050%
87	19.245	2744	2747	2749	rBV4	5487	6329	0.31%	0.067%
88	19.286	2753	2754	2758	rVB2	6333	6162	0.30%	0.065%
89	19.333	2758	2762	2764	rBV3	4748	7449	0.37%	0.078%
90	19.415	2774	2776	2779	rBV3	6661	6646	0.33%	0.070%
91	19.468	2781	2785	2788	rVB3	5743	7490	0.37%	0.079%
92	19.510	2788	2792	2794	rBV3	5820	9257	0.46%	0.097%
93	19.598	2802	2807	2809	rBV5	6214	10795	0.53%	0.114%
94	19.821	2843	2845	2848	rBV4	4881	5252	0.26%	0.055%
95	20.033	2880	2881	2882	rBV	7472	3585	0.18%	0.038%
96	20.086	2888	2890	2891	rBV2	7694	6110	0.30%	0.064%
97	20.139	2897	2899	2902	rVB4	10688	8196	0.40%	0.086%
98	20.162	2902	2903	2906	rBV3	7758	5692	0.28%	0.060%
99	21.292	3090	3095	3105	rBV2	1432023	1995421	98.39%	21.003%
100	23.545	3472	3478	3487	rBV2	1018448	2028152	100.00%	21.347%




Sum of corrected areas: 9500756

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014913.D
Acq On : 15 Jun 2021 00:02
Operator : CG/JU
Sample : PB137031BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK031

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

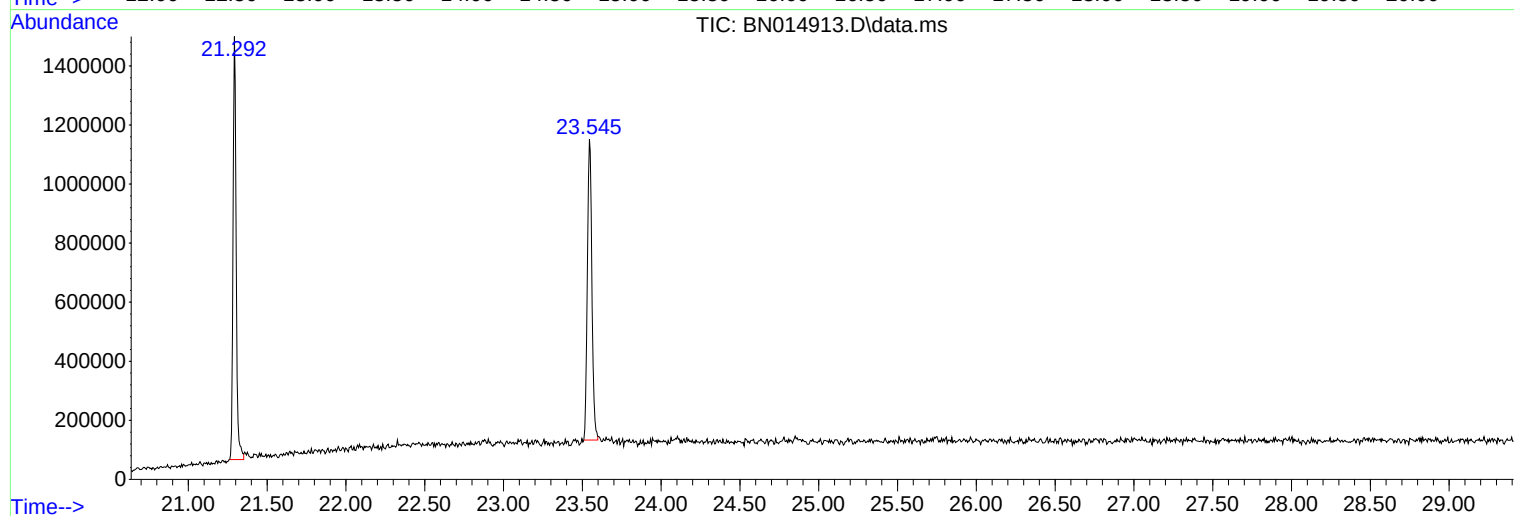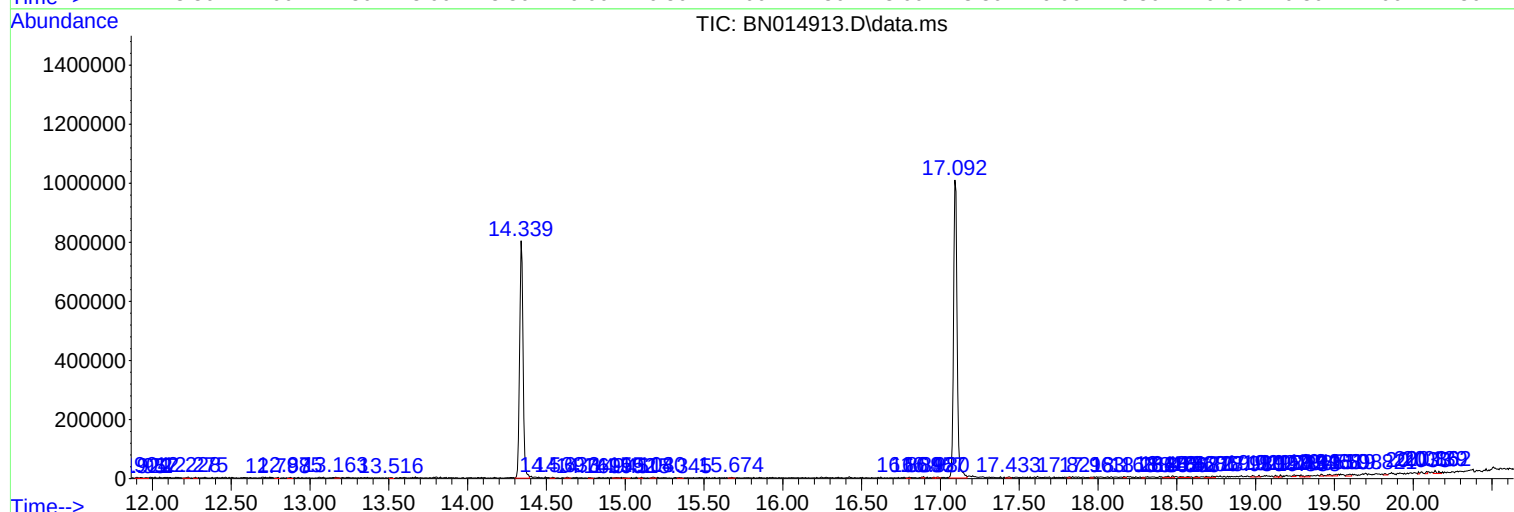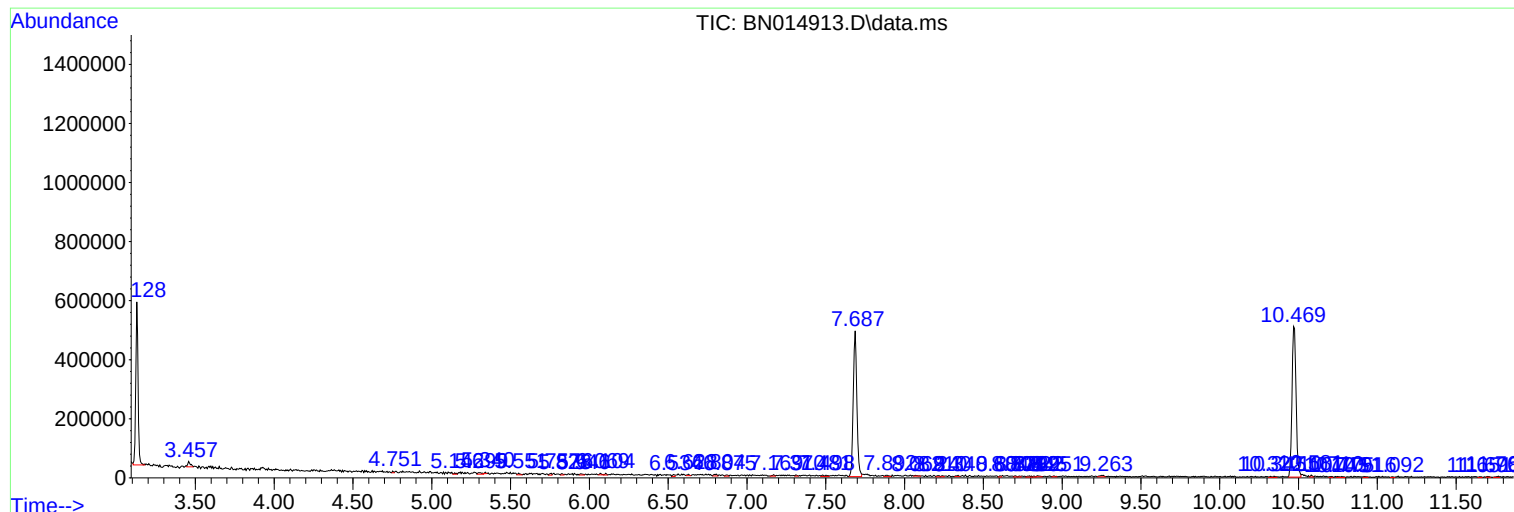

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014913.D
Acq On : 15 Jun 2021 00:02
Operator : CG/JU
Sample : PB137031BL
Misc :
ALS Vial : 16 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
SBLK031

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
3.128	14.21 ng/ul	561243	1,4-Dichlorobenzene-d4			7.687
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	Heptane		100	C7H16	000142-82-5	46
2	Butane, 2,2-dimethyl-		86	C6H14	000075-83-2	43
3	Hydroxylamine, O-(2-methylpropyl)-		89	C4H11NO	005618-62-2	42
4	Heptane		100	C7H16	000142-82-5	38
5	2-Penten-1-ol, 2-methyl-, (E)-		100	C6H12O	016958-19-3	38

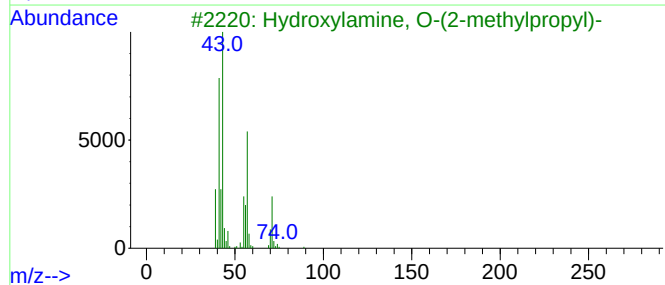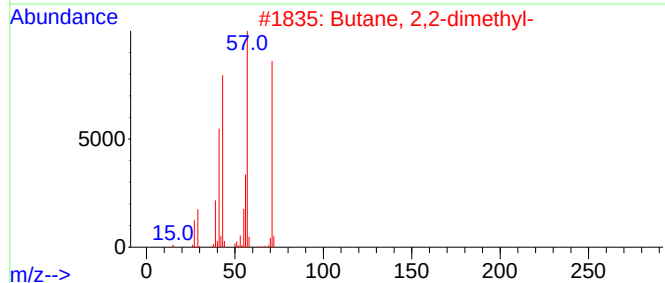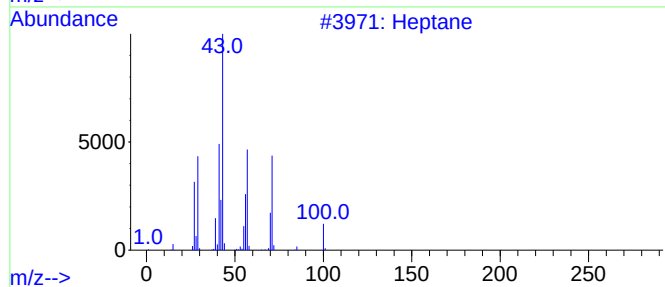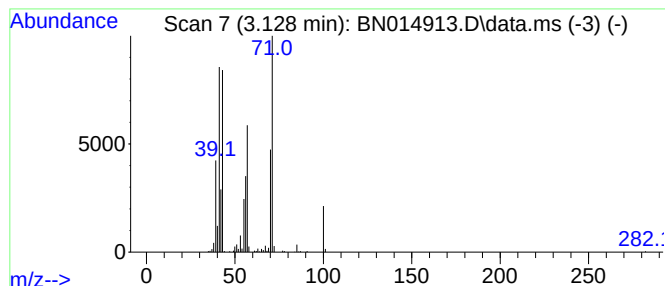

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014913.D
Acq On : 15 Jun 2021 00:02
Operator : CG/JU
Sample : PB137031BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK031

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.128	14.2	ng/u1	561243	1	7.687	790001	20.0