

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014920.D
 Acq On : 15 Jun 2021 10:40
 Operator : CG/JU
 Sample : M2649-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 B0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014920.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.622	88	91	98	rBV2	75121	127018	2.44%	0.319%
2	6.863	637	642	653	rBV2	186019	317697	6.11%	0.797%
3	7.022	664	669	677	rBV	372395	618951	11.90%	1.553%
4	7.222	697	703	712	rBV	543627	890601	17.12%	2.234%
5	7.687	775	782	792	rVB	445164	726660	13.97%	1.823%
6	7.916	819	821	826	rVB4	4651	6535	0.13%	0.016%
7	8.393	896	902	914	rBV2	484560	830533	15.96%	2.083%
8	8.840	971	978	988	rBV2	569996	992278	19.07%	2.489%
9	9.275	1050	1052	1061	rVB4	8202	13731	0.26%	0.034%
10	9.557	1094	1100	1109	rBV2	514931	876288	16.84%	2.198%
11	10.099	1184	1192	1201	rBV2	767127	1333516	25.63%	3.345%
12	10.469	1248	1255	1264	rBV	546050	922266	17.73%	2.314%
13	10.610	1271	1279	1289	rBV	534496	989759	19.02%	2.483%
14	11.581	1441	1444	1445	rBV	6889	6390	0.12%	0.016%
15	11.887	1492	1496	1497	rBV3	5984	8126	0.16%	0.020%
16	12.063	1523	1526	1533	rVB5	12719	24295	0.47%	0.061%
17	12.693	1629	1633	1635	rBV	5415	6525	0.13%	0.016%
18	13.751	1806	1813	1818	rBV	1632937	2217368	42.62%	5.562%
19	13.798	1818	1821	1827	rVB2	81892	117665	2.26%	0.295%
20	14.028	1853	1860	1870	rBV	1592531	2425347	46.62%	6.084%
21	14.240	1894	1896	1903	rVB4	6068	11495	0.22%	0.029%
22	14.339	1906	1913	1924	rVB	898825	1347764	25.90%	3.381%
23	14.557	1944	1950	1960	rBV3	85137	182468	3.51%	0.458%
24	14.728	1977	1979	1984	rVB2	6431	8506	0.16%	0.021%
25	14.816	1992	1994	2000	rVB4	5681	7441	0.14%	0.019%
26	14.969	2018	2020	2024	rBV2	4088	6272	0.12%	0.016%
27	15.175	2051	2055	2058	rVB4	8873	11442	0.22%	0.029%
28	15.339	2076	2083	2095	rBV	2109903	3095255	59.49%	7.764%
29	15.457	2097	2103	2109	rBV	696597	974653	18.73%	2.445%
30	15.581	2119	2124	2129	rBV6	26805	40496	0.78%	0.102%
31	15.839	2166	2168	2171	rVB2	7132	8430	0.16%	0.021%
32	16.128	2214	2217	2220	rVB4	10847	14857	0.29%	0.037%
33	16.328	2249	2251	2257	rBV2	4357	9269	0.18%	0.023%
34	16.769	2323	2326	2329	rBV3	8684	12994	0.25%	0.033%
35	16.875	2337	2344	2346	rBV3	11745	16967	0.33%	0.043%
36	17.092	2375	2381	2390	rBV	1225921	1779267	34.20%	4.463%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
 Data File : BN014920.D
 Acq On : 15 Jun 2021 10:40
 Operator : CG/JU
 Sample : M2649-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 B0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

37	17.192	2392	2398	2407	rBV	2437451	3464579	66.59%	8.691%
38	17.445	2436	2441	2443	rBV4	5737	7257	0.14%	0.018%
39	17.604	2466	2468	2473	rVB4	10501	11561	0.22%	0.029%
40	17.786	2495	2499	2501	rVB2	6305	9699	0.19%	0.024%
41	17.810	2501	2503	2505	rBV2	7612	6753	0.13%	0.017%
42	17.998	2530	2535	2542	rBV6	72545	118161	2.27%	0.296%
43	18.075	2545	2548	2551	rVB3	11524	13952	0.27%	0.035%
44	18.222	2569	2573	2576	rVB3	5667	7212	0.14%	0.018%
45	18.304	2582	2587	2589	rBV4	8638	13467	0.26%	0.034%
46	18.516	2620	2623	2625	rBV4	6283	7599	0.15%	0.019%
47	18.892	2686	2687	2691	rBV4	6841	8439	0.16%	0.021%
48	19.057	2713	2715	2717	rBV3	7698	6616	0.13%	0.017%
49	19.133	2724	2728	2733	rVB2	33994	41323	0.79%	0.104%
50	19.292	2751	2755	2762	rBV7	34040	46992	0.90%	0.118%
51	19.386	2768	2771	2774	rVB2	25532	28164	0.54%	0.071%
52	19.427	2774	2778	2784	rVB	64804	67171	1.29%	0.168%
53	19.498	2784	2790	2798	rBV	3165344	4420870	84.97%	11.090%
54	19.622	2808	2811	2812	rBV3	7972	7322	0.14%	0.018%
55	19.639	2812	2814	2818	rVB5	7847	7237	0.14%	0.018%
56	19.751	2827	2833	2839	rVB5	53093	81037	1.56%	0.203%
57	20.039	2881	2882	2884	rBV2	12097	11534	0.22%	0.029%
58	20.516	2961	2963	2966	rVB2	32973	27771	0.53%	0.070%
59	20.557	2966	2970	2975	rBV7	18504	33221	0.64%	0.083%
60	21.016	3045	3048	3054	rBV6	98875	163520	3.14%	0.410%
61	21.298	3090	3096	3106	rBV	1775709	2501116	48.07%	6.274%
62	23.410	3448	3455	3470	rBV	2609457	5202725	100.00%	13.051%
63	23.551	3472	3479	3489	rVB	1289153	2570056	49.40%	6.447%


Sum of corrected areas: 39864479

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014920.D
Acq On : 15 Jun 2021 10:40
Operator : CG/JU
Sample : M2649-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
B0AA9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

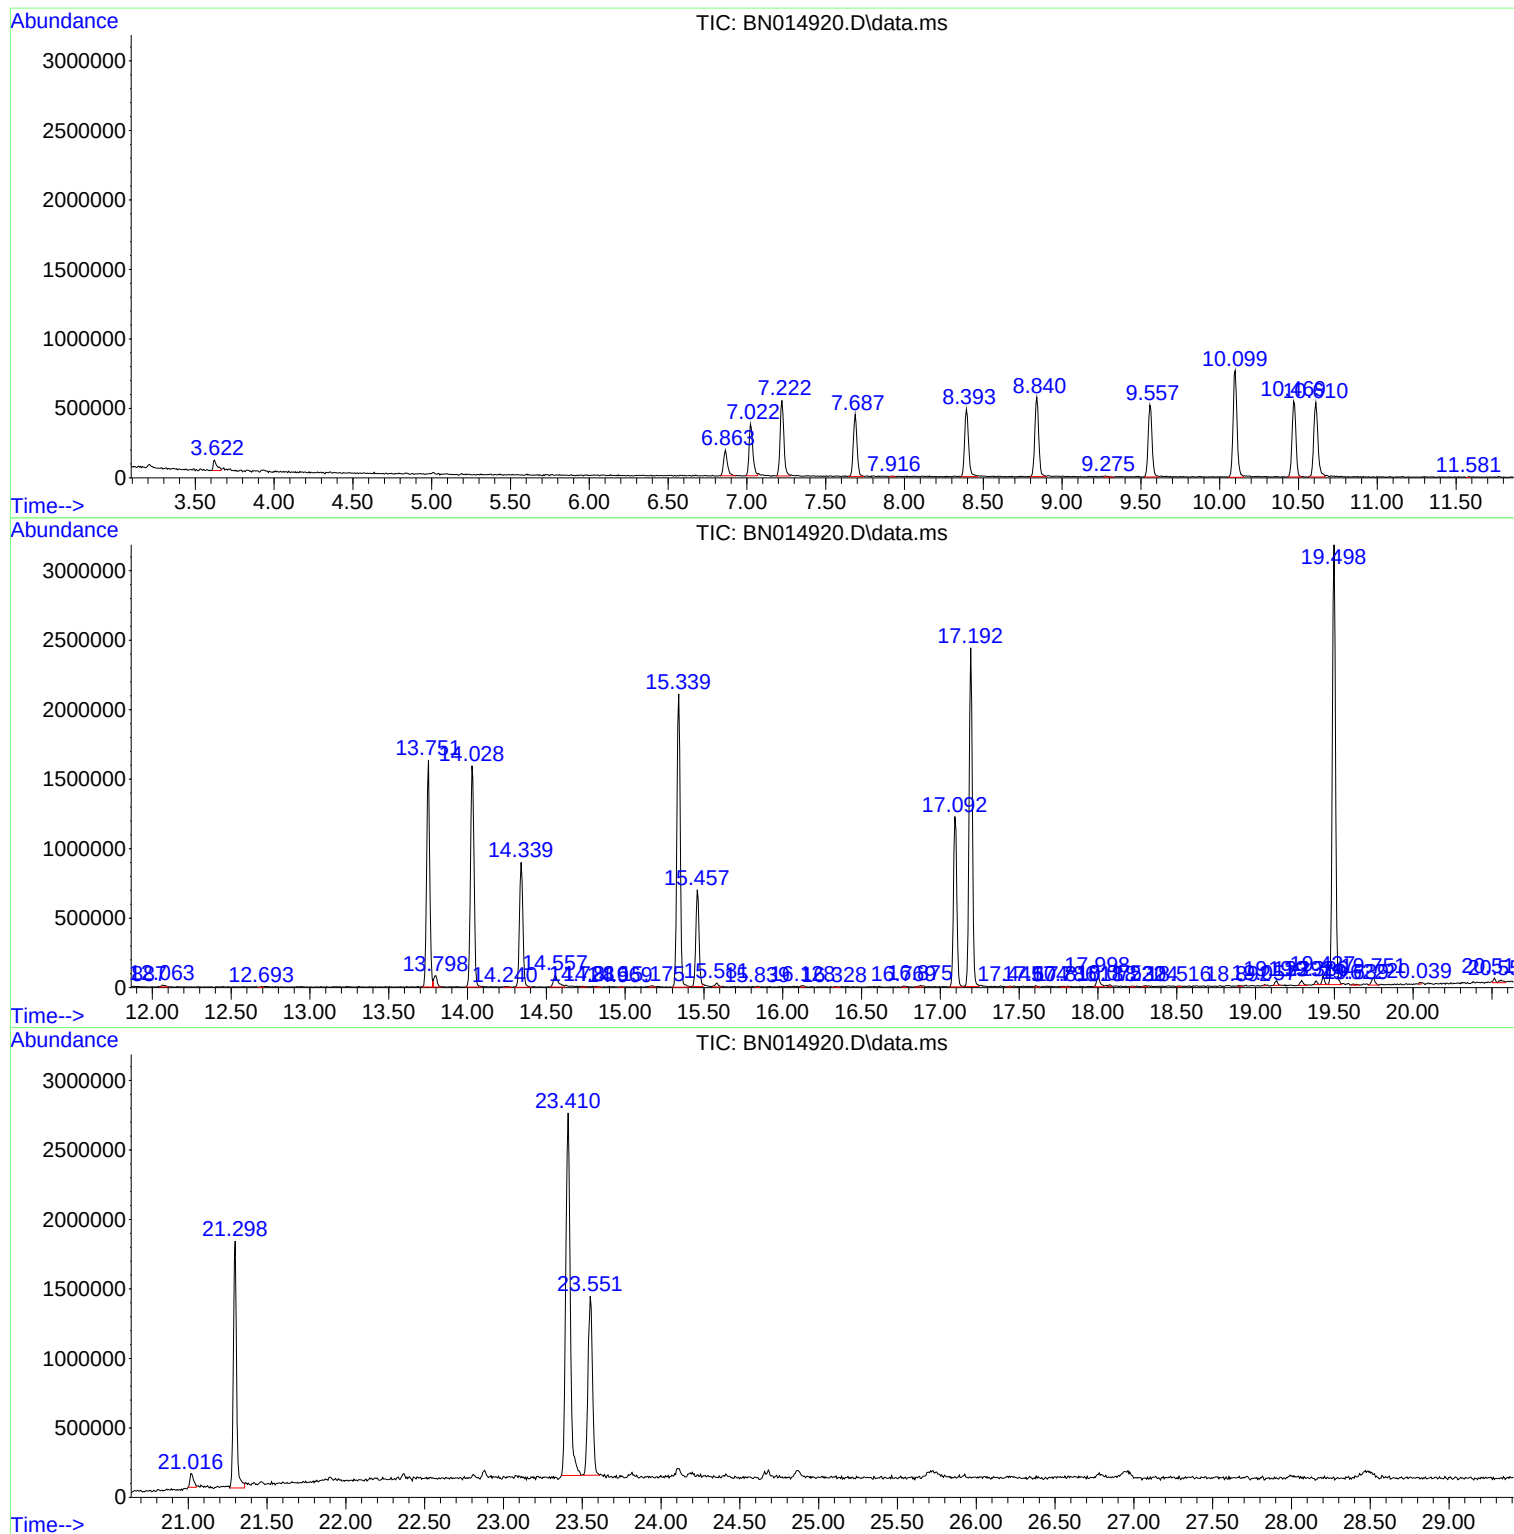

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014920.D
Acq On : 15 Jun 2021 10:40
Operator : CG/JU
Sample : M2649-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
B0AA9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061421\
Data File : BN014920.D
Acq On : 15 Jun 2021 10:40
Operator : CG/JU
Sample : M2649-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
B0AA9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
