
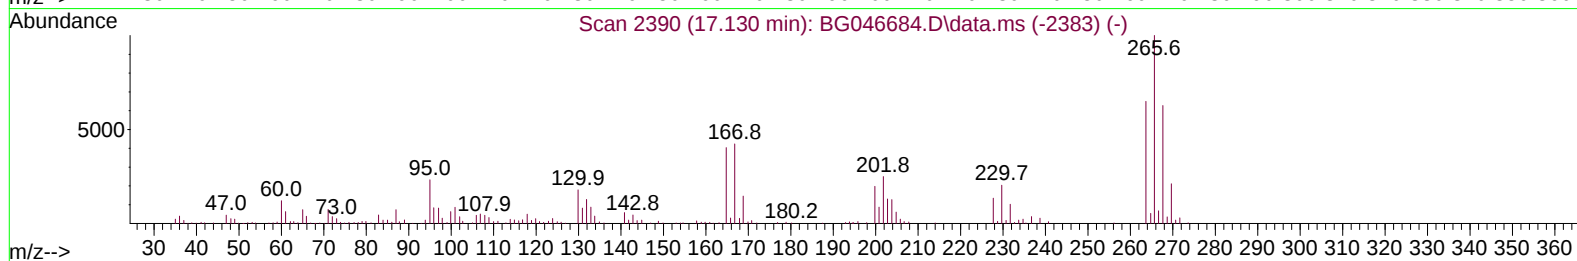
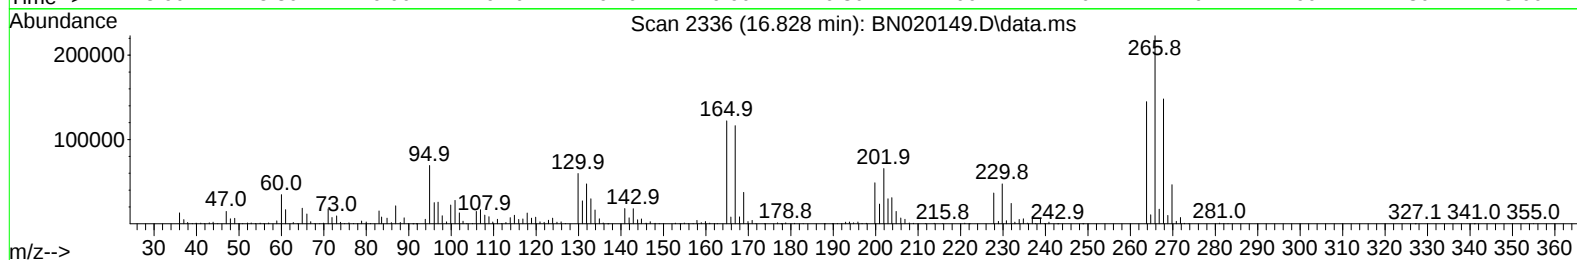


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061422\
Data File : BN020149.D
Acq On : 14 Jun 2022 09:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 13:27:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 14 13:27:42 2022
Response via : Initial Calibration

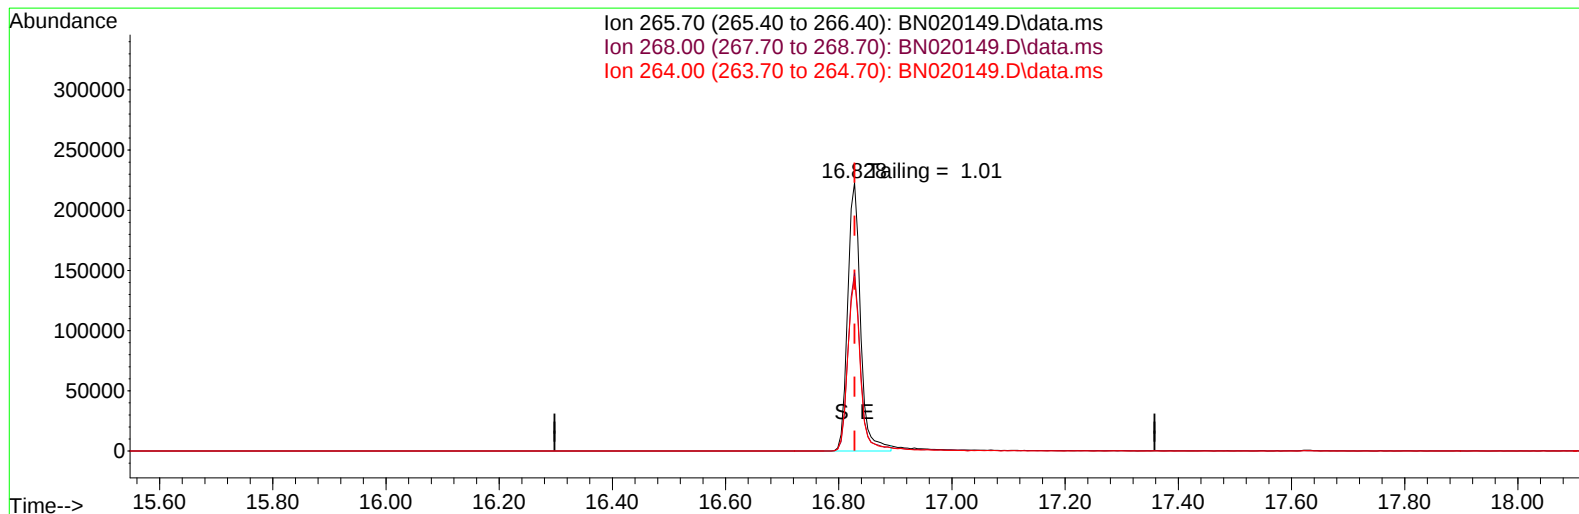

TIC: BN020149.D\data.ms

(70) Pentachlorophenol (C)




16.828min (0.000) 22939.47 ng

response 364367

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.39
264.00	61.60	64.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061422\
Data File : BN020149.D
Acq On : 14 Jun 2022 09:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 13:27:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 14 13:27:42 2022
Response via : Initial Calibration

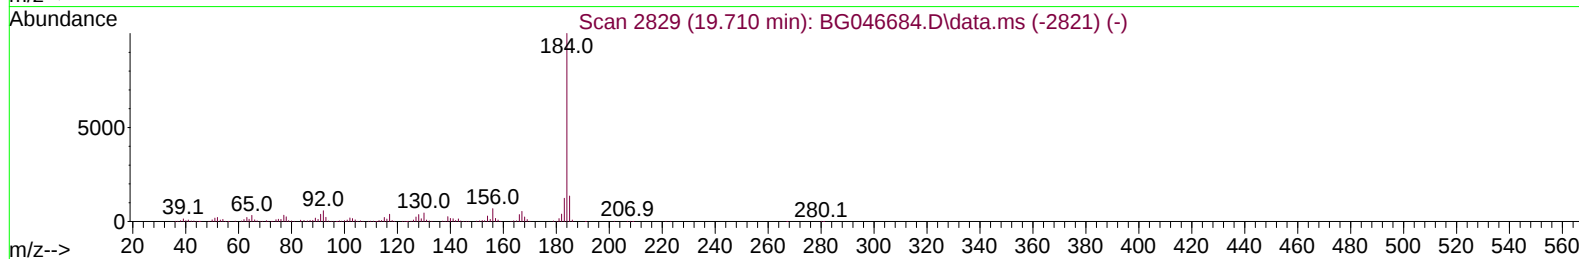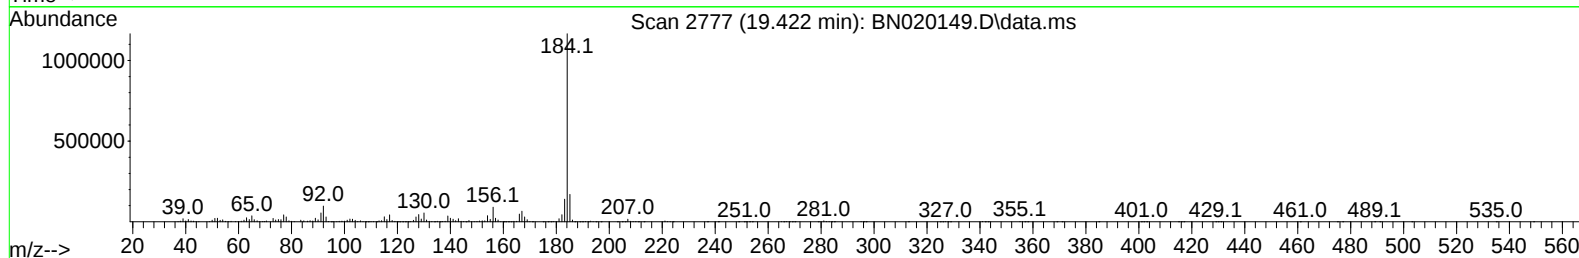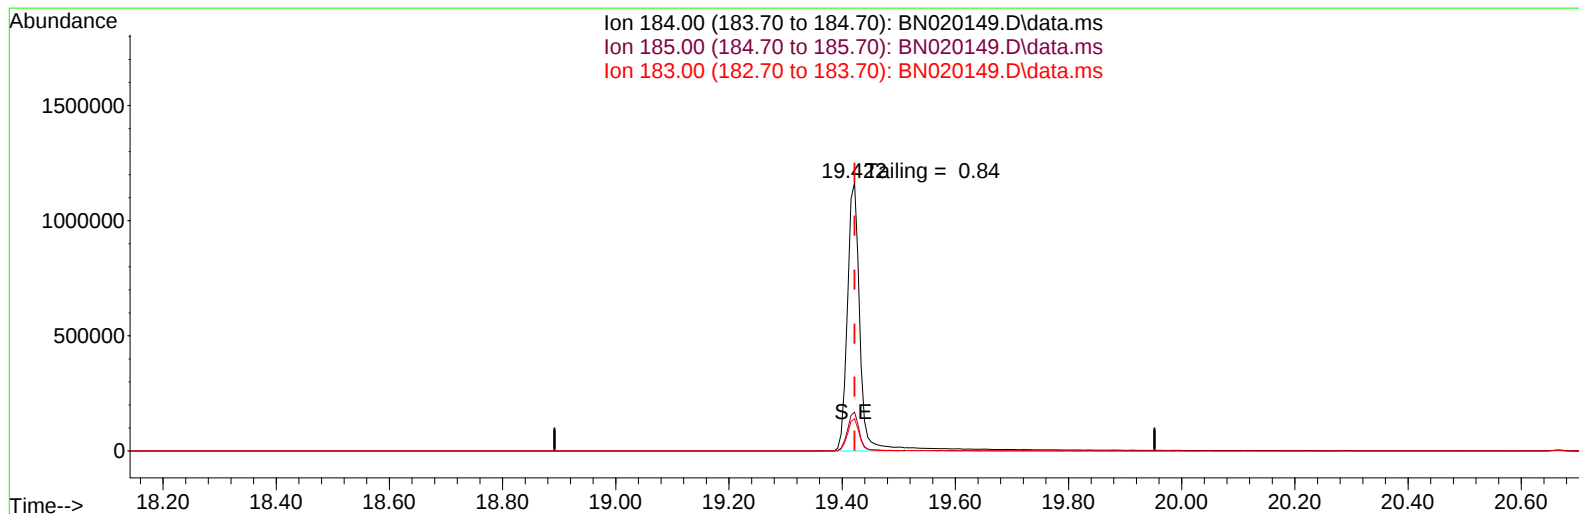

TIC: BN020149.D\data.ms

(77) Benzidine**19.422min (0.000) 916952.65 ng****response 1808986**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.55
183.00	13.20	12.03
0.00	0.00	0.00