
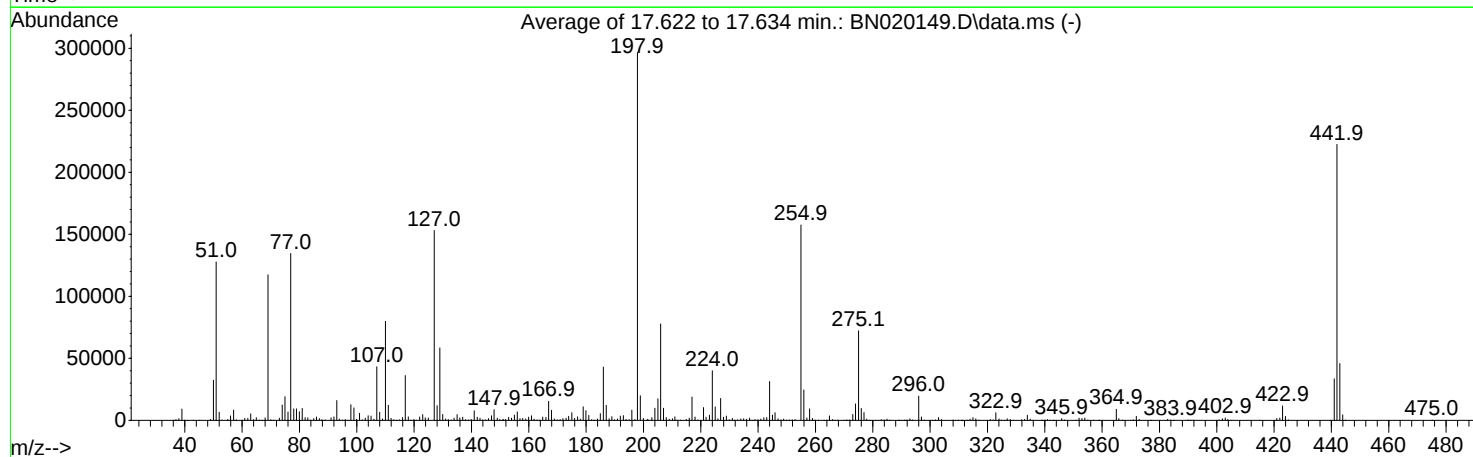


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061422\
 Data File : BN020149.D
 Acq On : 14 Jun 2022 09:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 14 16:17:22 2022

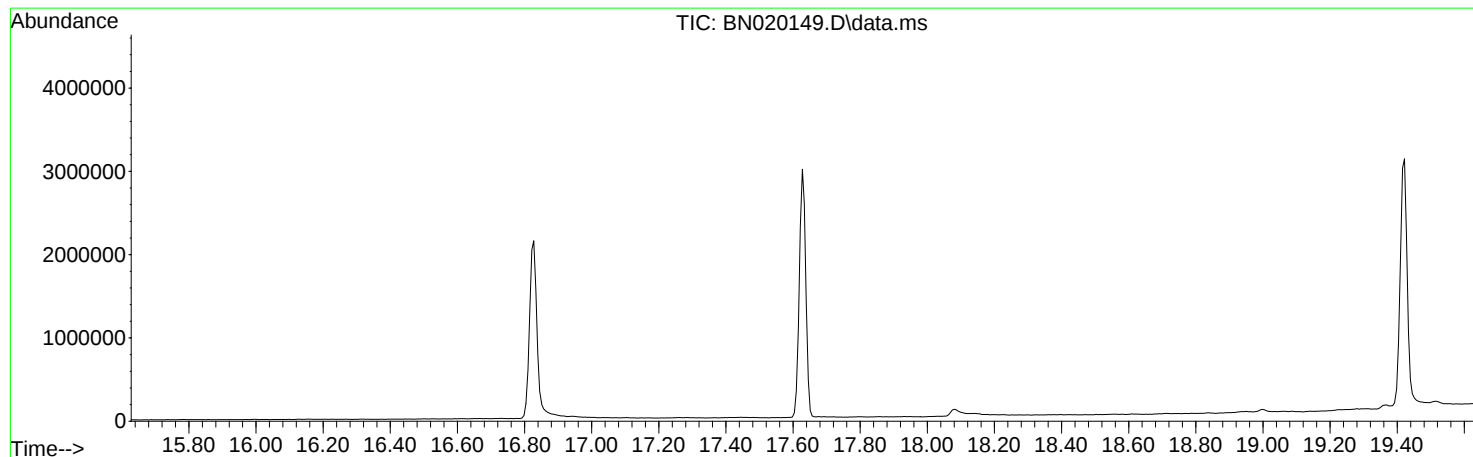




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	127766	PASS
68	69	0.00	2	1.8	2101	PASS
69	198	0.00	100	39.6	117467	PASS
70	69	0.00	2	0.5	568	PASS
127	198	10	80	51.6	153109	PASS
197	198	0.00	2	0.2	639	PASS
198	198	100	100	100.0	296619	PASS
199	198	5	9	6.7	19891	PASS
275	198	10	60	24.4	72227	PASS
365	198	1	100	3.0	8969	PASS
441	198	0.01	100	11.3	33611	PASS
442	442	50	100	100.0	222549	PASS
443	442	15	24	20.6	45795	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061422\
 Data File : BN020149.D
 Acq On : 14 Jun 2022 09:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 14 13:27:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 14 13:27:42 2022
 Response via : Initial Calibration

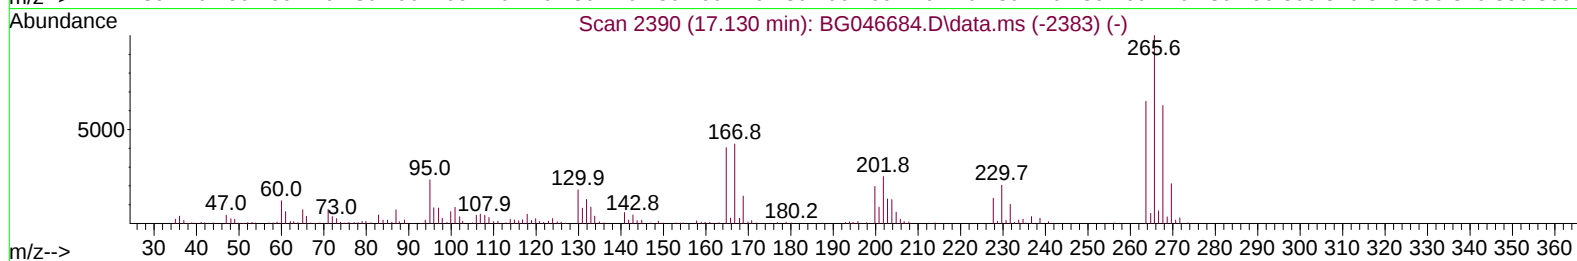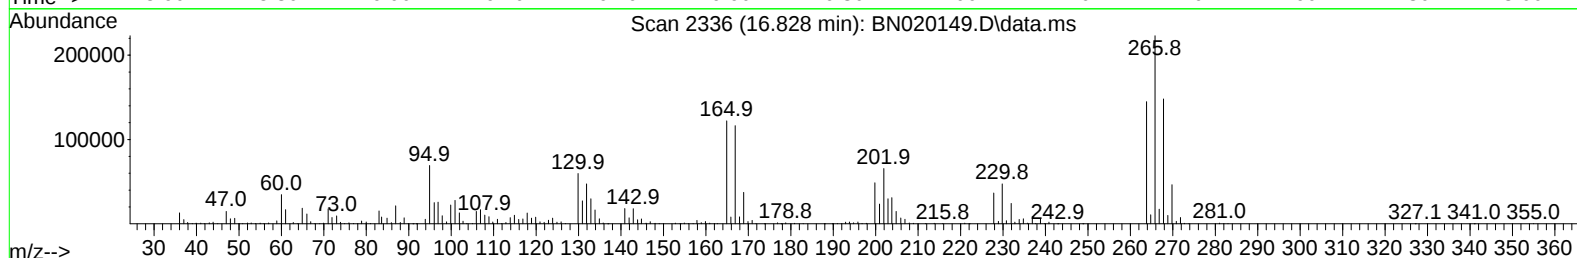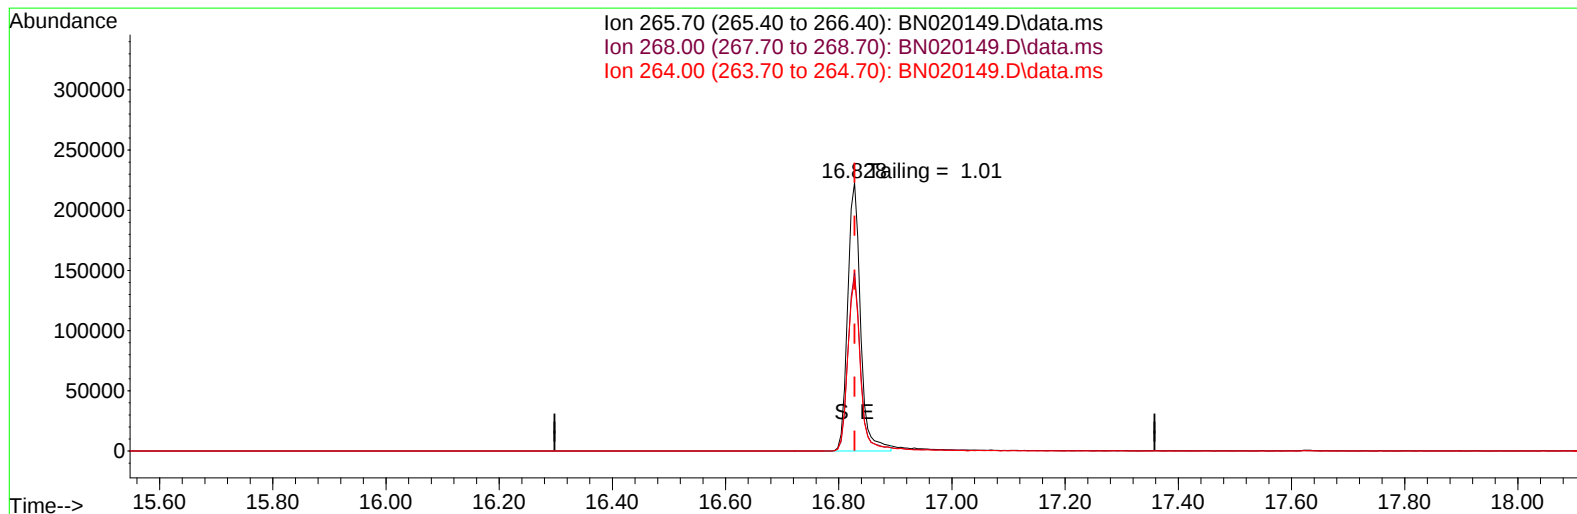

TIC: BN020149.D\data.ms

(70) Pentachlorophenol (C)

16.828min (0.000) 22939.47 ng




response 364367

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.39
264.00	61.60	64.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061422\
Data File : BN020149.D
Acq On : 14 Jun 2022 09:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 14 13:27:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 14 13:27:42 2022
Response via : Initial Calibration

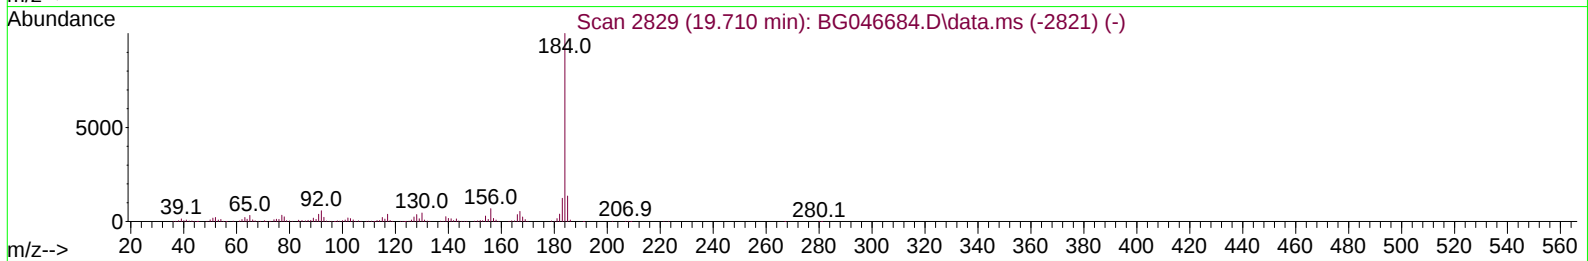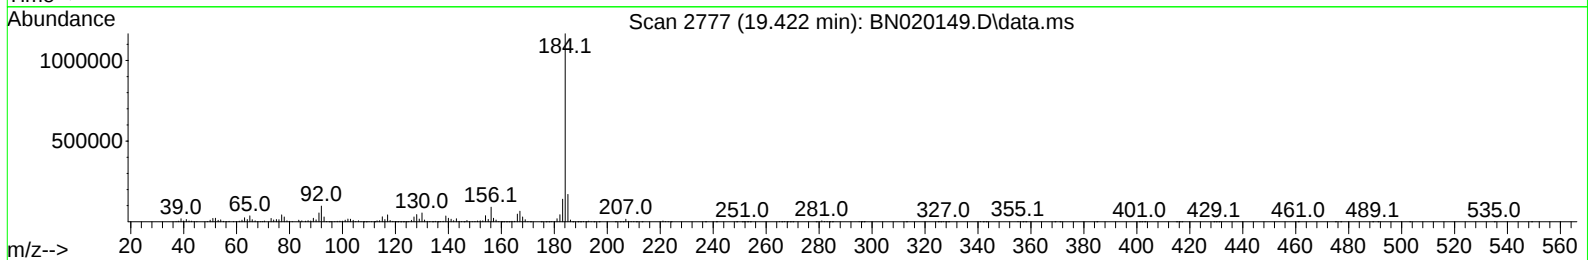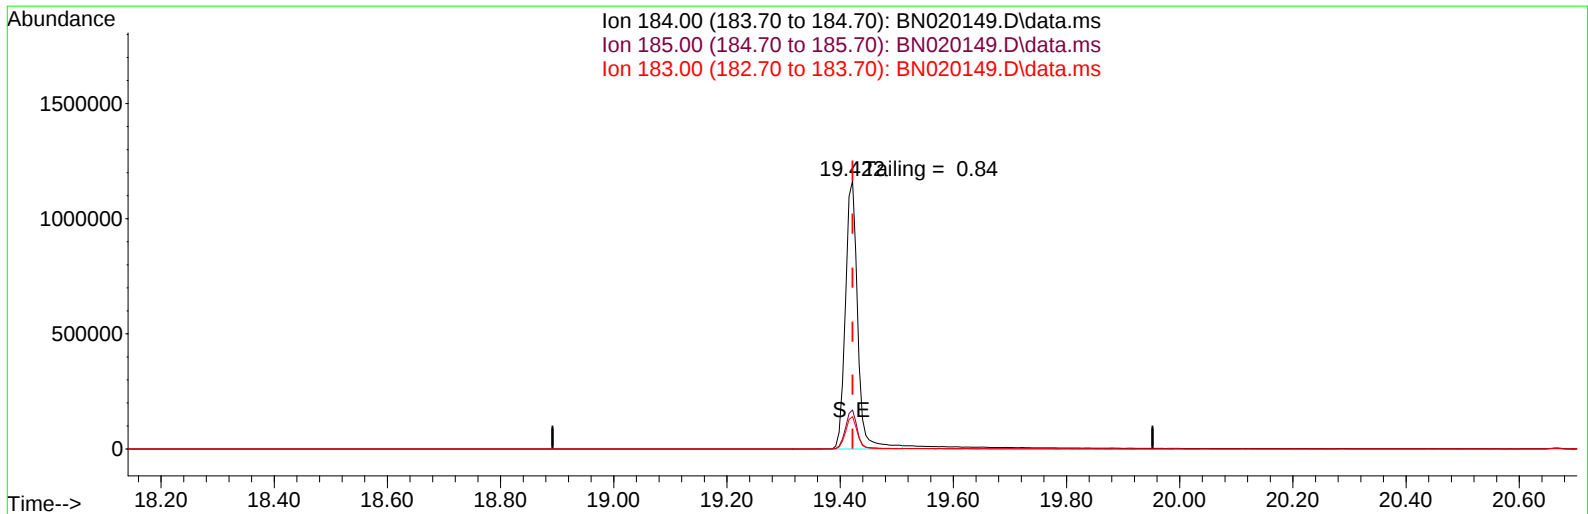

TIC: BN020149.D\data.ms

(77) Benzidine

19.422min (0.000) 916952.65 ng

response 1808986

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.55
183.00	13.20	12.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/14/2022	BNA_N	<u>BN020149.D</u>
Compound Name	Response	Retention Time
DDT	983640	20.66
DDD	18785	20.22
DDE	1382	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20167	1003807	2.01

Instrument :
BNA_N
ClientSampleId :
DFTPP