

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
 Data File : BN032010.D
 Acq On : 14 Jun 2024 21:06
 Operator : MA/JU
 Sample : P2696-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4BN5

Quant Time: Jun 14 22:46:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 11 22:28:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.652	152	295851	20.000	ng/u1	0.00
20) Naphthalene-d8	10.434	136	1346768	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.298	164	924688	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.051	188	1921537	20.000	ng/u1	0.00
79) Chrysene-d12	21.280	240	1369420	20.000	ng/u1	-0.01
88) Perylene-d12	24.210	264	1223996	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.176	96	20524	2.870	ng/uL	0.00
4) Pyridine-d5	3.581	84	298916	14.849	ng/u1	0.00
7) Phenol-d5	6.834	99	416663	16.428	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	241562	16.283	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.187	132	342749	17.711	ng/u1	0.00
15) 4-Methylphenol-d8	8.364	113	355080	17.175	ng/u1	0.00
21) Nitrobenzene-d5	8.811	128	174607	16.956	ng/u1	0.00
24) 2-Nitrophenol-d4	9.528	143	186478	17.531	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.063	165	329085	16.572	ng/u1	0.00
31) 4-Chloroaniline-d4	10.581	131	506369	17.174	ng/u1	0.00
46) Dimethylphthalate-d6	13.716	166	1106493	17.176	ng/u1	0.00
49) Acenaphthylene-d8	13.993	160	1287016	17.375	ng/u1	0.00
54) 4-Nitrophenol-d4	14.522	143	183306	14.212	ng/u1	0.00
60) Fluorene-d10	15.298	176	948968	17.410	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.428	200	107080	11.087	ng/u1	0.00
73) Anthracene-d10	17.145	188	1467229	17.835	ng/u1	0.00
81) Pyrene-d10	19.445	212	1600410	21.839	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	999535	17.102	ng/u1	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.192	149	68252	1.103	ng/u1	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
Data File : BN032010.D
Acq On : 14 Jun 2024 21:06
Operator : MA/JU
Sample : P2696-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BN5


Quant Time: Jun 14 22:46:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 11 22:28:10 2024
Response via : Initial Calibration

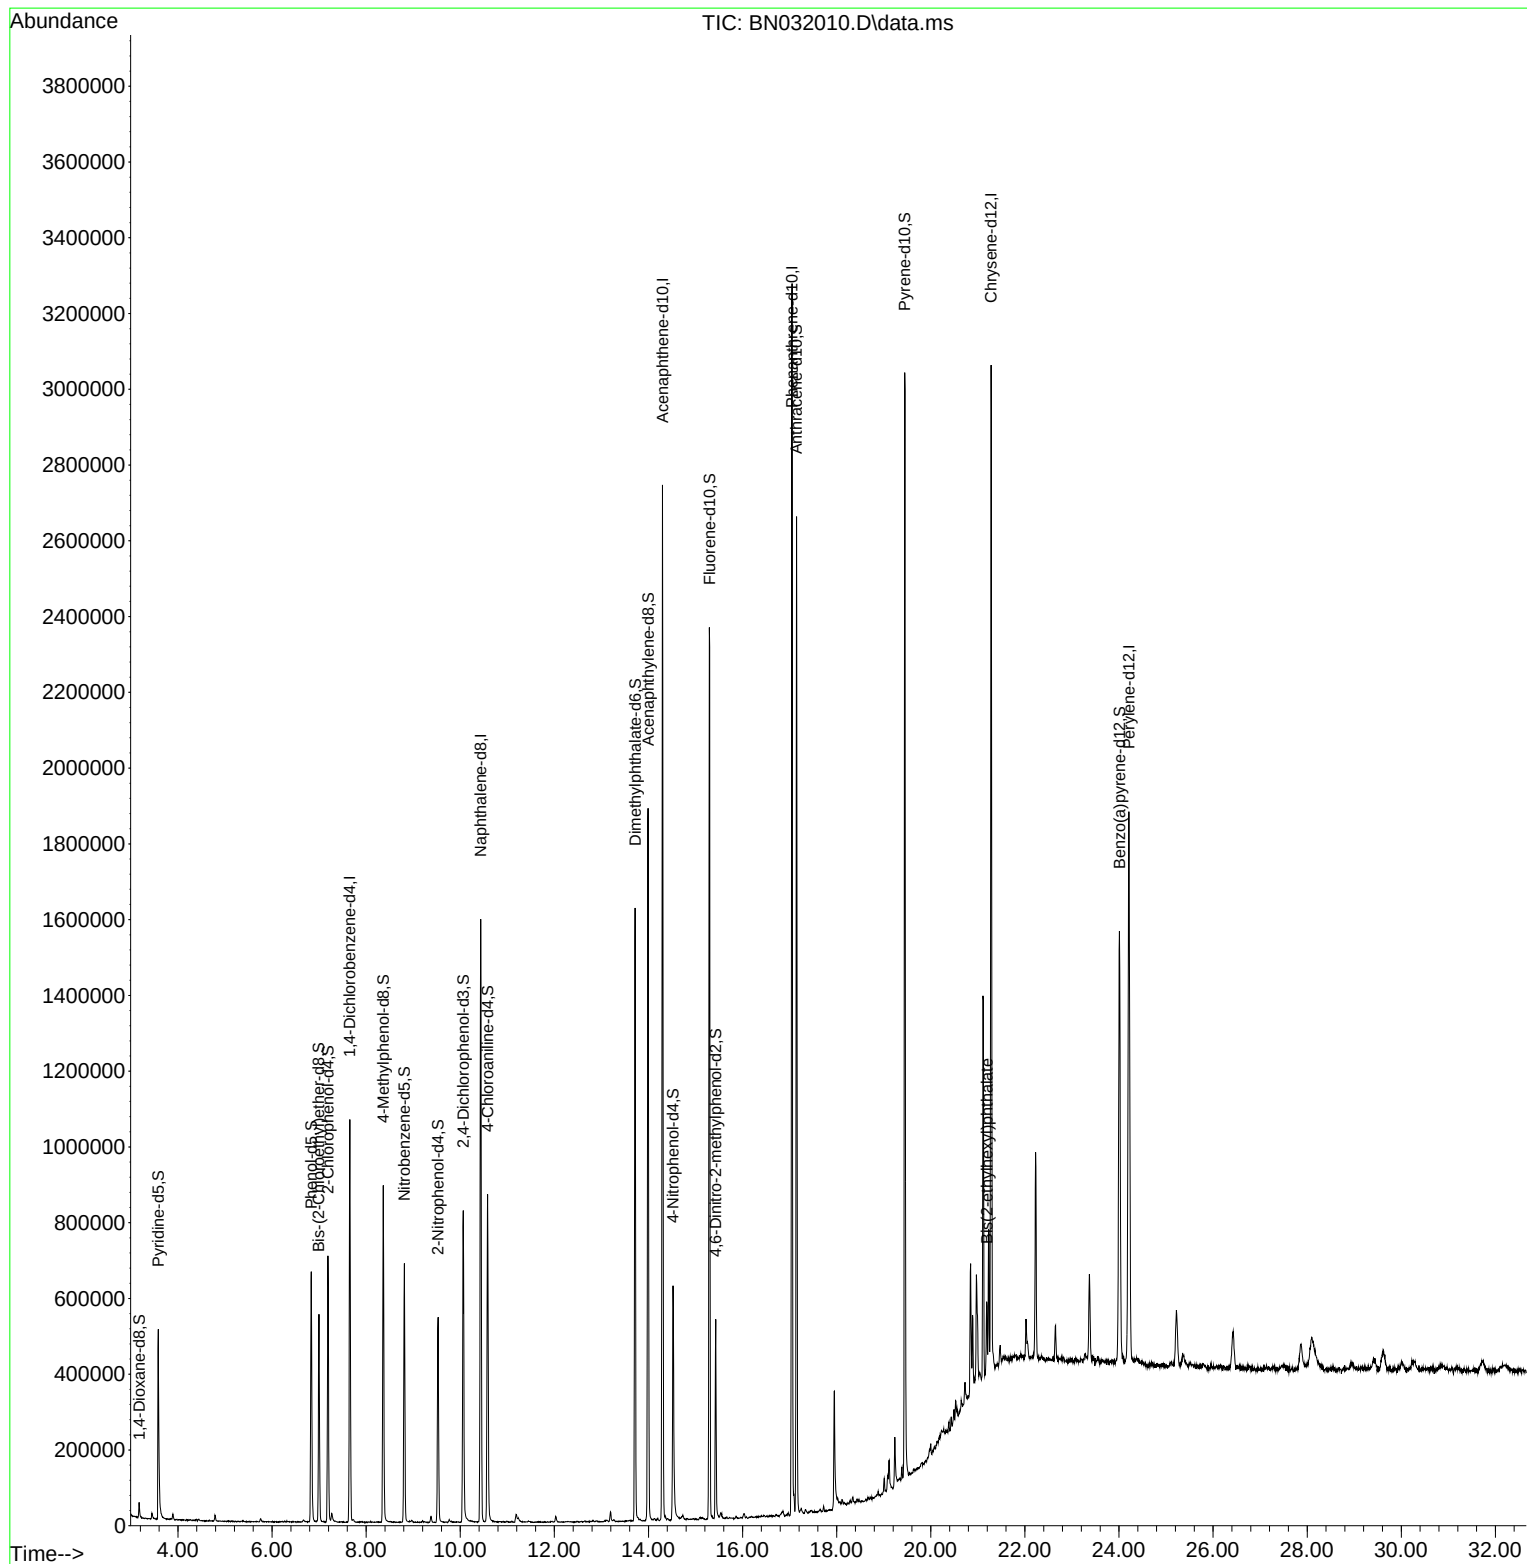

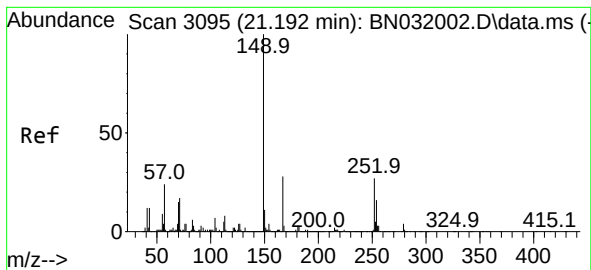

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.103 ng/ul
 RT: 21.192 min Scan# 3095
 Delta R.T. -0.011 min
 Lab File: BN032010.D
 Acq: 14 Jun 2024 21:06

Instrument :
 BNA_N
 ClientSampleId :
 A4BN5

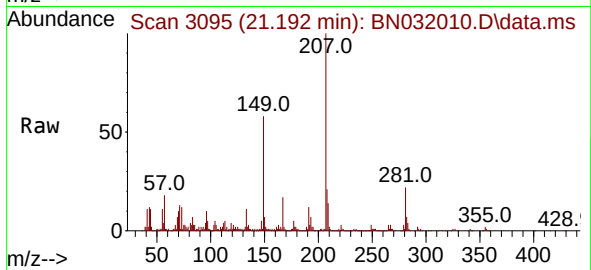

Tgt Ion:149 Resp: 68252

Ion	Ratio	Lower	Upper
149	100		
167	29.3	21.4	32.0
279	4.3	3.3	4.9

