

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
 Data File : BN032014.D
 Acq On : 14 Jun 2024 23:44
 Operator : MA/JU
 Sample : P2696-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4BN2

Quant Time: Jun 15 00:13:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 11 22:28:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.652	152	293211	20.000	ng/u1	0.00
20) Naphthalene-d8	10.434	136	1358726	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.298	164	927511	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.051	188	1891002	20.000	ng/u1	0.00
79) Chrysene-d12	21.280	240	1251303	20.000	ng/u1	-0.01
88) Perylene-d12	24.204	264	1208577	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	29962	4.227	ng/uL	0.00
4) Pyridine-d5	3.581	84	426063	21.356	ng/u1	0.00
7) Phenol-d5	6.834	99	627123	24.949	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	363056	24.693	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.187	132	501018	26.122	ng/u1	0.00
15) 4-Methylphenol-d8	8.363	113	549765	26.831	ng/u1	0.00
21) Nitrobenzene-d5	8.810	128	269774	25.968	ng/u1	0.00
24) 2-Nitrophenol-d4	9.528	143	295382	27.525	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.063	165	521979	26.054	ng/u1	0.00
31) 4-Chloroaniline-d4	10.581	131	781513	26.273	ng/u1	0.00
46) Dimethylphthalate-d6	13.716	166	1811609	28.037	ng/u1	0.00
49) Acenaphthylene-d8	13.993	160	2086805	28.087	ng/u1	0.00
54) 4-Nitrophenol-d4	14.522	143	320709	24.789	ng/u1	0.00
60) Fluorene-d10	15.292	176	1526519	27.921	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.428	200	204202	21.483	ng/u1	0.00
73) Anthracene-d10	17.145	188	2347193	28.993	ng/u1	0.00
81) Pyrene-d10	19.445	212	2456699	36.689	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	1650107	28.593	ng/u1	-0.01
Target Compounds						
80) Fluoranthene	19.110	202	91852	1.148	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
Data File : BN032014.D
Acq On : 14 Jun 2024 23:44
Operator : MA/JU
Sample : P2696-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BN2

Quant Time: Jun 15 00:13:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 11 22:28:10 2024
Response via : Initial Calibration

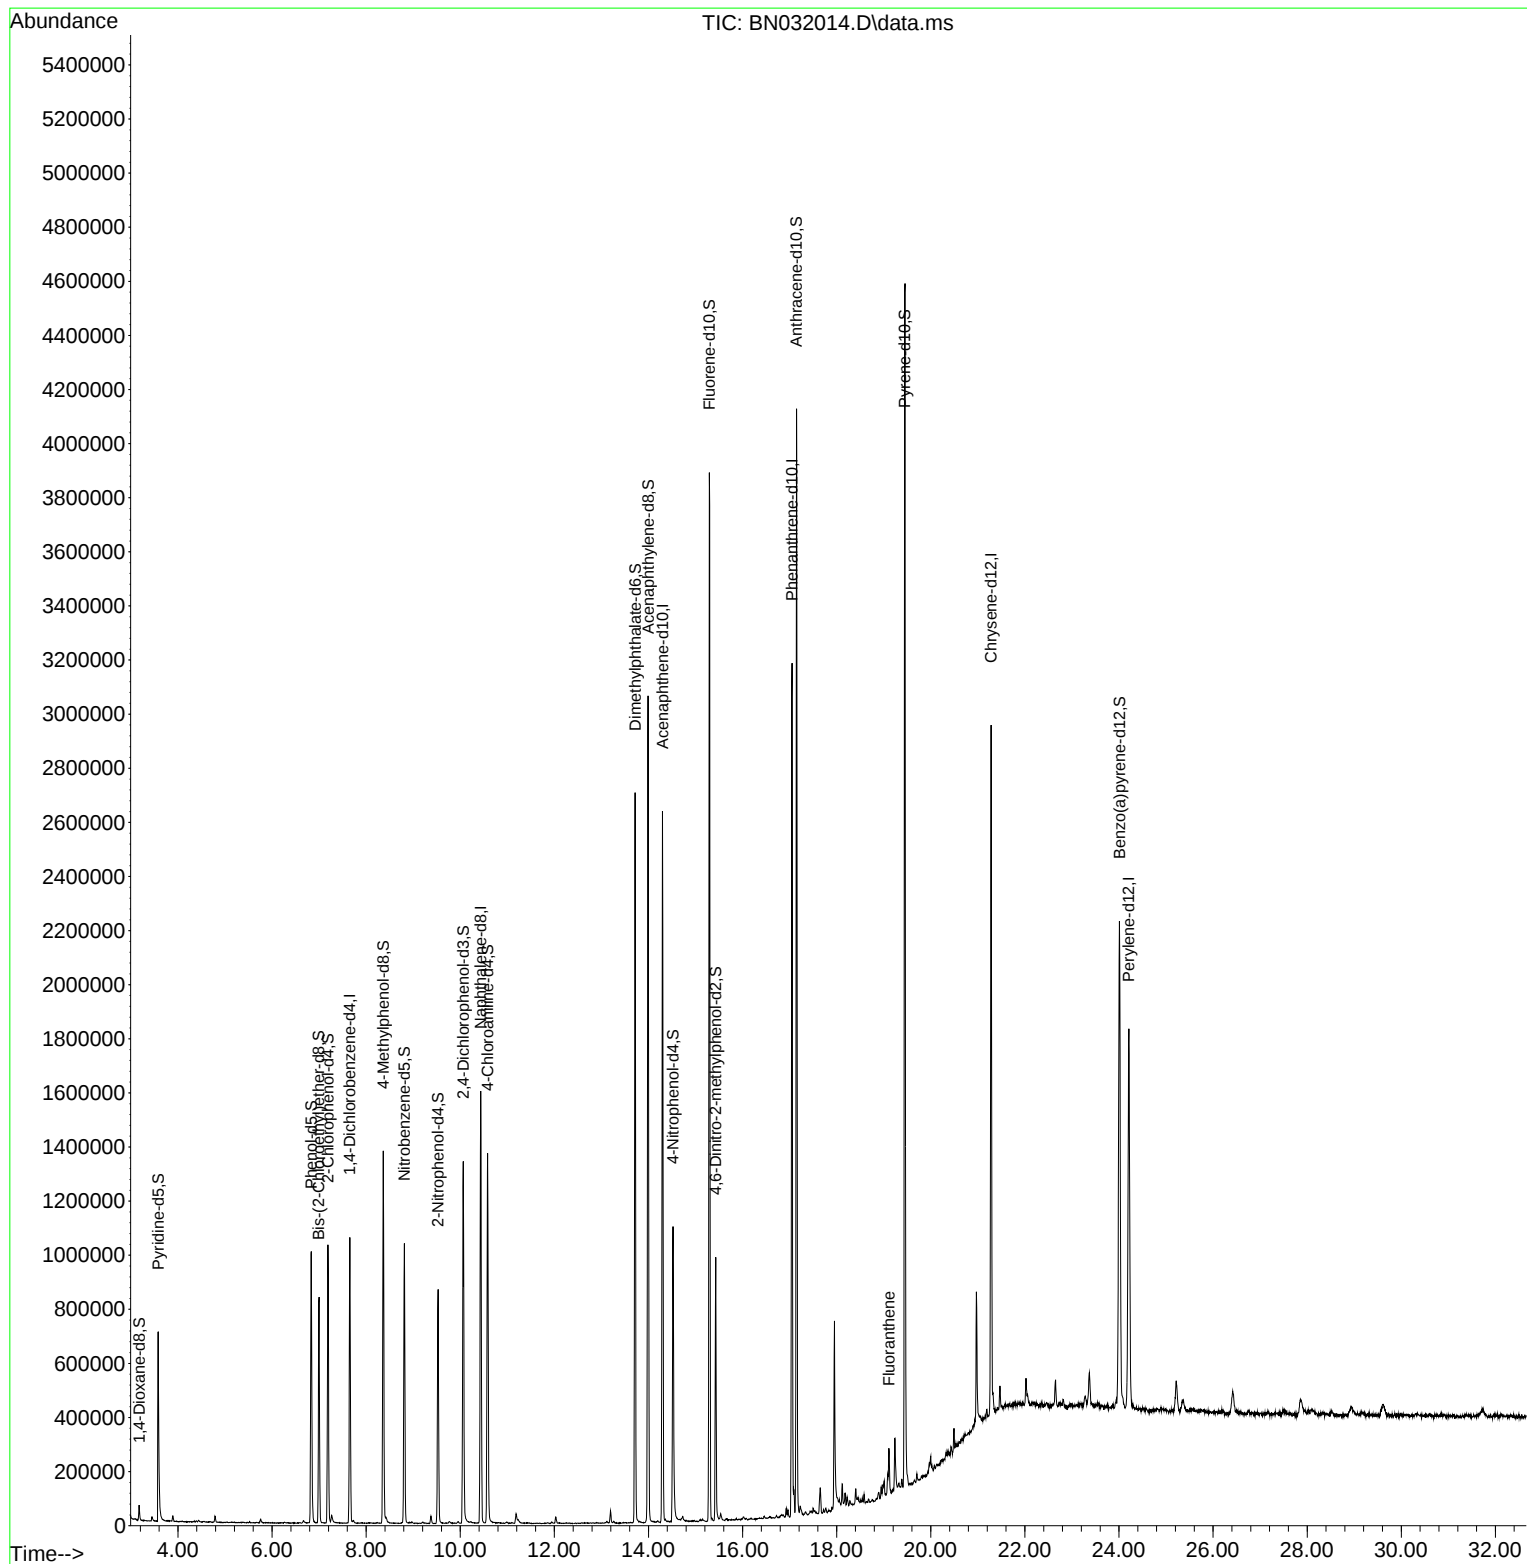

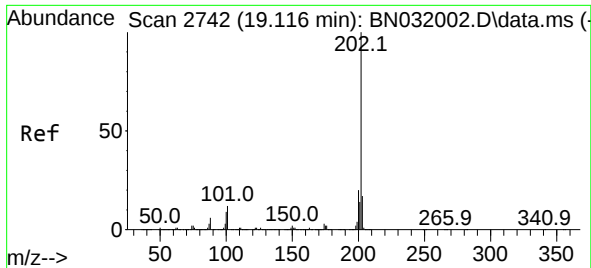

#80
 Fluoranthene
 Concen: 1.148 ng/ul
 RT: 19.110 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BN032014.D
 Acq: 14 Jun 2024 23:44

Instrument :
 BNA_N
 ClientSampleId :
 A4BN2

Tgt Ion:202 Resp: 91852
 Ion Ratio Lower Upper
 202 100
 101 12.2 10.3 15.5
 100 9.9 8.0 12.0

