

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
 Data File : BN032003.D
 Acq On : 14 Jun 2024 16:30
 Operator : MA/JU
 Sample : PB161357BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK357

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	28	32	39	rBV	76846	103064	1.27%	0.126%
2	3.576	98	100	118	rBV	934196	1442279	17.71%	1.765%
3	3.893	149	154	158	rBV	14518	19625	0.24%	0.024%
4	6.834	646	654	669	rBV	1169399	1909649	23.45%	2.336%
5	6.999	672	682	694	rBV	1019924	1595569	19.59%	1.952%
6	7.187	707	714	732	rBV	1231617	1998007	24.53%	2.445%
7	7.652	785	793	807	rBV	988838	1604877	19.70%	1.964%
8	8.363	906	914	927	rBV	1558939	2558772	31.42%	3.131%
9	8.811	982	990	1000	rBV	1207324	2002577	24.59%	2.450%
10	9.528	1101	1112	1125	rBV	1021587	1693865	20.80%	2.072%
11	10.063	1195	1203	1219	rBV	1443385	2565683	31.50%	3.139%
12	10.434	1257	1266	1277	rBV	1483090	2543009	31.22%	3.111%
13	10.581	1282	1291	1306	rBV	1611907	2831280	34.76%	3.464%
14	11.246	1399	1404	1409	rBV6	5313	12023	0.15%	0.015%
15	12.034	1531	1538	1546	rBV2	24362	47944	0.59%	0.059%
16	13.716	1817	1824	1835	rBV	3181232	4416805	54.23%	5.404%
17	13.993	1864	1871	1883	rBV2	3359390	5188627	63.70%	6.348%
18	14.298	1916	1923	1939	rBV	2548589	3826734	46.98%	4.682%
19	14.416	1939	1943	1948	rVB8	4659	8901	0.11%	0.011%
20	14.522	1954	1961	1982	rBV	1290385	2240812	27.51%	2.742%
21	15.298	2085	2093	2102	rBV	4224864	6392293	78.48%	7.821%
22	15.428	2108	2115	2129	rBV	1404767	1952011	23.97%	2.388%
23	15.534	2129	2133	2140	rVB	25326	42414	0.52%	0.052%
24	16.728	2331	2336	2340	rBV6	6412	10066	0.12%	0.012%
25	16.834	2351	2354	2361	rVB	8078	13008	0.16%	0.016%
26	17.051	2384	2391	2400	rBV	3151779	4744652	58.25%	5.805%
27	17.151	2400	2408	2418	rBV	4892072	7137430	87.63%	8.733%
28	17.434	2453	2456	2460	rBV3	7761	11690	0.14%	0.014%
29	17.716	2500	2504	2509	rBV8	6185	11760	0.14%	0.014%
30	17.951	2539	2544	2553	rBV3	37387	72201	0.89%	0.088%
31	19.010	2720	2724	2730	rBV2	65239	91887	1.13%	0.112%
32	19.081	2732	2736	2742	rBV	65962	99656	1.22%	0.122%
33	19.239	2760	2763	2771	rBV8	20208	34686	0.43%	0.042%
34	19.386	2785	2788	2792	rVB2	23675	28231	0.35%	0.035%
35	19.451	2792	2799	2811	rBV	5771224	8144878	100.00%	9.965%
36	21.286	3105	3111	3118	rBV	3062670	4497959	55.22%	5.503%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
Data File : BN032003.D
Acq On : 14 Jun 2024 16:30
Operator : MA/JU
Sample : PB161357BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK357

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	24.016	3567	3575	3584	rVB2	2332604	5666639	69.57%	6.933%
38	24.216	3601	3609	3622	rVB2	1612361	4170223	51.20%	5.102%




Sum of corrected areas: 81731786

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
Data File : BN032003.D
Acq On : 14 Jun 2024 16:30
Operator : MA/JU
Sample : PB161357BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK357

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

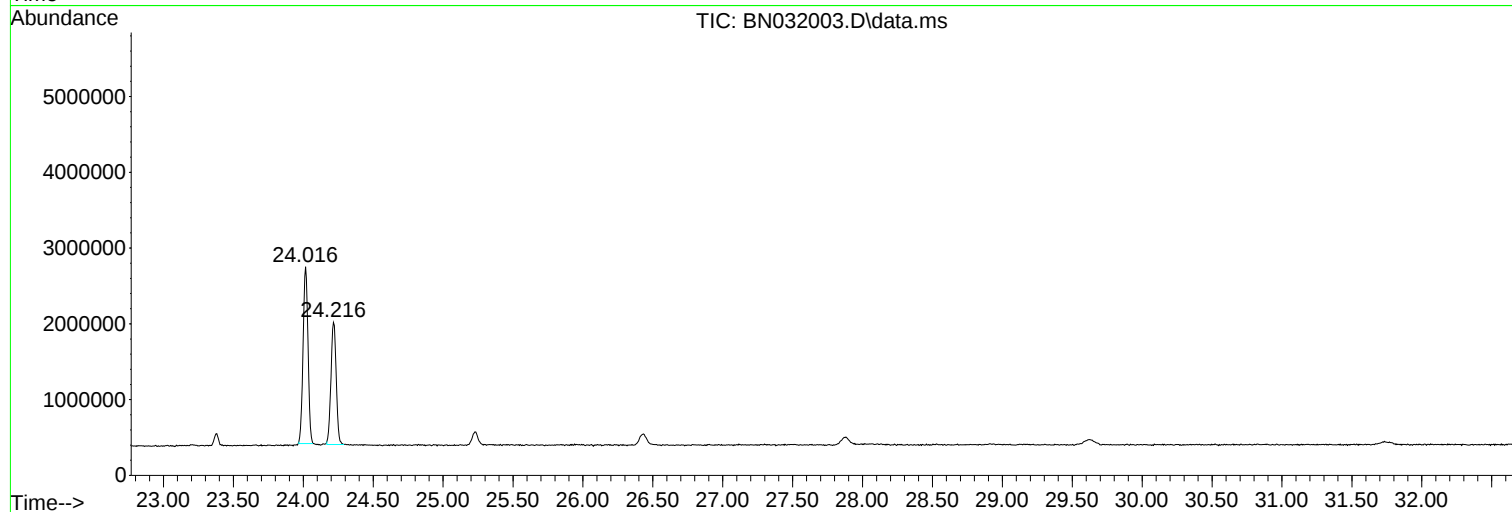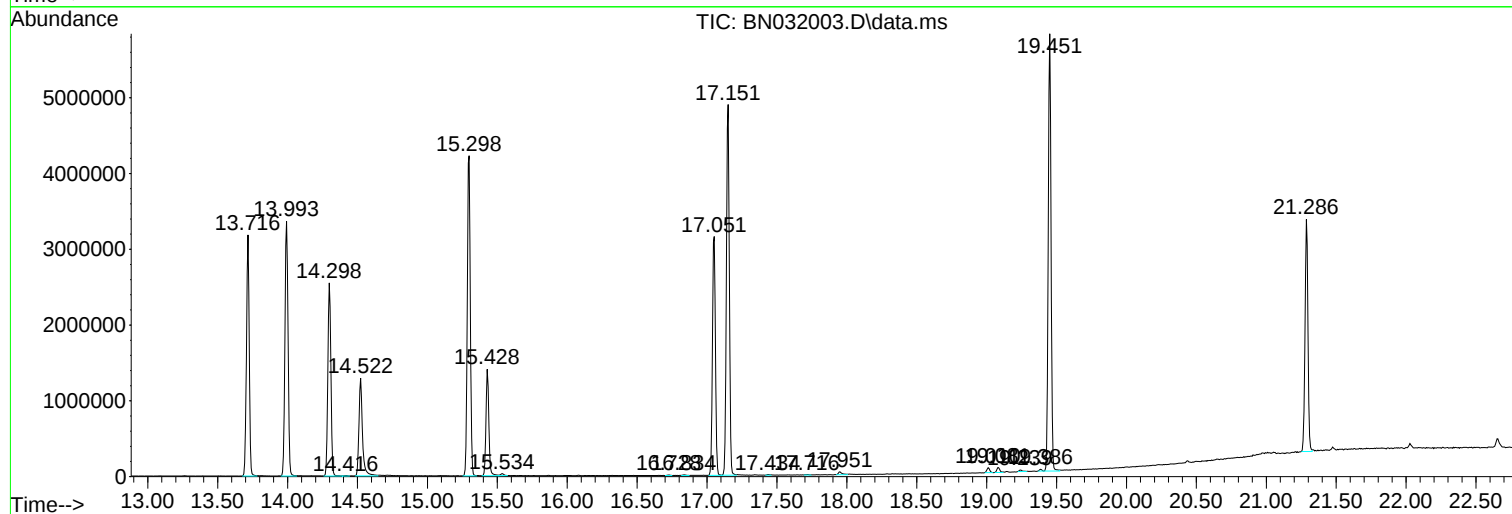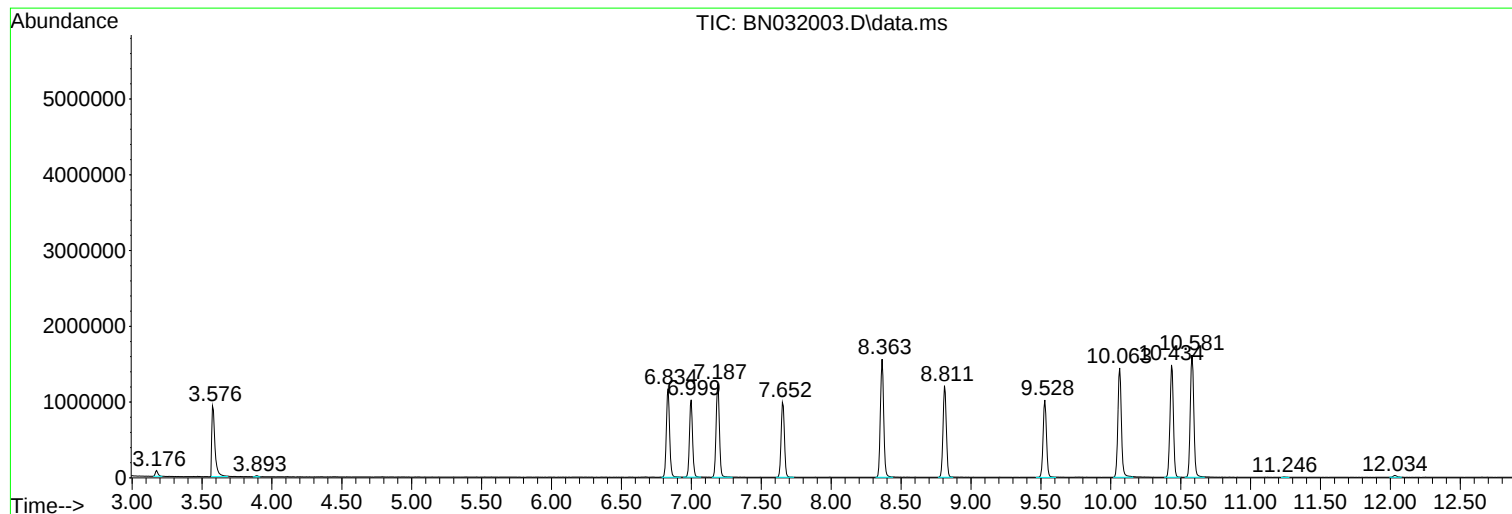

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
Data File : BN032003.D
Acq On : 14 Jun 2024 16:30
Operator : MA/JU
Sample : PB161357BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK357

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
Data File : BN032003.D
Acq On : 14 Jun 2024 16:30
Operator : MA/JU
Sample : PB161357BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK357

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------