

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
 Data File : BN032018.D
 Acq On : 15 Jun 2024 03:01
 Operator : MA/JU
 Sample : PB161388BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK388

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	43	rVB	91957	118982	1.87%	0.160%
2	3.575	98	100	126	rBV	1092808	1745275	27.49%	2.340%
3	3.893	150	154	160	rVB	15184	22882	0.36%	0.031%
4	6.834	647	654	666	rBV	1323569	2200208	34.66%	2.950%
5	6.999	675	682	695	rVB	1108657	1778400	28.01%	2.385%
6	7.187	705	714	726	rBV	1381040	2299130	36.22%	3.083%
7	7.651	786	793	804	rBV	1000725	1641277	25.85%	2.201%
8	8.363	906	914	929	rBV	1727699	2826185	44.52%	3.790%
9	8.810	982	990	1002	rBV	1345146	2189461	34.49%	2.936%
10	9.528	1104	1112	1128	rBV	1079970	1829029	28.81%	2.453%
11	10.063	1195	1203	1221	rBV	1556217	2821253	44.44%	3.783%
12	10.434	1258	1266	1280	rVB	1468214	2493131	39.27%	3.343%
13	10.581	1283	1291	1304	rBV	1668900	2926385	46.10%	3.924%
14	11.240	1396	1403	1406	rBV9	3858	8594	0.14%	0.012%
15	12.034	1532	1538	1547	rBV2	24795	50824	0.80%	0.068%
16	13.716	1816	1824	1837	rBV	2667040	3877678	61.08%	5.200%
17	13.992	1863	1871	1884	rBV	3128070	4850722	76.41%	6.504%
18	14.298	1916	1923	1933	rBV	2152424	3209542	50.56%	4.304%
19	14.522	1954	1961	1981	rBV	974890	1771341	27.90%	2.375%
20	15.292	2084	2092	2108	rBV	3806157	5633685	88.74%	7.554%
21	15.428	2108	2115	2128	rVV	936841	1366641	21.53%	1.833%
22	15.533	2128	2133	2141	rVB	20868	36860	0.58%	0.049%
23	15.863	2186	2189	2194	rVB6	3836	6366	0.10%	0.009%
24	16.833	2350	2354	2359	rVB2	5585	9622	0.15%	0.013%
25	17.045	2384	2390	2399	rBV	2288674	3361692	52.96%	4.508%
26	17.145	2401	2407	2418	rBV2	3844200	5585964	87.99%	7.490%
27	17.339	2436	2440	2442	rBV5	6346	8720	0.14%	0.012%
28	17.433	2454	2456	2461	rVB5	6048	9085	0.14%	0.012%
29	17.951	2540	2544	2550	rBV6	11225	21002	0.33%	0.028%
30	19.010	2720	2724	2731	rVB3	48466	71100	1.12%	0.095%
31	19.080	2731	2736	2742	rBV	47431	81703	1.29%	0.110%
32	19.380	2785	2787	2790	rVB3	15921	16114	0.25%	0.022%
33	19.451	2792	2799	2808	rBV	4204842	5951220	93.75%	7.980%
34	21.280	3105	3110	3117	rBV2	2232130	3301623	52.01%	4.427%
35	24.009	3565	3574	3586	rVB2	2615383	6348180	100.00%	8.512%
36	24.209	3600	3608	3622	rVB	1617989	4107673	64.71%	5.508%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
Data File : BN032018.D
Acq On : 15 Jun 2024 03:01
Operator : MA/JU
Sample : PB161388BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK388

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 74577549

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
Data File : BN032018.D
Acq On : 15 Jun 2024 03:01
Operator : MA/JU
Sample : PB161388BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

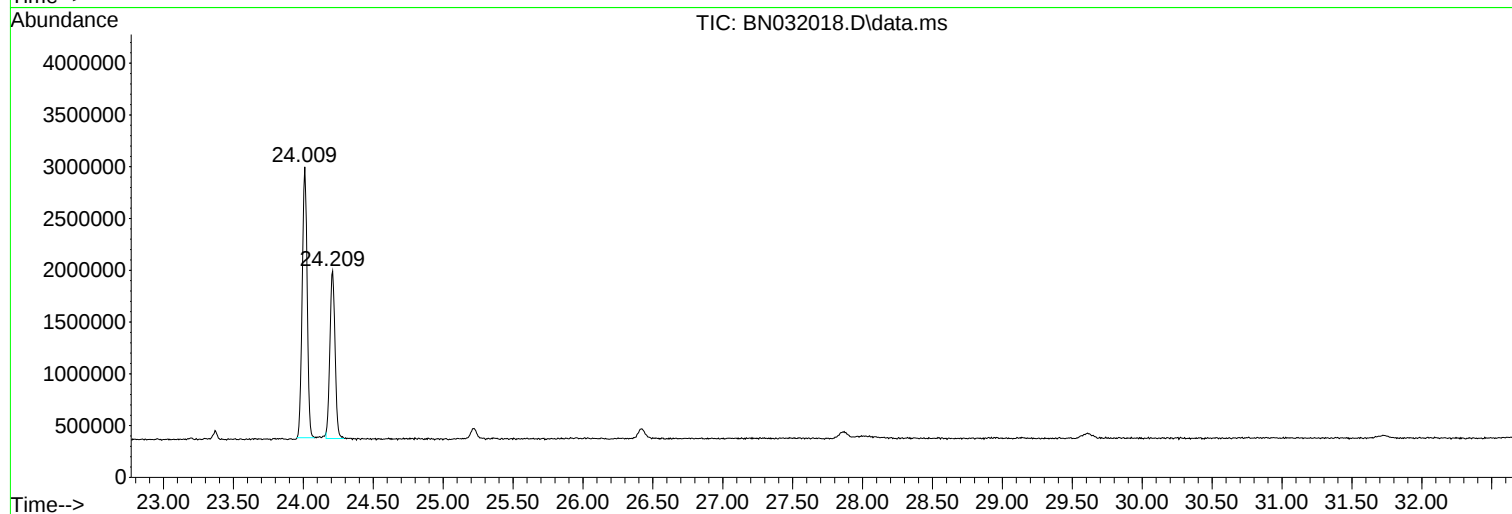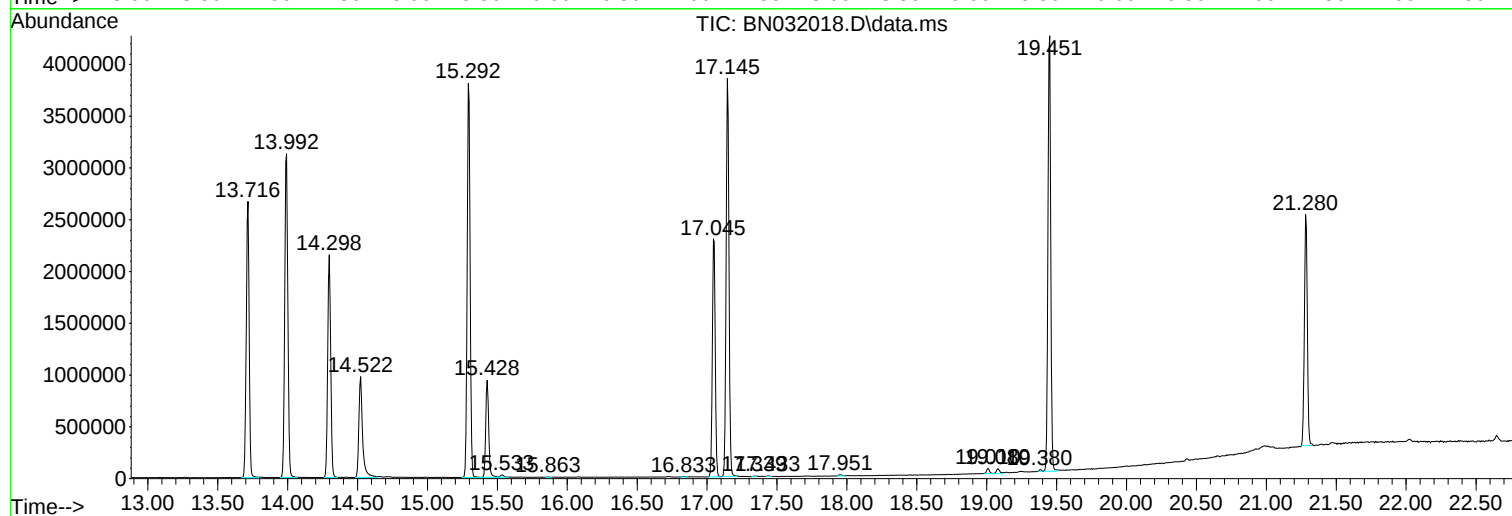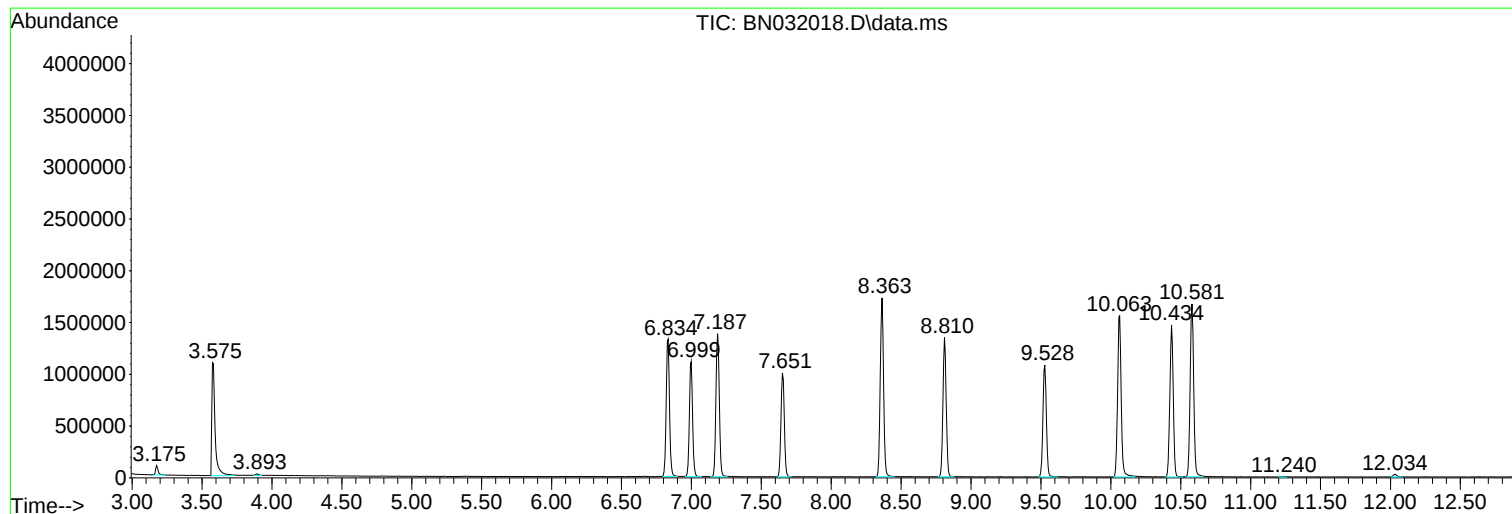

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
Data File : BN032018.D
Acq On : 15 Jun 2024 03:01
Operator : MA/JU
Sample : PB161388BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
Data File : BN032018.D
Acq On : 15 Jun 2024 03:01
Operator : MA/JU
Sample : PB161388BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc