

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
 Data File : BN032019.D
 Acq On : 15 Jun 2024 03:41
 Operator : MA/JU
 Sample : P2696-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4BN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	38	rBV	46417	64332	1.18%	0.098%
2	3.446	75	78	83	rBV	9546	15283	0.28%	0.023%
3	3.575	97	100	116	rBV	585331	946780	17.33%	1.447%
4	3.893	149	154	162	rVB	79600	119254	2.18%	0.182%
5	4.393	233	239	243	rBV7	4184	7461	0.14%	0.011%
6	4.434	243	246	255	rVB3	5642	10328	0.19%	0.016%
7	4.787	301	306	312	rVB	17483	25600	0.47%	0.039%
8	5.046	343	350	353	rBV7	4224	9407	0.17%	0.014%
9	5.758	466	471	480	rVB2	9561	19567	0.36%	0.030%
10	6.669	618	626	631	rBV8	5130	12270	0.22%	0.019%
11	6.834	647	654	667	rVB	821607	1416878	25.93%	2.166%
12	6.993	674	681	695	rVB	676798	1096931	20.07%	1.677%
13	7.187	707	714	724	rBV	855172	1389970	25.44%	2.125%
14	7.269	724	728	738	rVB2	14235	30176	0.55%	0.046%
15	7.652	785	793	801	rBV	1246681	2001026	36.62%	3.059%
16	8.363	906	914	931	rBV	1085924	1864780	34.13%	2.850%
17	8.758	974	981	982	rBV6	4422	5475	0.10%	0.008%
18	8.810	983	990	1003	rVV	825508	1385570	25.36%	2.118%
19	8.969	1014	1017	1022	rVB6	3786	6572	0.12%	0.010%
20	9.199	1050	1056	1060	rBV5	4207	7693	0.14%	0.012%
21	9.381	1082	1087	1097	rVB	19046	32171	0.59%	0.049%
22	9.528	1103	1112	1122	rBV	664073	1146310	20.98%	1.752%
23	9.763	1146	1152	1153	rBV5	4173	5556	0.10%	0.008%
24	10.063	1194	1203	1225	rBV	1036982	1902768	34.82%	2.909%
25	10.434	1257	1266	1279	rBV	1886973	3224178	59.00%	4.928%
26	10.581	1282	1291	1303	rBV	1040818	1877380	34.36%	2.870%
27	10.963	1350	1356	1357	rBV6	3607	5548	0.10%	0.008%
28	10.987	1357	1360	1366	rVV8	4043	8020	0.15%	0.012%
29	11.187	1387	1394	1400	rBV2	30643	71434	1.31%	0.109%
30	12.028	1531	1537	1546	rBV3	19645	38719	0.71%	0.059%
31	13.122	1718	1723	1727	rBV6	8652	15437	0.28%	0.024%
32	13.193	1730	1735	1740	rVV2	26900	44463	0.81%	0.068%
33	13.257	1744	1746	1753	rVB6	6574	9539	0.17%	0.015%
34	13.716	1817	1824	1837	rBV	1957443	2938534	53.78%	4.492%
35	13.804	1837	1839	1846	rVB7	5210	8777	0.16%	0.013%
36	13.993	1858	1871	1883	rBV	2251358	3649502	66.79%	5.579%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
 Data File : BN032019.D
 Acq On : 15 Jun 2024 03:41
 Operator : MA/JU
 Sample : P2696-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4BN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

37	14.298	1914	1923	1931	rBV	3102465	4653934	85.17%	7.114%
38	14.357	1931	1933	1938	rVV4	11913	15729	0.29%	0.024%
39	14.416	1940	1943	1948	rVB7	4944	6857	0.13%	0.010%
40	14.522	1953	1961	1975	rBV	777579	1426149	26.10%	2.180%
41	14.757	1999	2001	2006	rVB5	7620	10156	0.19%	0.016%
42	15.098	2053	2059	2061	rBV5	6670	10294	0.19%	0.016%
43	15.292	2085	2092	2100	rBV	3079449	4411560	80.73%	6.743%
44	15.351	2100	2102	2105	rVV4	6469	6571	0.12%	0.010%
45	15.428	2108	2115	2128	rBV	695450	1018901	18.65%	1.557%
46	15.534	2128	2133	2142	rVB2	18980	36942	0.68%	0.056%
47	15.863	2184	2189	2193	rBV8	4493	8607	0.16%	0.013%
48	16.016	2211	2215	2222	rVB7	6369	13859	0.25%	0.021%
49	16.081	2222	2226	2229	rVB6	4382	5546	0.10%	0.008%
50	16.187	2242	2244	2252	rVB8	4102	6460	0.12%	0.010%
51	16.328	2262	2268	2269	rBV5	4031	5620	0.10%	0.009%
52	16.463	2286	2291	2300	rBV9	12410	28974	0.53%	0.044%
53	16.716	2329	2334	2335	rBV5	5006	8175	0.15%	0.012%
54	16.834	2351	2354	2358	rVB3	5292	6530	0.12%	0.010%
55	16.922	2367	2369	2372	rBV4	4291	5697	0.10%	0.009%
56	16.969	2375	2377	2381	rVB5	7402	7463	0.14%	0.011%
57	17.045	2383	2390	2396	rBV	3647398	5464303	100.00%	8.353%
58	17.086	2396	2397	2401	rVV	63302	66725	1.22%	0.102%
59	17.145	2401	2407	2418	rVB	3200306	4581190	83.84%	7.003%
60	17.339	2438	2440	2448	rVB7	7940	11828	0.22%	0.018%
61	17.445	2453	2458	2459	rBV4	5726	9470	0.17%	0.014%
62	17.945	2536	2543	2553	rBV	266047	491405	8.99%	0.751%
63	18.116	2569	2572	2575	rBV4	10444	15158	0.28%	0.023%
64	19.010	2720	2724	2728	rVB3	44588	60290	1.10%	0.092%
65	19.080	2732	2736	2738	rBV	47495	69778	1.28%	0.107%
66	19.110	2738	2741	2749	rVB	151841	222055	4.06%	0.339%
67	19.233	2758	2762	2770	rBV3	89328	156634	2.87%	0.239%
68	19.380	2785	2787	2791	rVB2	33594	37041	0.68%	0.057%
69	19.445	2792	2798	2812	rVV	3594662	5198622	95.14%	7.947%
70	20.969	3054	3057	3066	rVB2	168817	255281	4.67%	0.390%
71	21.280	3104	3110	3116	rBV2	2999895	4444809	81.34%	6.794%
72	24.004	3566	3573	3582	rVB2	1345223	3197495	58.52%	4.888%
73	24.210	3600	3608	3621	rVB	1637771	4030357	73.76%	6.161%




Sum of corrected areas: 65420154

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
Data File : BN032019.D
Acq On : 15 Jun 2024 03:41
Operator : MA/JU
Sample : P2696-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

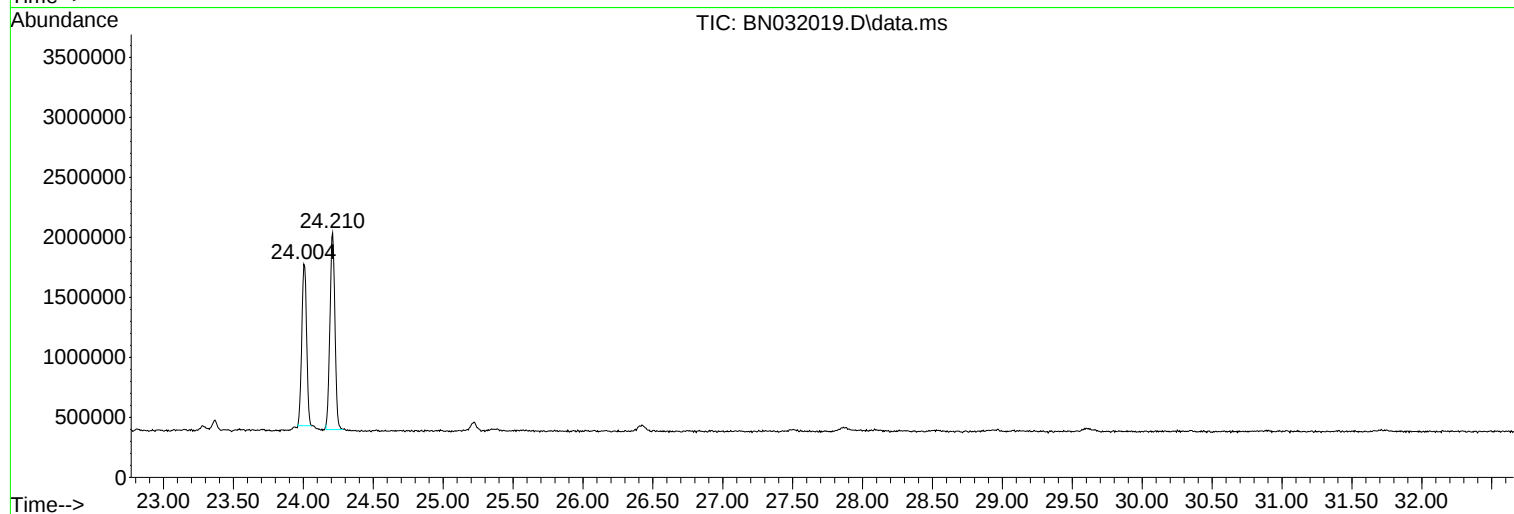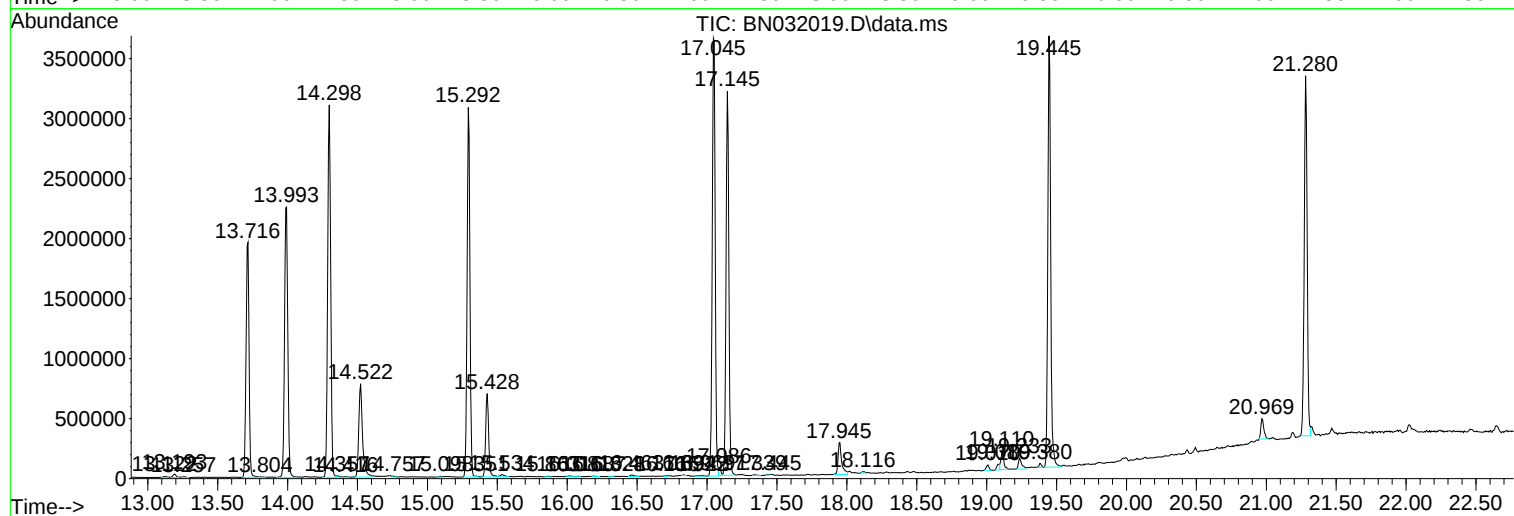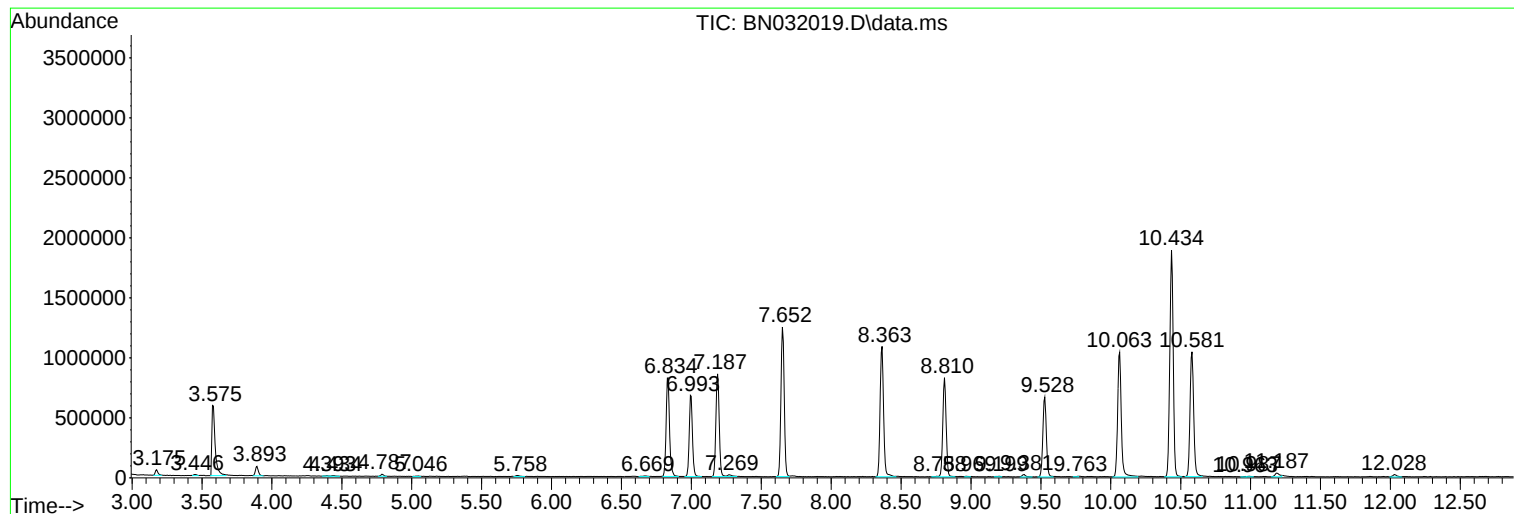

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
Data File : BN032019.D
Acq On : 15 Jun 2024 03:41
Operator : MA/JU
Sample : P2696-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061424\
Data File : BN032019.D
Acq On : 15 Jun 2024 03:41
Operator : MA/JU
Sample : P2696-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------