
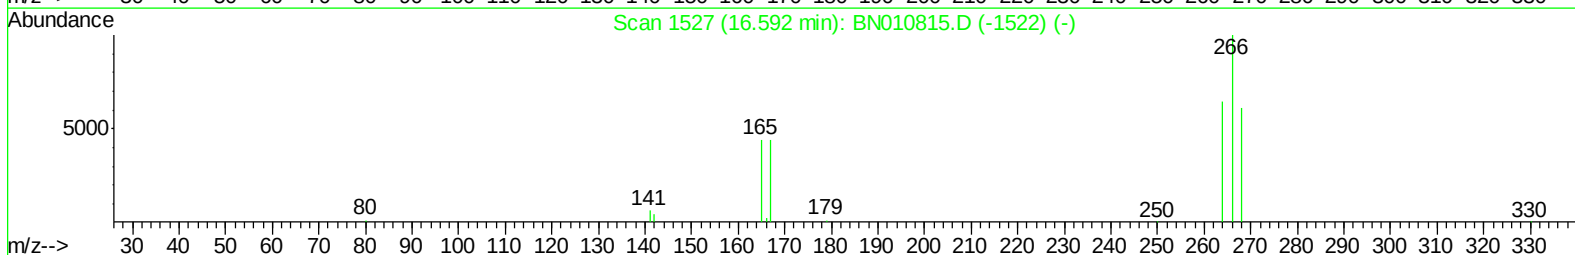
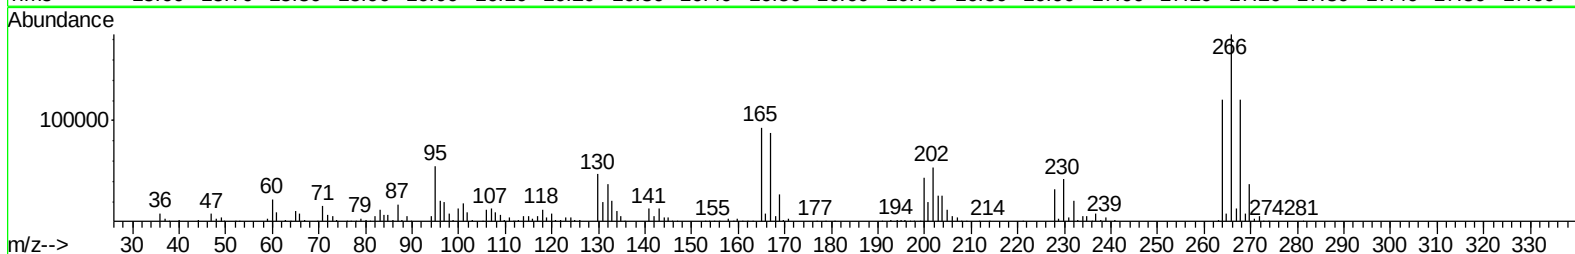


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061520\
 Data File : BN010883.D
 Acq On : 15 Jun 2020 23:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 00:29:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 11:09:46 2020
 Response via : Initial Calibration

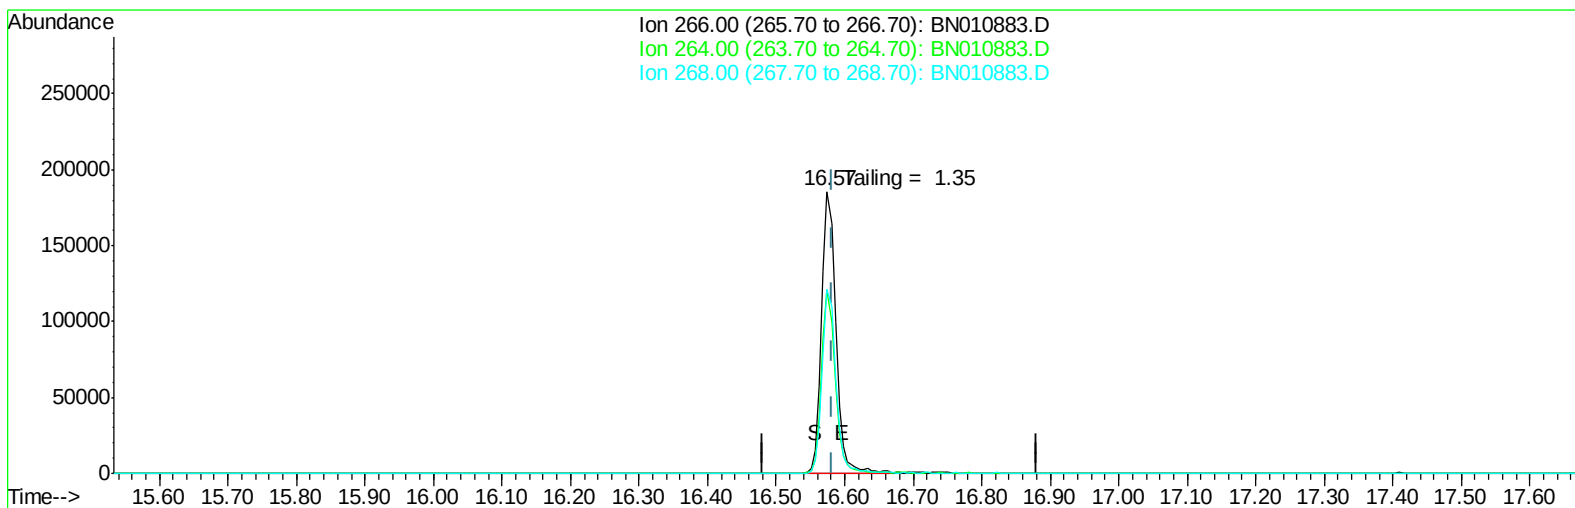

TIC: BN010883.D

(22) Pentachlorophenol

16.575min (-0.007) 0.00ng

response 266412

Ion	Exp%	Act%
266.00	100	100
264.00	68.50	64.84
268.00	69.90	65.34
0.00	0.00	0.00