


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061520\
 Data File : BN010866.D
 Acq On : 15 Jun 2020 09:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 16 08:49:35 2020

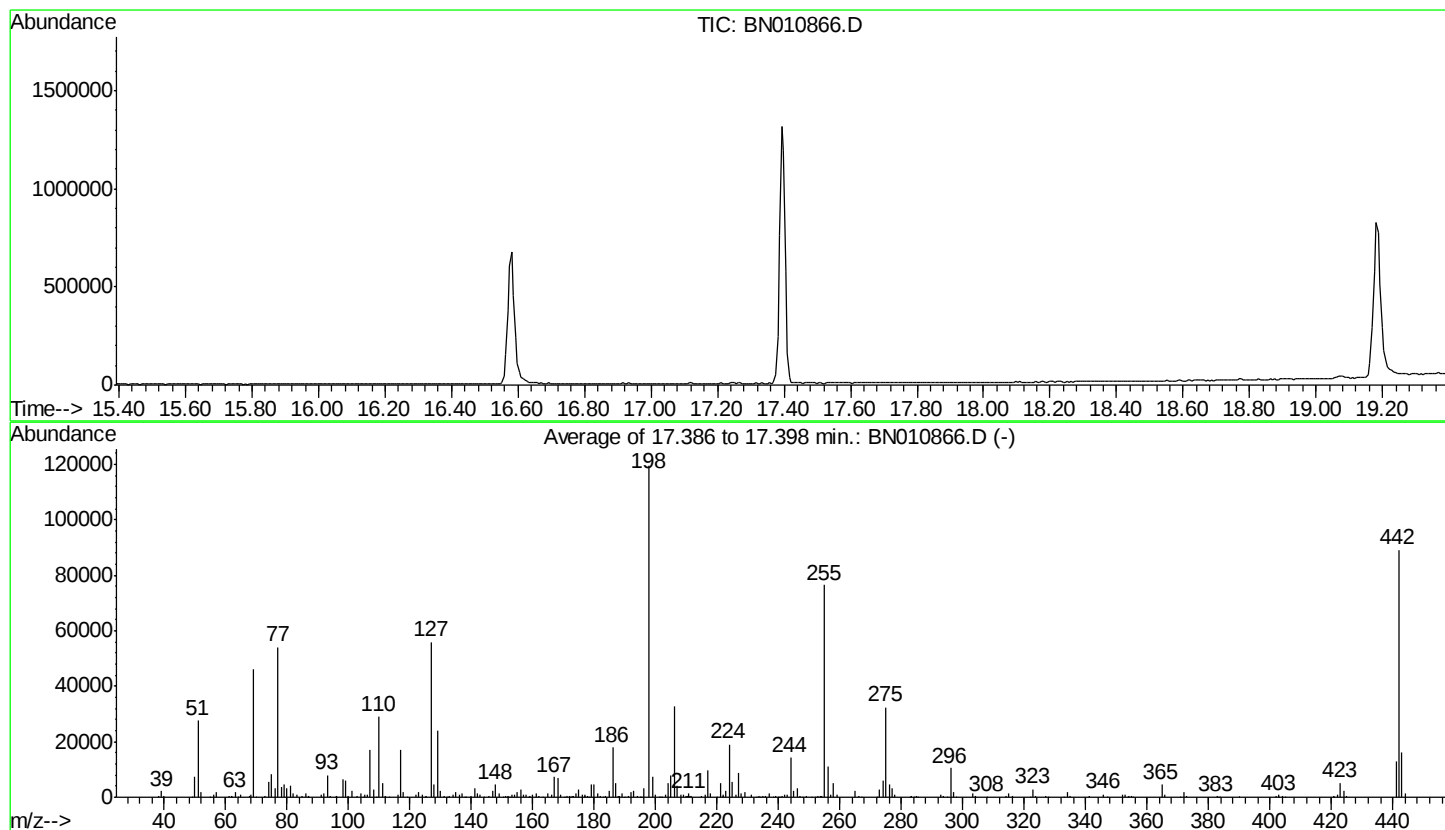

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.0	27456	PASS
68	69	0.00	2	1.8	815	PASS
69	198	0.00	100	38.8	46320	PASS
70	69	0.00	2	0.5	232	PASS
127	198	10	80	46.8	55968	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	119472	PASS
199	198	5	9	6.2	7453	PASS
275	198	10	60	27.1	32328	PASS
365	198	1	100	3.8	4591	PASS
441	198	0.01	100	11.0	13111	PASS
442	198	50	100	74.6	89074	PASS
443	442	15	24	18.1	16102	PASS