


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061520\
 Data File : BN010883.D
 Acq On : 15 Jun 2020 23:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 16 08:49:35 2020

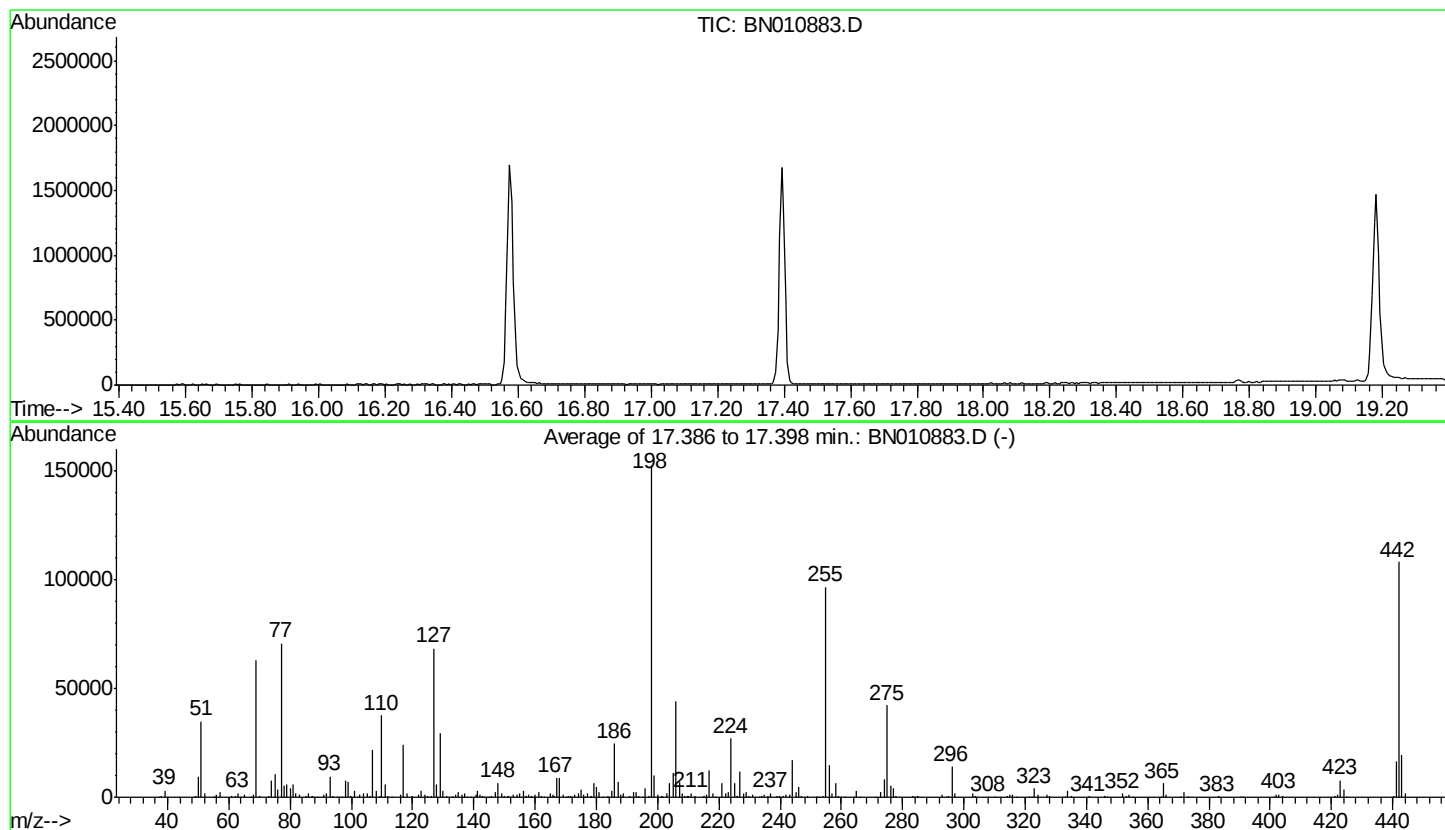

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.0	34922	PASS
68	69	0.00	2	2.0	1256	PASS
69	198	0.00	100	41.4	62928	PASS
70	69	0.00	2	0.6	372	PASS
127	198	10	80	45.0	68389	PASS
197	198	0.00	2	0.3	453	PASS
198	198	100	100	100.0	152088	PASS
199	198	5	9	6.7	10255	PASS
275	198	10	60	27.6	42024	PASS
365	198	1	100	4.2	6370	PASS
441	198	0.01	100	10.7	16214	PASS
442	198	50	100	70.9	107797	PASS
443	442	15	24	18.2	19616	PASS