

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020168.D
 Acq On : 15 Jun 2022 11:03
 Operator : CG/JU
 Sample : PB145541BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 16 01:10:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 16 00:50:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	147146	20.000	ng/ul	0.00
20) Naphthalene-d8	10.581	136	715231	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.428	164	498443	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.163	188	1055776	20.000	ng/ul	0.00
79) Chrysene-d12	21.357	240	1033264	20.000	ng/ul	0.00
88) Perylene-d12	23.674	264	1014803	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	19933	5.867	ng/uL	0.00
4) Pyridine-d5	3.675	84	267419	28.799	ng/ul	0.00
7) Phenol-d5	6.969	99	344362	28.282	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	233441	30.686	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132	297737	30.095	ng/ul	0.00
15) 4-Methylphenol-d8	8.505	113	309502	29.381	ng/ul	0.00
21) Nitrobenzene-d5	8.952	128	151778	27.894	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143	167220	28.957	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.210	165	277753	27.552	ng/ul	0.00
31) 4-Chloroaniline-d4	10.716	131	468075	28.672	ng/ul	0.00
46) Dimethylphthalate-d6	13.840	166	1087952	29.998	ng/ul	0.00
49) Acenaphthylene-d8	14.116	160	1244141	29.581	ng/ul	0.00
54) 4-Nitrophenol-d4	14.622	143	175386	24.133	ng/ul	0.00
60) Fluorene-d10	15.416	176	908236	30.263	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.540	200	152827	24.989	ng/ul	0.00
73) Anthracene-d10	17.263	188	1479772	32.115	ng/ul	0.00
81) Pyrene-d10	19.563	212	1653913	29.526	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.522	264	1555658	31.331	ng/ul	-0.01
Target Compounds						
					Qvalue	
48) 2,6-Dinitrotoluene	13.846	165	7900	1.107	ng/ul#	37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020168.D
Acq On : 15 Jun 2022 11:03
Operator : CG/JU
Sample : PB145541BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jun 16 01:10:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 16 00:50:14 2022
Response via : Initial Calibration

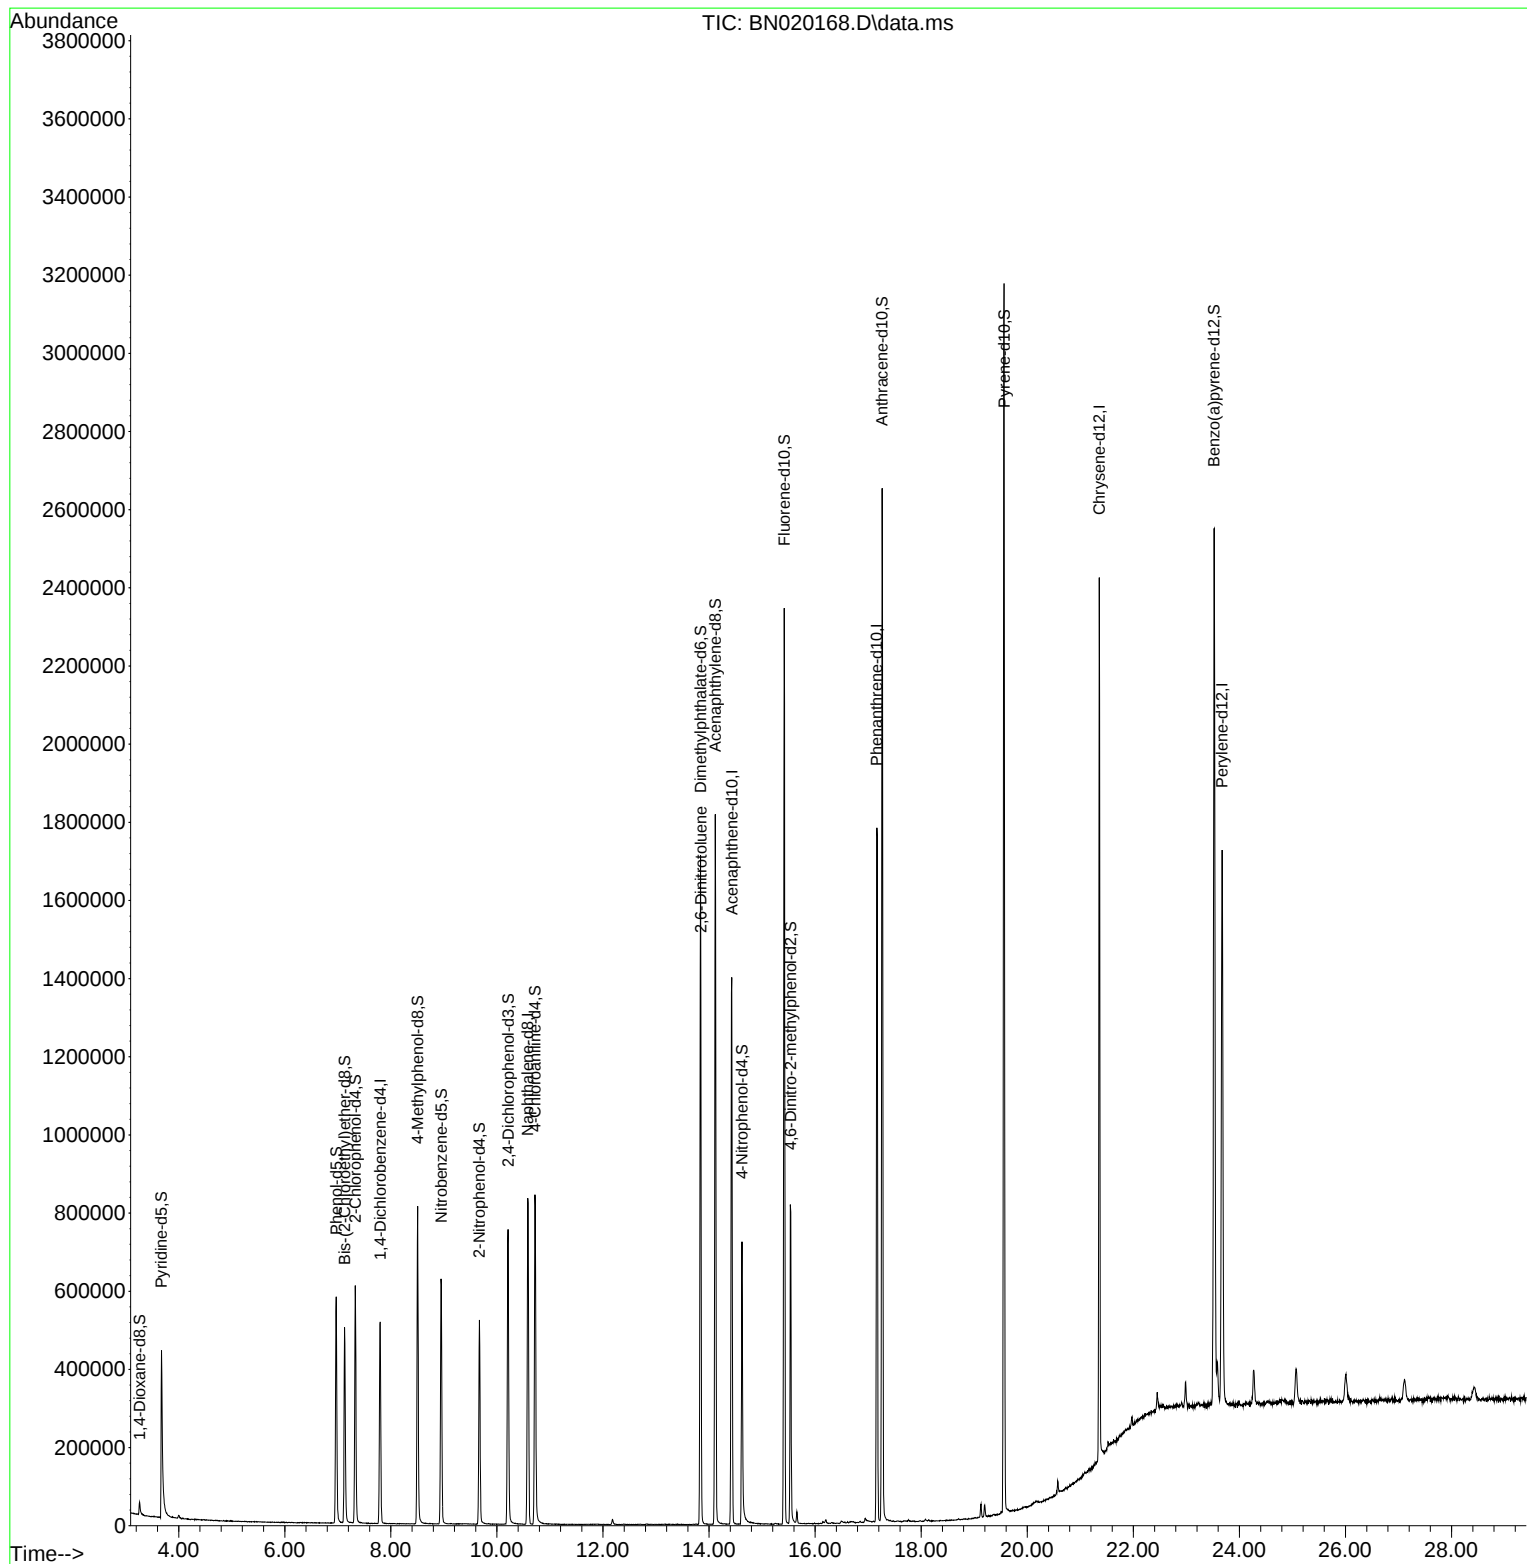

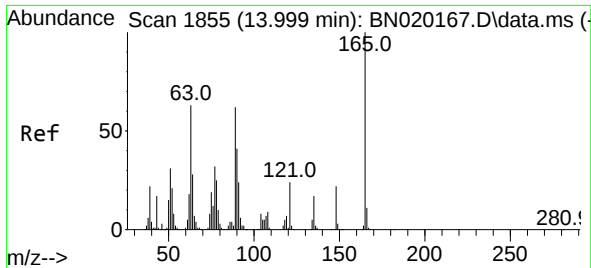

#48
 2,6-Dinitrotoluene
 Concen: 1.107 ng/ul
 RT: 13.846 min Scan# 11
 Delta R.T. -0.153 min
 Lab File: BN020168.D
 Acq: 15 Jun 2022 11:03

Instrument :
 BNA_N
 ClientSampleId :

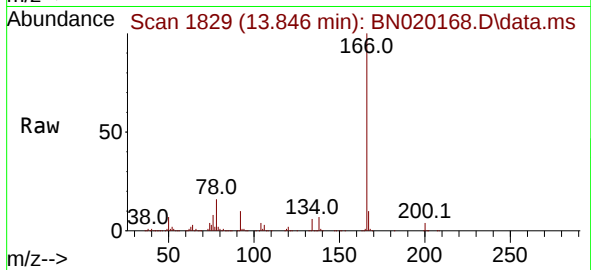

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	50.6	75.8#
121	27.9	17.9	26.9#

