

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020185.D
 Acq On : 15 Jun 2022 21:57
 Operator : CG/JU
 Sample : PB145547BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 16 01:12:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 16 00:50:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	72018	20.000	ng/u1	0.00
20) Naphthalene-d8	10.581	136	349189	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.428	164	243320	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.163	188	538582	20.000	ng/u1	0.00
79) Chrysene-d12	21.351	240	521531	20.000	ng/u1	-0.01
88) Perylene-d12	23.662	264	455221	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	18579	11.174	ng/uL	0.00
4) Pyridine-d5	3.669	84	241431	53.124	ng/u1	0.00
7) Phenol-d5	6.981	99	317982	53.359	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.128	67	207566	55.749	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	271464	56.064	ng/u1	0.00
15) 4-Methylphenol-d8	8.510	113	282324	54.759	ng/u1	0.00
21) Nitrobenzene-d5	8.946	128	136561	51.405	ng/u1	0.00
24) 2-Nitrophenol-d4	9.669	143	152752	54.180	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	258488	52.519	ng/u1	0.00
31) 4-Chloroaniline-d4	10.722	131	425071	53.332	ng/u1	0.00
46) Dimethylphthalate-d6	13.839	166	952785	53.816	ng/u1	0.00
49) Acenaphthylene-d8	14.116	160	1099962	53.574	ng/u1	0.00
54) 4-Nitrophenol-d4	14.645	143	160116	45.132	ng/u1	0.02
60) Fluorene-d10	15.416	176	816676	55.744	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.533	200	154359	49.477	ng/u1	0.00
73) Anthracene-d10	17.263	188	1338687	56.953	ng/u1	0.00
81) Pyrene-d10	19.563	212	1510109	53.411	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.515	264	1272970	57.153	ng/u1	-0.02


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.510	70	6692	1.671	ng/u1#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020185.D
Acq On : 15 Jun 2022 21:57
Operator : CG/JU
Sample : PB145547BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jun 16 01:12:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 16 00:50:14 2022
Response via : Initial Calibration

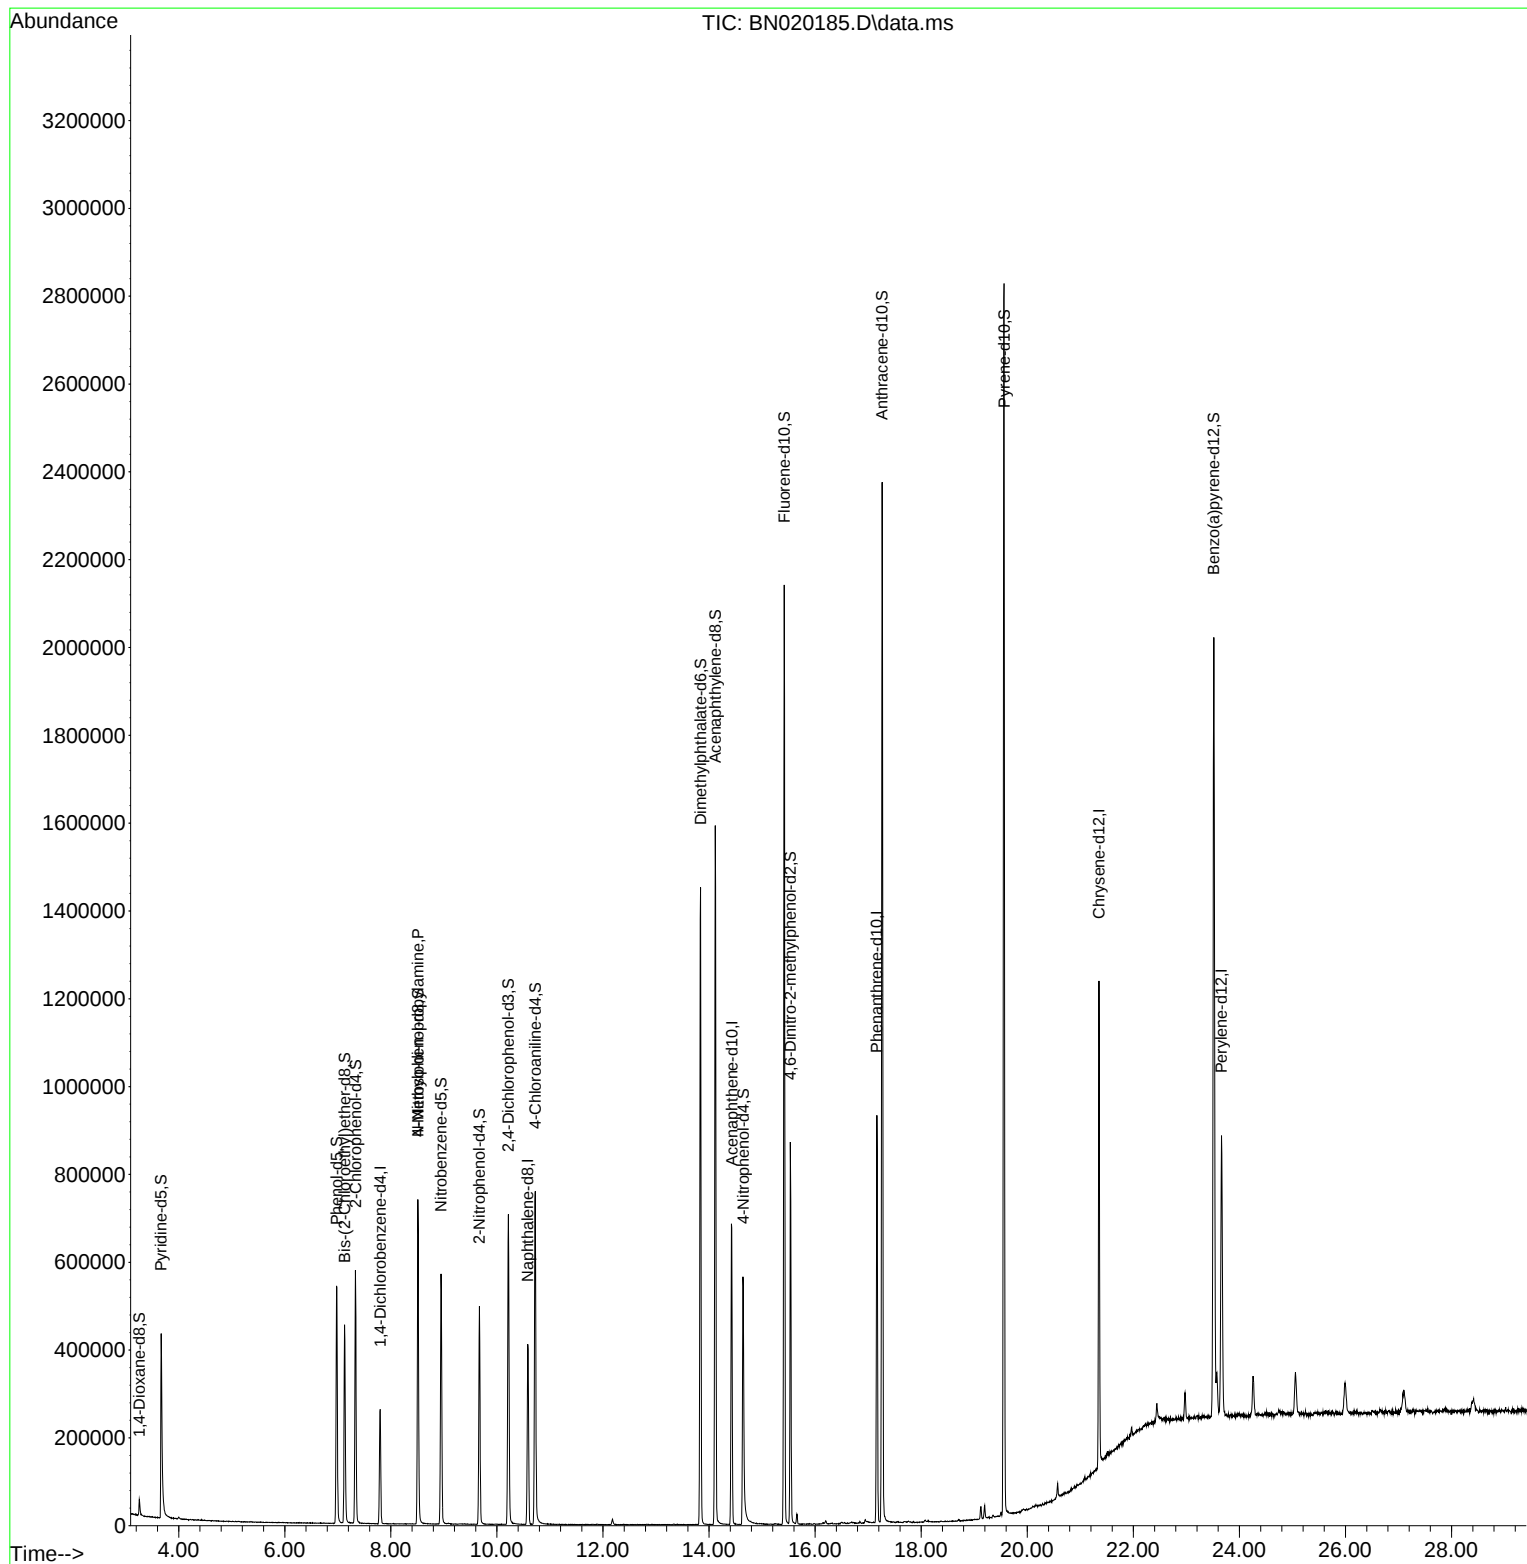

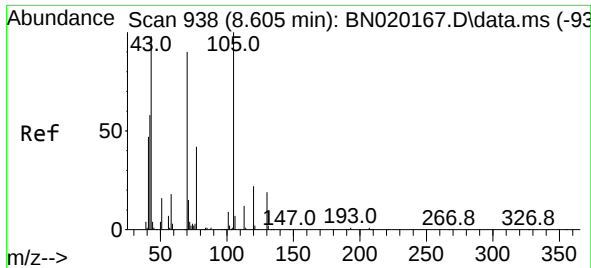

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.671 ng/ul
 RT: 8.510 min Scan# 91
 Delta R.T. -0.094 min
 Lab File: BN020185.D
 Acq: 15 Jun 2022 21:57

Instrument :
 BNA_N
 ClientSampleId :

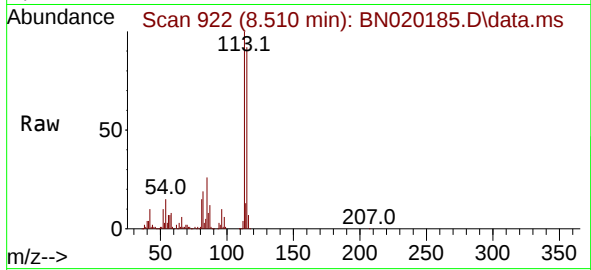

Tgt Ion:	70	Resp:	6692
Ion	Ratio	Lower	Upper
70	100		
42	413.0	47.8	71.6#
101	0.0	7.8	11.6#
130	0.0	15.8	23.8#

