

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020197.D
 Acq On : 16 Jun 2022 09:31
 Operator : CG/JU
 Sample : PB145548BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 17 02:26:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 16 00:50:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	104408	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.569	136	489441	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.416	164	337913	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.163	188	717178	20.000	ng/ul	0.00
79) Chrysene-d12	21.357	240	677496	20.000	ng/ul	# 0.00
88) Perylene-d12	23.668	264	625692	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	21602	8.961	ng/uL	-0.01
4) Pyridine-d5	3.658	84	291034	44.172	ng/ul	-0.02
7) Phenol-d5	6.975	99	355763	41.179	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.116	67	232780	43.125	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.322	132	303482	43.233	ng/ul	0.00
15) 4-Methylphenol-d8	8.504	113	321234	42.977	ng/ul	0.00
21) Nitrobenzene-d5	8.934	128	156670	42.075	ng/ul	-0.02
24) 2-Nitrophenol-d4	9.657	143	174166	44.073	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.210	165	285307	41.357	ng/ul	0.00
31) 4-Chloroaniline-d4	10.710	131	461072	41.272	ng/ul	-0.01
46) Dimethylphthalate-d6	13.833	166	1072916	43.637	ng/ul	0.00
49) Acenaphthylene-d8	14.110	160	1198571	42.035	ng/ul	0.00
54) 4-Nitrophenol-d4	14.663	143	183905	37.327	ng/ul	0.03
60) Fluorene-d10	15.410	176	897665	44.120	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.533	200	175752	42.306	ng/ul	0.00
73) Anthracene-d10	17.257	188	1433613	45.803	ng/ul	0.00
81) Pyrene-d10	19.557	212	1674318	45.587	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.527	264	1390196	45.411	ng/ul	0.00


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.504	70	7530	1.297	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020197.D
Acq On : 16 Jun 2022 09:31
Operator : CG/JU
Sample : PB145548BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jun 17 02:26:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 16 00:50:14 2022
Response via : Initial Calibration

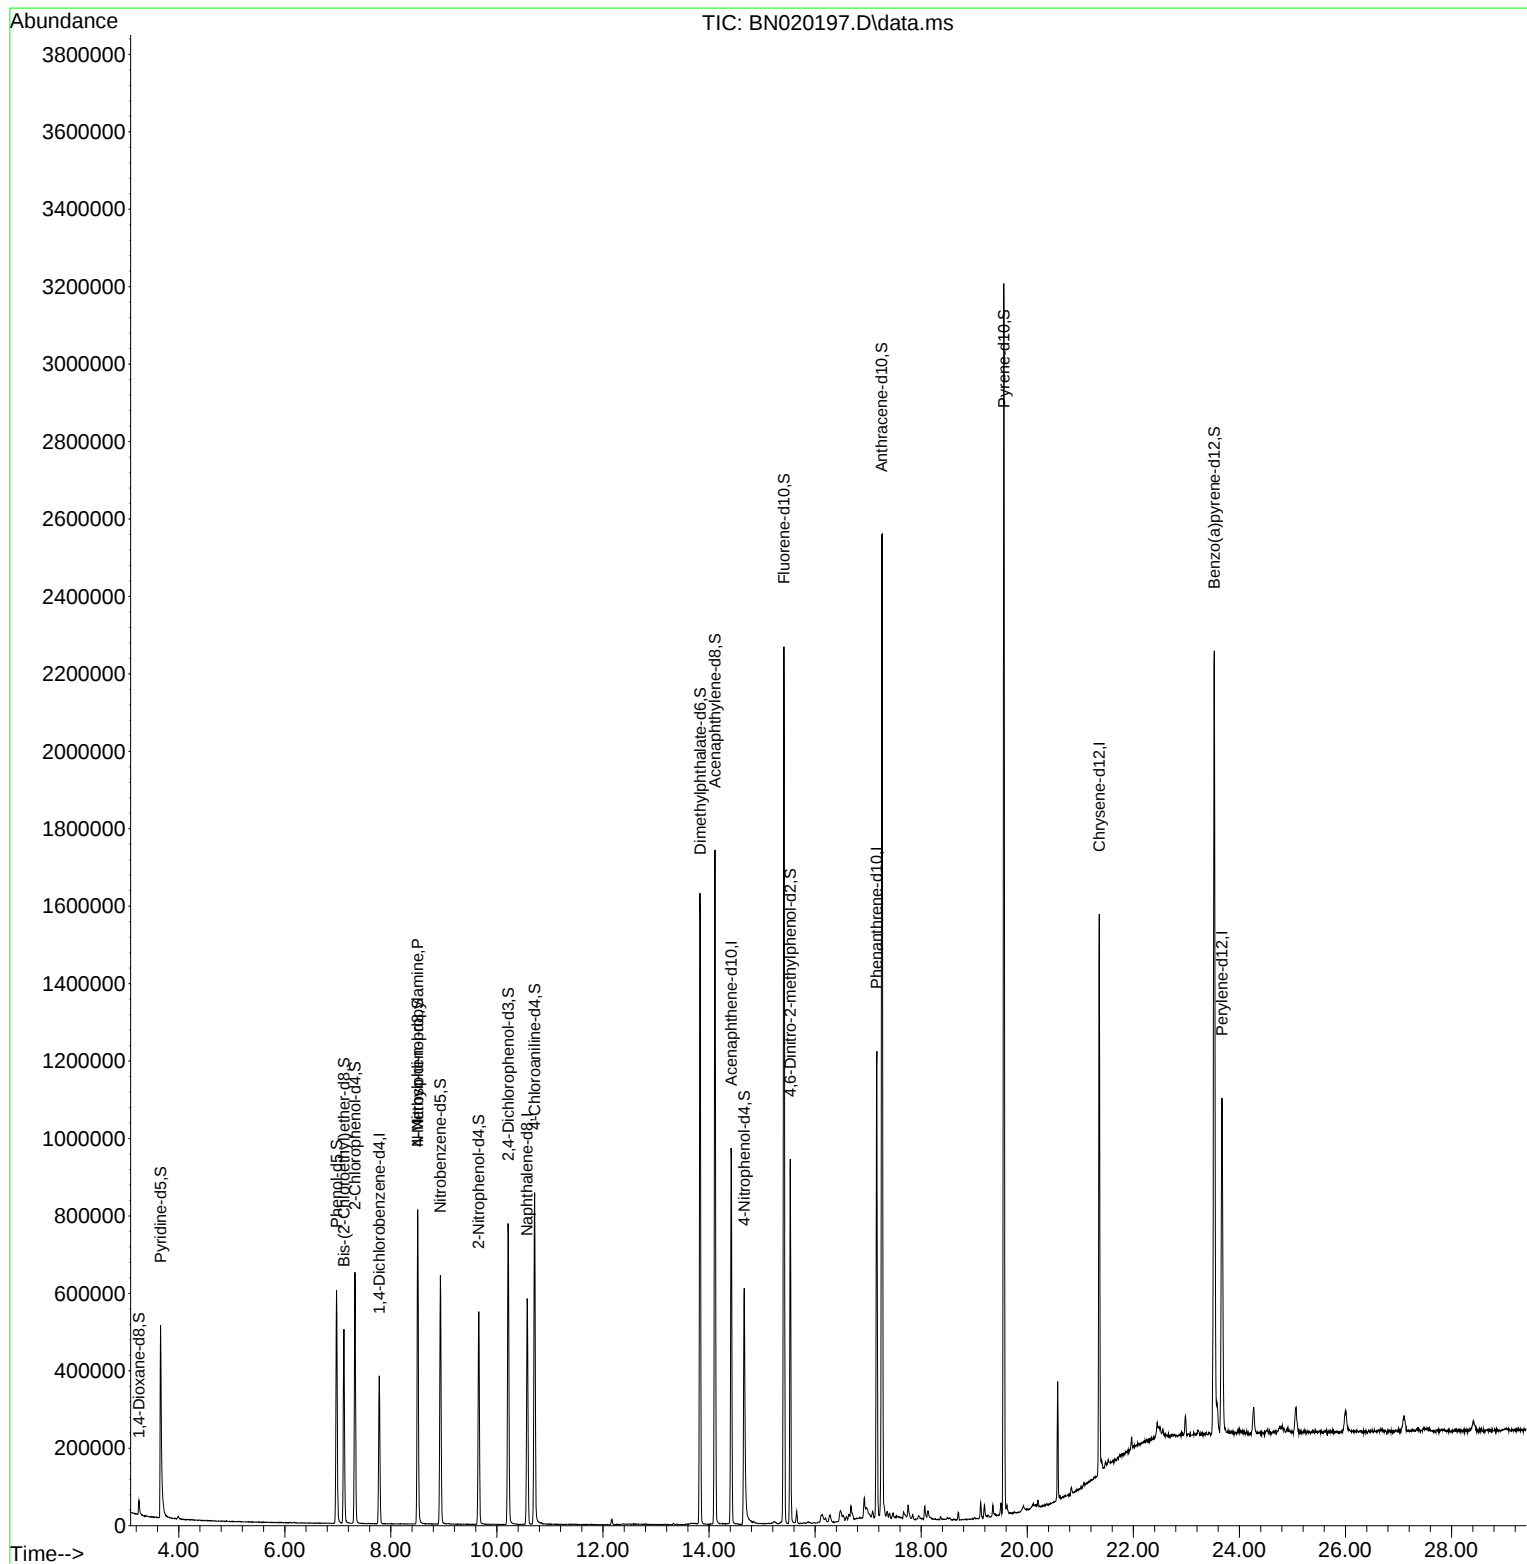

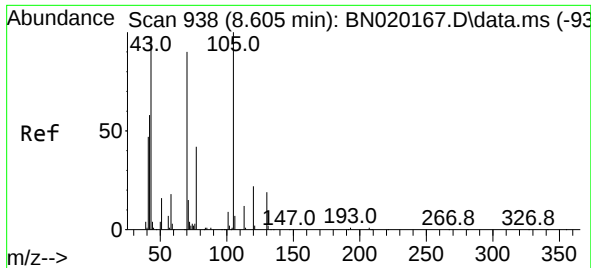

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.297 ng/ul
 RT: 8.504 min Scan# 91
 Delta R.T. -0.100 min
 Lab File: BN020197.D
 Acq: 16 Jun 2022 09:31

Instrument :
 BNA_N
 ClientSampleId :

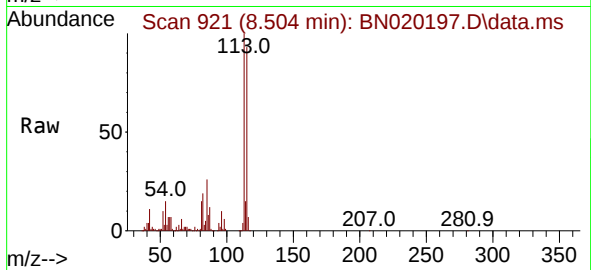

Tgt Ion:	70	Resp:	7530
Ion	Ratio	Lower	Upper
70	100		
42	453.5	47.8	71.6#
101	0.0	7.8	11.6#
130	0.0	15.8	23.8#

