

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020214.D
 Acq On : 16 Jun 2022 20:56
 Operator : CG/JU
 Sample : N3285-17
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 17 02:29:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 16 00:50:14 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	165922	20.000	ng/ul	0.00
20) Naphthalene-d8	10.581	136	791852	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.422	164	538014	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.163	188	1108452	20.000	ng/ul	0.00
79) Chrysene-d12	21.351	240	813191	20.000	ng/ul	-0.01
88) Perylene-d12	23.663	264	686108	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	17940	4.683	ng/uL	0.00
4) Pyridine-d5	3.669	84	79016	7.547	ng/ul	0.00
7) Phenol-d5	6.993	99	88113	6.418	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.128	67	256802	29.937	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	268614	24.079	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	192417	16.199	ng/ul	0.01
21) Nitrobenzene-d5	8.946	128	175583	29.146	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143	192767	30.151	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	321834	28.835	ng/ul	0.01
31) 4-Chloroaniline-d4	10.716	131	360975	19.972	ng/ul	0.00
46) Dimethylphthalate-d6	13.834	166	1284604	32.815	ng/ul	0.00
49) Acenaphthylene-d8	14.116	160	1405583	30.961	ng/ul	0.00
54) 4-Nitrophenol-d4	14.675	143	35823	4.567	ng/ul	0.05
60) Fluorene-d10	15.416	176	1074631	33.174	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.534	200	213968	33.324	ng/ul	0.00
73) Anthracene-d10	17.263	188	1710206	35.353	ng/ul	0.00
81) Pyrene-d10	19.557	212	1790950	40.625	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.515	264	1212083	36.106	ng/ul	-0.02
Target Compounds						
35) 4-Chloro-3-methylphenol	11.940	107	114322	8.386	ng/ul#	20


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020214.D
Acq On : 16 Jun 2022 20:56
Operator : CG/JU
Sample : N3285-17
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jun 17 02:29:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 16 00:50:14 2022
Response via : Initial Calibration

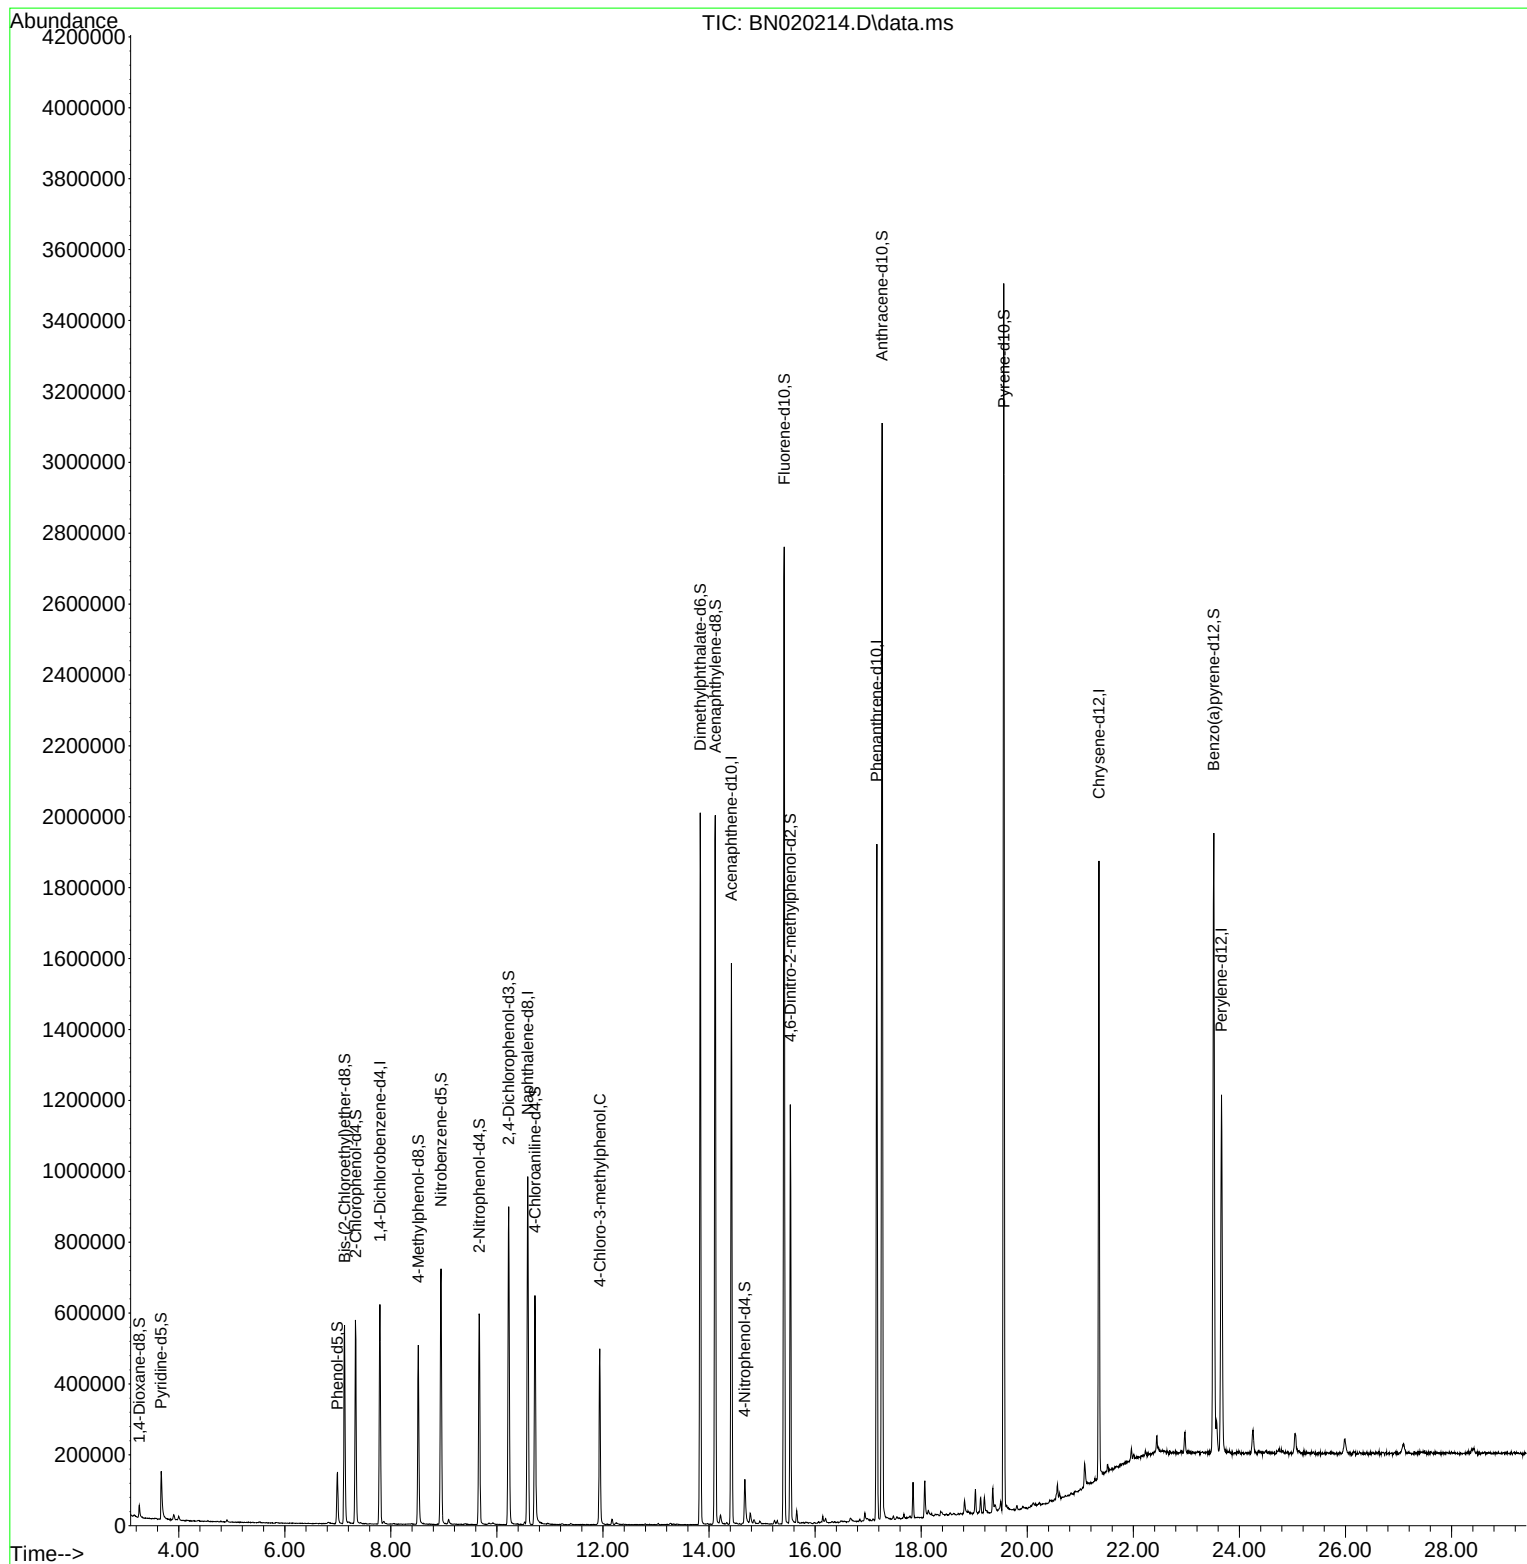

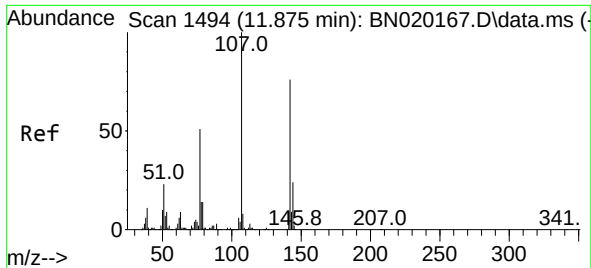

#35
 4-Chloro-3-methylphenol
 Concen: 8.386 ng/ul
 RT: 11.940 min Scan# 11
 Delta R.T. 0.064 min
 Lab File: BN020214.D
 Acq: 16 Jun 2022 20:56

Instrument :
 BNA_N
 ClientSampleId :

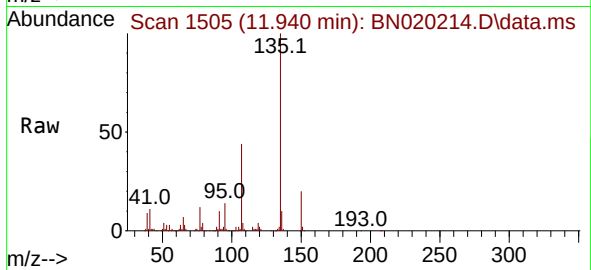

Tgt Ion:107 Resp: 114322
 Ion Ratio Lower Upper
 107 100
 144 0.0 20.6 31.0#
 142 0.0 62.2 93.4#

