

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020215.D
 Acq On : 16 Jun 2022 21:32
 Operator : CG/JU
 Sample : N3285-16
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 17 02:29:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 16 00:50:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	169708	20.000	ng/u1	0.00
20) Naphthalene-d8	10.581	136	821955	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.422	164	549609	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.163	188	1144019	20.000	ng/u1	0.00
79) Chrysene-d12	21.351	240	988135	20.000	ng/u1	-0.01
88) Perylene-d12	23.669	264	831026	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	17120	4.369	ng/uL	0.00
4) Pyridine-d5	3.670	84	110256	10.295	ng/u1	0.00
7) Phenol-d5	6.987	99	105482	7.511	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	7.122	67	269358	30.701	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	285586	25.029	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	211303	17.392	ng/u1	0.01
21) Nitrobenzene-d5	8.946	128	185023	29.588	ng/u1	0.00
24) 2-Nitrophenol-d4	9.669	143	204826	30.864	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	324118	27.976	ng/u1	0.01
31) 4-Chloroaniline-d4	10.716	131	375878	20.035	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	1259529	31.496	ng/u1	0.00
49) Acenaphthylene-d8	14.116	160	1431563	30.868	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	44290	5.527	ng/u1	0.05
60) Fluorene-d10	15.416	176	1055713	31.902	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.534	200	205838	31.061	ng/u1	0.00
73) Anthracene-d10	17.263	188	1630425	32.656	ng/u1	0.00
81) Pyrene-d10	19.557	212	1847678	34.492	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.516	264	1386302	34.095	ng/u1	-0.02
Target Compounds						Qvalue
8) Phenol	7.017	94	59379	3.971	ng/u1	98
35) 4-Chloro-3-methylphenol	11.940	107	548672	38.774	ng/u1#	20


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020215.D
Acq On : 16 Jun 2022 21:32
Operator : CG/JU
Sample : N3285-16
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 17 02:29:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 16 00:50:14 2022
Response via : Initial Calibration

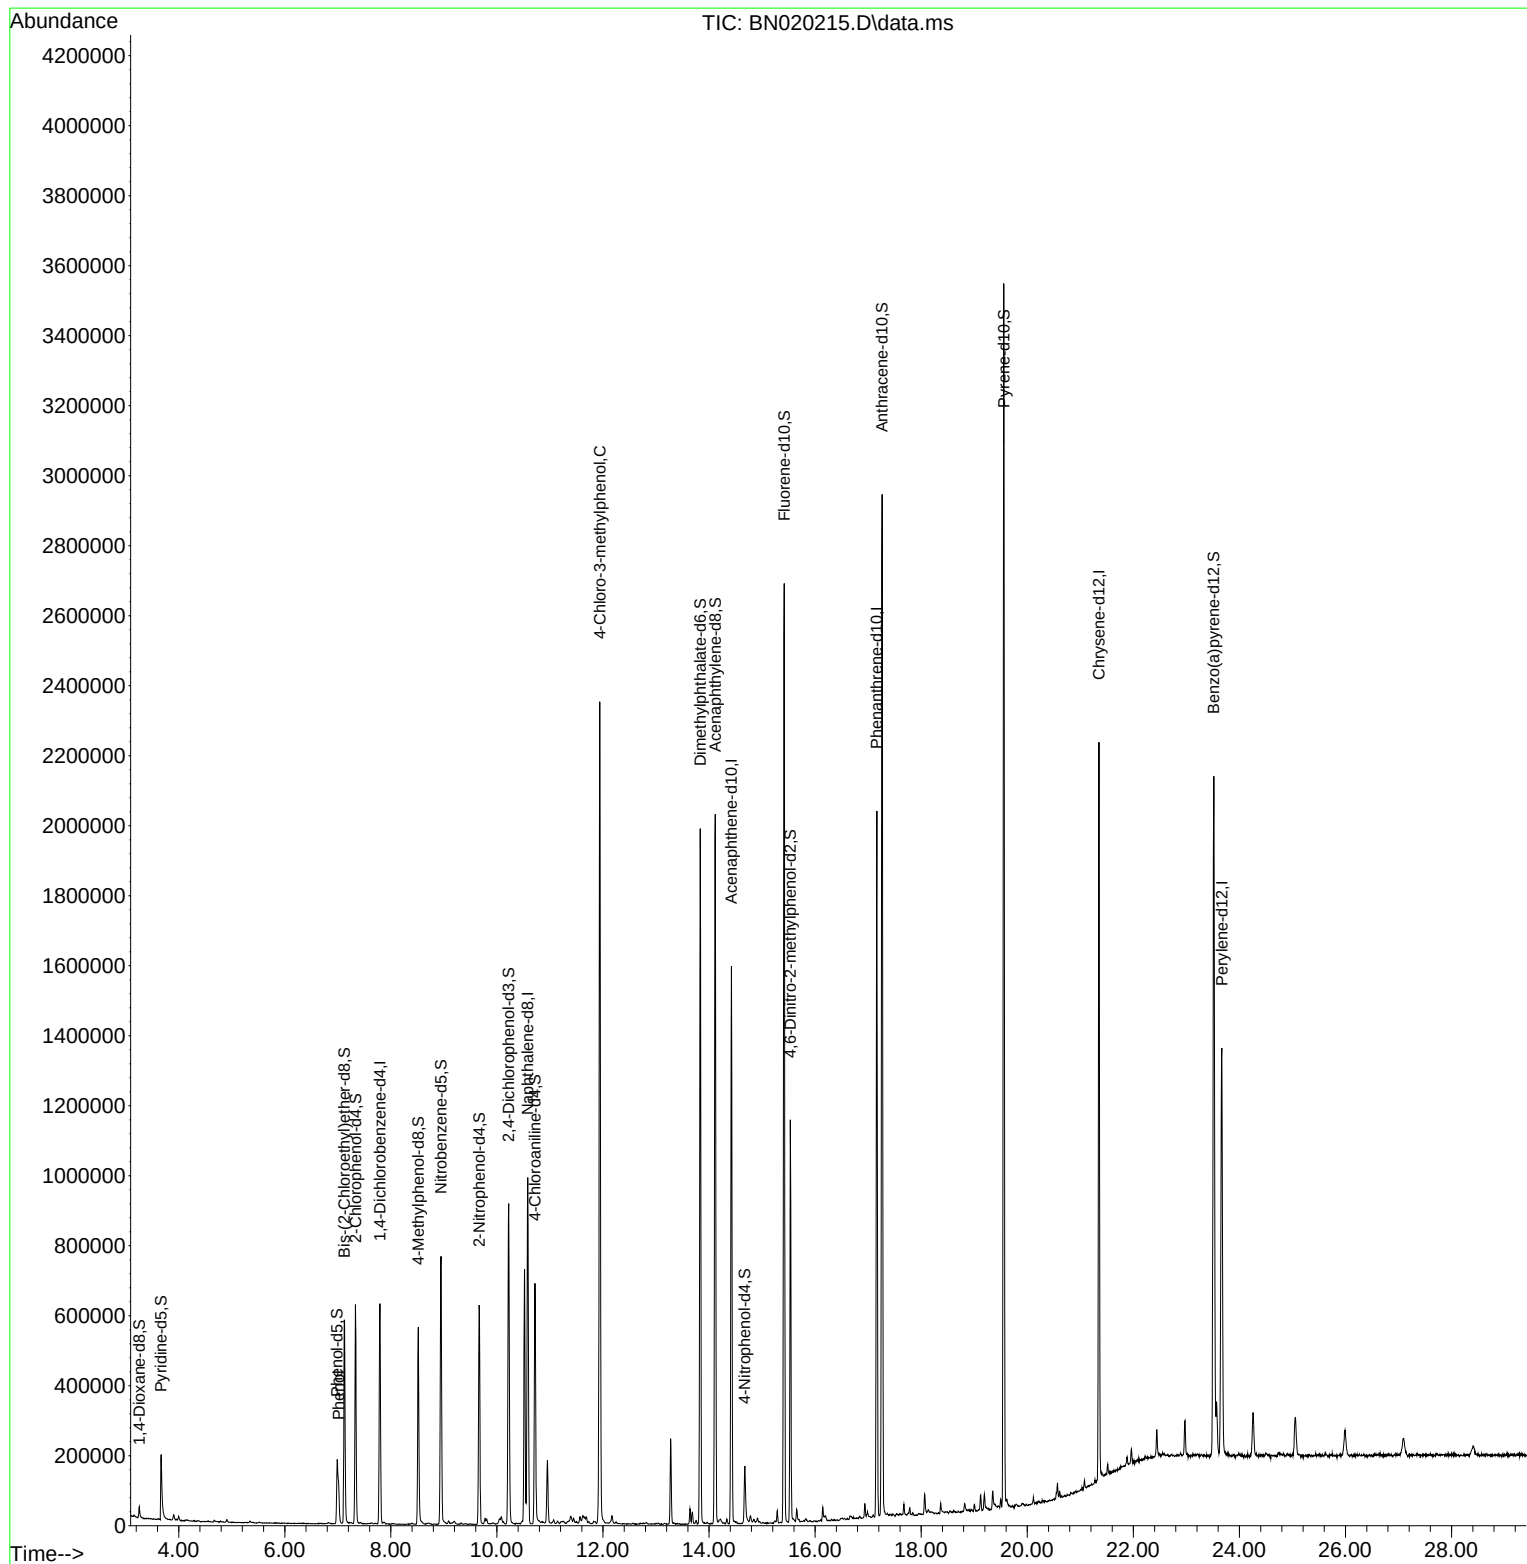

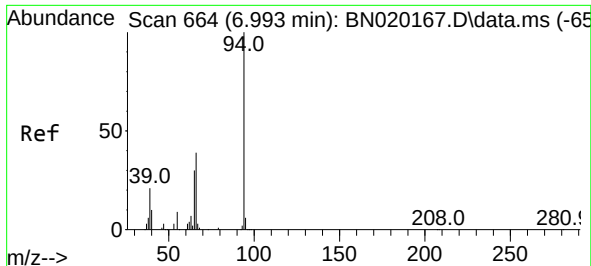

#8

Phenol

Concen: 3.971 ng/ul

RT: 7.017 min Scan# 6

Delta R.T. 0.024 min


Lab File: BN020215.D

Acq: 16 Jun 2022 21:32

Instrument :

BNA_N

ClientSampleId :

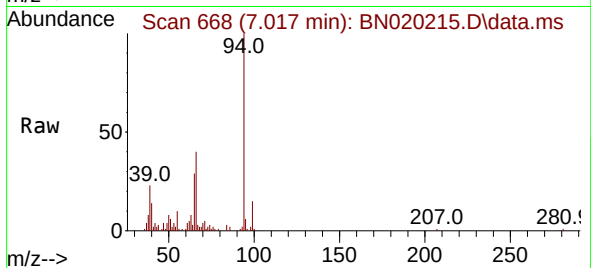




Tgt Ion: 94 Resp: 59379

Ion Ratio Lower Upper

94 100

65 29.0 23.6 35.4

66 40.2 31.2 46.8

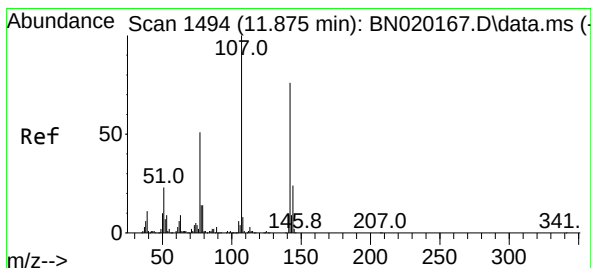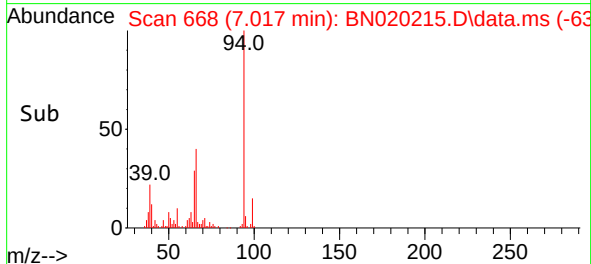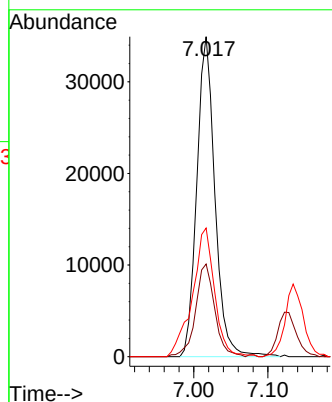

#35

4-Chloro-3-methylphenol

Concen: 38.774 ng/ul

RT: 11.940 min Scan# 1505

Delta R.T. 0.065 min

Lab File: BN020215.D

Acq: 16 Jun 2022 21:32

Tgt Ion: 107 Resp: 548672

Ion Ratio Lower Upper

107 100

144 0.0 20.6 31.0#

142 0.1 62.2 93.4#

