




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020188.D
 Acq On : 15 Jun 2022 23:46
 Operator : CG/JU
 Sample : N3294-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4P6

Manual IntegrationsAPPROVED

Quant Time: Jun 16 03:07:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 16 00:50:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/16/2022
 Supervised By :mohammad ahmed 06/22/2022

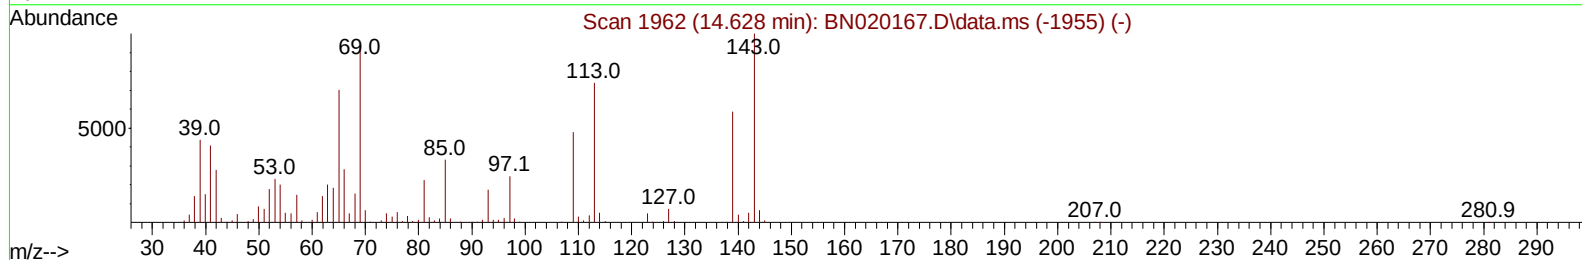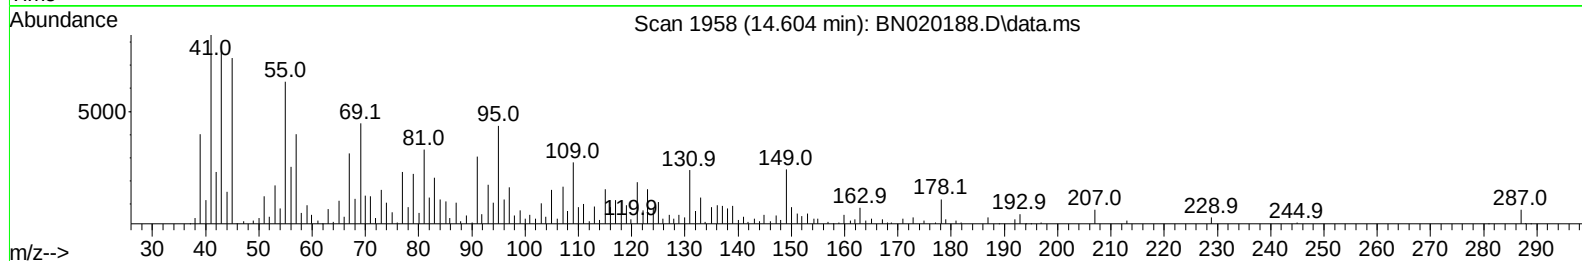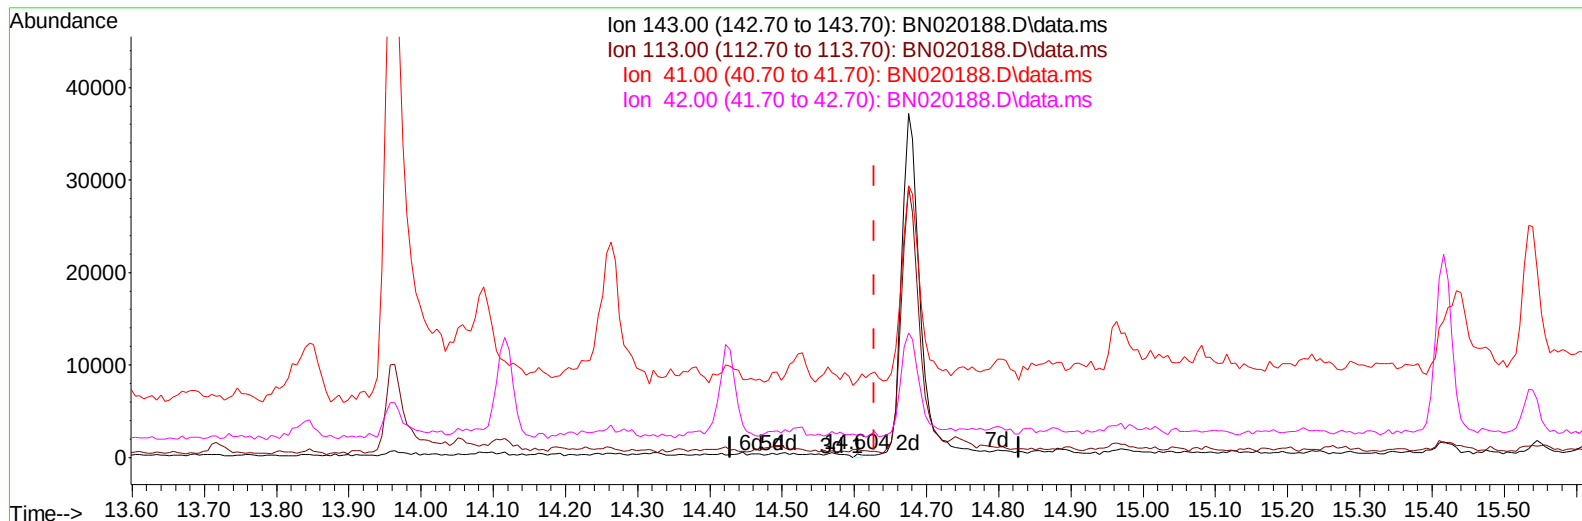

TIC: BN020188.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.604min (-0.024) 0.03 ng/u1

response 213

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	244.75#
41.00	39.70	2292.54#
42.00	27.00	657.18#




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020188.D
Acq On : 15 Jun 2022 23:46
Operator : CG/JU
Sample : N3294-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P6

Manual IntegrationsAPPROVED

Quant Time: Jun 16 03:07:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 16 00:50:14 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/16/2022
Supervised By :mohammad ahmed 06/22/2022

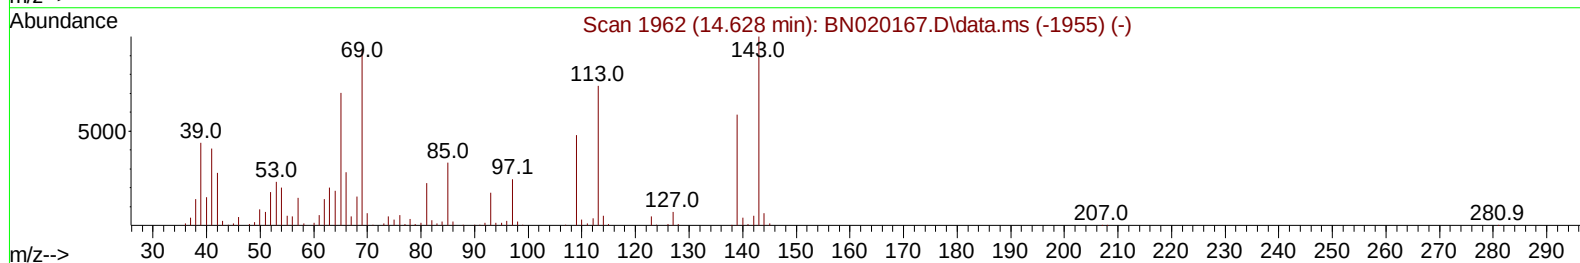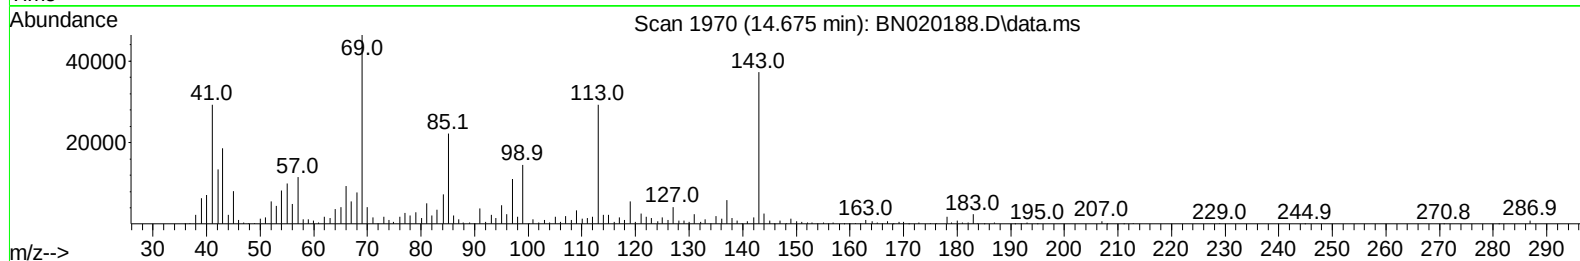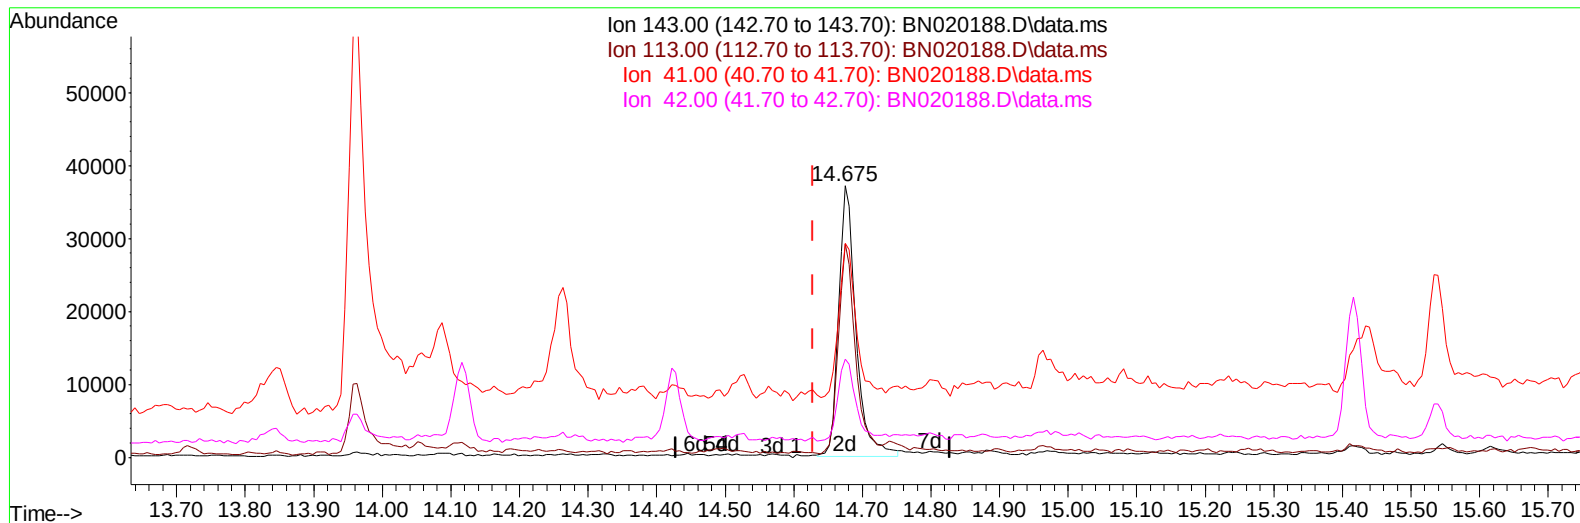

TIC: BN020188.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.675min (+ 0.047) 9.21 ng/ul m

response 65621

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	78.55
41.00	39.70	78.89#
42.00	27.00	36.25#

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020188.D
 Acq On : 15 Jun 2022 23:46
 Operator : CG/JU
 Sample : N3294-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4P6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/16/2022
 Supervised By :mohammad ahmed 06/22/2022

Quant Time: Jun 16 03:07:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 16 00:50:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	157408	20.000	ng/ul	0.00
20) Naphthalene-d8	10.587	136	757069	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.428	164	488519	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.163	188	950486	20.000	ng/ul	0.00
79) Chrysene-d12	21.357	240	814685	20.000	ng/ul	0.00
88) Perylene-d12	23.674	264	716968	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	16784	4.618	ng/uL	0.00
4) Pyridine-d5	3.675	84	136521	13.744	ng/ul	0.00
7) Phenol-d5	6.987	99	126746	9.731	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.128	67	243876	29.968	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	294844	27.860	ng/ul	0.00
15) 4-Methylphenol-d8	8.522	113	239216	21.228	ng/ul	0.02
21) Nitrobenzene-d5	8.952	128	179840	31.224	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143	200000	32.720	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	352932	33.074	ng/ul	0.01
31) 4-Chloroaniline-d4	10.722	131	305709	17.691	ng/ul	0.00
46) Dimethylphthalate-d6	13.840	166	1210622	34.058	ng/ul	0.00
49) Acenaphthylene-d8	14.116	160	1334936	32.384	ng/ul	0.00
54) 4-Nitrophenol-d4	14.675	143	65621m	9.213	ng/ul	0.05
60) Fluorene-d10	15.416	176	999863	33.993	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.539	200	211236	38.366	ng/ul	0.00
73) Anthracene-d10	17.263	188	1508570	36.367	ng/ul	0.00
81) Pyrene-d10	19.563	212	1651574	37.395	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.521	264	1254859	35.772	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.299	88	4750	1.238	ng/ul#	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020188.D
Acq On : 15 Jun 2022 23:46
Operator : CG/JU
Sample : N3294-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/16/2022
Supervised By :mohammad ahmed 06/22/2022

Quant Time: Jun 16 03:07:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 16 00:50:14 2022
Response via : Initial Calibration

