




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020222.D
Acq On : 17 Jun 2022 01:44
Operator : CG/JU
Sample : N3294-15
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/17/2022
Supervised By :mohammad ahmed 06/22/2022

Quant Time: Jun 17 02:30:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 16 00:50:14 2022
Response via : Initial Calibration

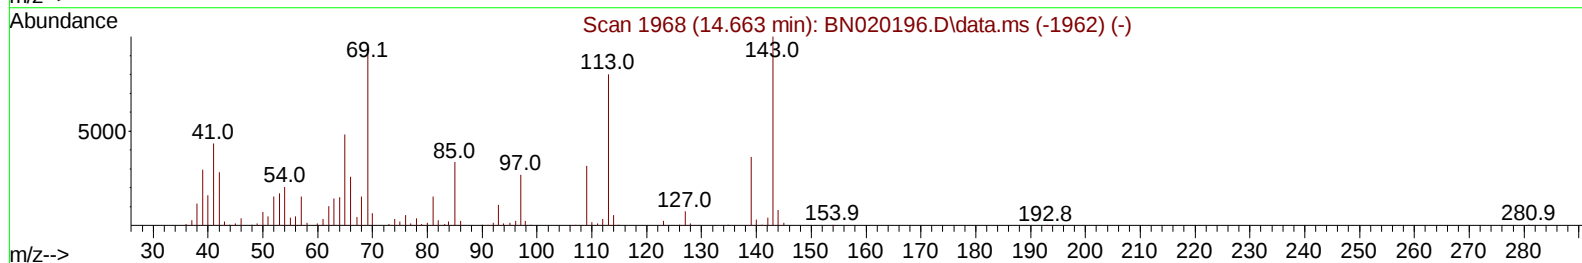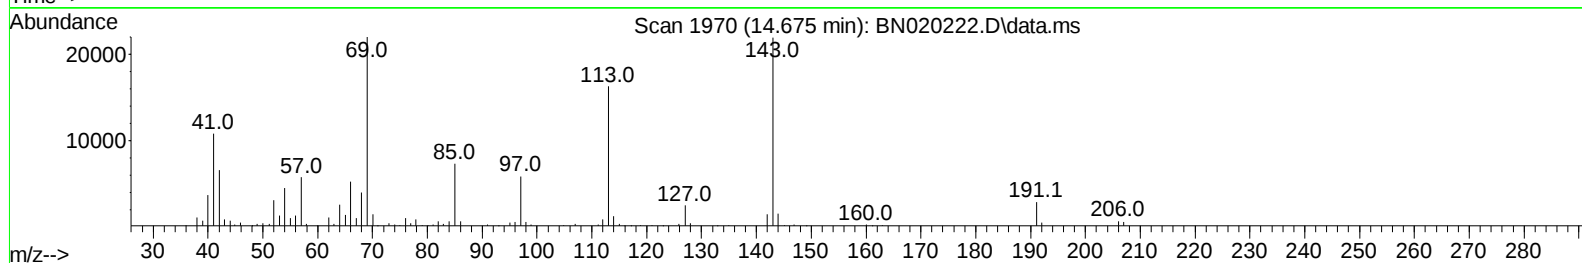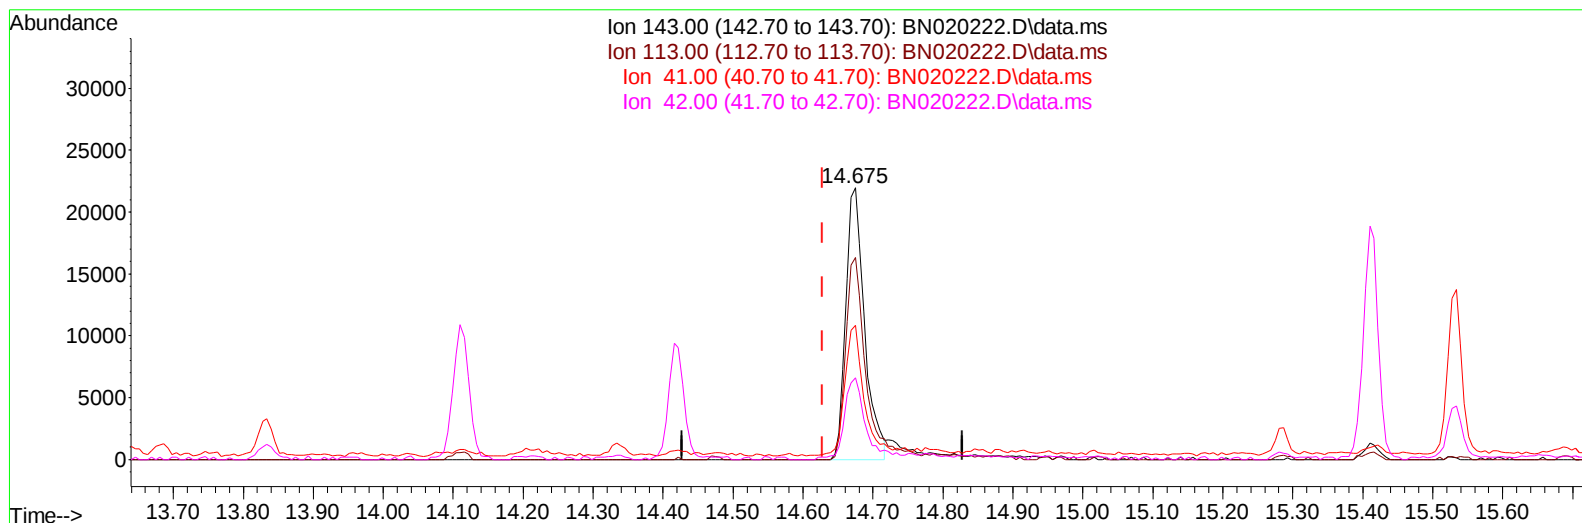

TIC: BN020222.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.675min (+ 0.047) 6.41 ng/ul

response 40708

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	74.34
41.00	39.70	49.43#
42.00	27.00	30.20




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020222.D
Acq On : 17 Jun 2022 01:44
Operator : CG/JU
Sample : N3294-15
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/17/2022
Supervised By :mohammad ahmed 06/22/2022

Quant Time: Jun 17 02:30:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 16 00:50:14 2022
Response via : Initial Calibration

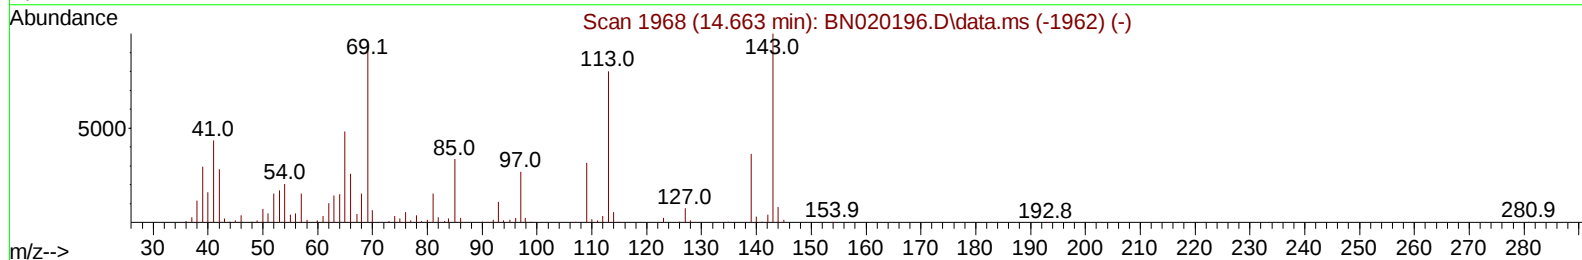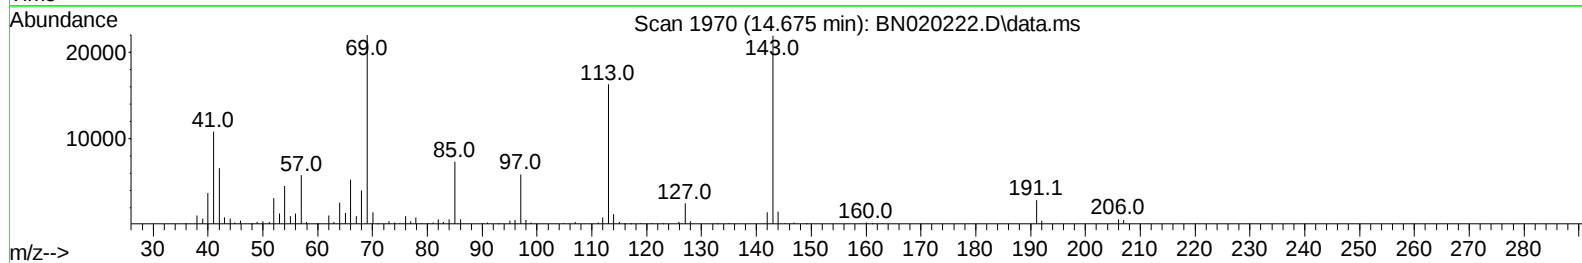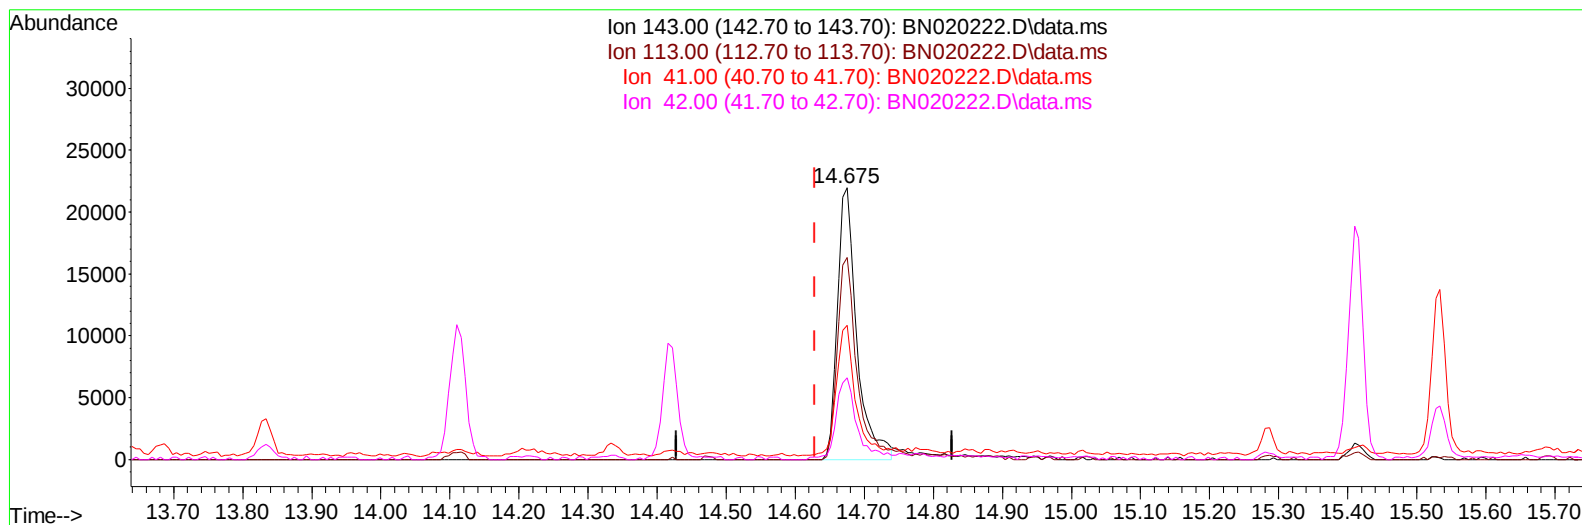

TIC: BN020222.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.675min (+ 0.047) 6.71 ng/ul m

response 42621

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	74.34
41.00	39.70	49.43#
42.00	27.00	30.20

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020222.D
 Acq On : 17 Jun 2022 01:44
 Operator : CG/JU
 Sample : N3294-15
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/17/2022
 Supervised By :mohammad ahmed 06/22/2022

Quant Time: Jun 17 02:30:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 16 00:50:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	139528	20.000	ng/ul	0.00
20) Naphthalene-d8	10.581	136	660439	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.422	164	435543	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.163	188	915990	20.000	ng/ul	0.00
79) Chrysene-d12	21.351	240	864790	20.000	ng/ul	-0.01
88) Perylene-d12	23.662	264	754387	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	16860	5.234	ng/uL	0.00
4) Pyridine-d5	3.669	84	103435	11.747	ng/ul	0.00
7) Phenol-d5	6.987	99	100395	8.696	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.122	67	257405	35.684	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	276488	29.473	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	201979	20.220	ng/ul	0.01
21) Nitrobenzene-d5	8.946	128	178309	35.488	ng/ul	0.00
24) 2-Nitrophenol-d4	9.663	143	191767	35.963	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	307409	33.023	ng/ul	0.00
31) 4-Chloroaniline-d4	10.716	131	354197	23.496	ng/ul	0.00
46) Dimethylphthalate-d6	13.834	166	1198137	37.807	ng/ul	0.00
49) Acenaphthylene-d8	14.110	160	1353109	36.818	ng/ul	0.00
54) 4-Nitrophenol-d4	14.675	143	42621m	6.712	ng/ul	0.05
60) Fluorene-d10	15.416	176	994082	37.907	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.533	200	188955	35.612	ng/ul	0.00
73) Anthracene-d10	17.263	188	1588342	39.732	ng/ul	0.00
81) Pyrene-d10	19.557	212	1810772	38.624	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.521	264	1491637	40.412	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020222.D
Acq On : 17 Jun 2022 01:44
Operator : CG/JU
Sample : N3294-15
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/17/2022
Supervised By :mohammad ahmed 06/22/2022

Quant Time: Jun 17 02:30:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 16 00:50:14 2022
Response via : Initial Calibration

