

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020168.D
 Acq On : 15 Jun 2022 11:03
 Operator : CG/JU
 Sample : PB145541BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK541

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	37	rVB	31736	47922	1.07%	0.102%
2	3.675	97	100	116	rBV	428120	784258	17.48%	1.664%
3	3.999	152	155	163	rVB5	9079	17415	0.39%	0.037%
4	6.969	653	660	674	rBV	578528	987916	22.02%	2.096%
5	7.128	681	687	701	rBV	498962	832475	18.56%	1.766%
6	7.328	714	721	735	rBV	607013	1049239	23.39%	2.226%
7	7.799	793	801	811	rBV	516123	890628	19.85%	1.889%
8	8.505	911	921	940	rBV	813386	1366667	30.47%	2.899%
9	8.946	989	996	1013	rBV	627068	1087281	24.24%	2.307%
10	9.669	1110	1119	1135	rBV	522710	904612	20.17%	1.919%
11	10.210	1203	1211	1231	rBV	754081	1341980	29.92%	2.847%
12	10.581	1266	1274	1285	rBV	834491	1483503	33.07%	3.147%
13	10.716	1289	1297	1313	rBV	843115	1555328	34.67%	3.299%
14	12.181	1540	1546	1552	rBV2	12488	21422	0.48%	0.045%
15	13.840	1821	1828	1842	rBV	1711862	2401222	53.53%	5.094%
16	14.116	1868	1875	1893	rBV	1816501	2743815	61.17%	5.821%
17	14.428	1920	1928	1937	rBV	1399370	2181208	48.62%	4.627%
18	14.622	1955	1961	1979	rBV	722818	1156911	25.79%	2.454%
19	15.245	2063	2067	2070	rBV6	2949	5409	0.12%	0.011%
20	15.416	2089	2096	2106	rBV	2344420	3493631	77.88%	7.411%
21	15.534	2110	2116	2131	rVV	816789	1175207	26.20%	2.493%
22	15.657	2132	2137	2143	rVB	29804	45239	1.01%	0.096%
23	16.145	2217	2220	2224	rBV6	5424	8180	0.18%	0.017%
24	16.204	2224	2230	2235	rVB6	8776	15299	0.34%	0.032%
25	16.316	2245	2249	2253	rBV7	2705	4734	0.11%	0.010%
26	16.492	2275	2279	2288	rBV7	5438	14260	0.32%	0.030%
27	16.663	2303	2308	2309	rBV4	3749	4652	0.10%	0.010%
28	16.851	2335	2340	2344	rBV7	3325	4644	0.10%	0.010%
29	16.945	2351	2356	2362	rBV4	11054	25126	0.56%	0.053%
30	17.163	2387	2393	2403	rBV	1775456	2640048	58.85%	5.601%
31	17.263	2403	2410	2425	rVV	2642063	3954589	88.16%	8.389%
32	17.410	2433	2435	2442	rVB8	3329	4663	0.10%	0.010%
33	17.763	2490	2495	2500	rBV8	4405	7945	0.18%	0.017%
34	18.081	2545	2549	2555	rBV9	5035	8467	0.19%	0.018%
35	18.139	2556	2559	2563	rVB4	3475	4823	0.11%	0.010%
36	19.128	2722	2727	2731	rBV	34675	46269	1.03%	0.098%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020168.D
Acq On : 15 Jun 2022 11:03
Operator : CG/JU
Sample : PB145541BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK541

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	19.198	2735	2739	2746	rVV2	30248	44929	1.00%	0.095%
38	19.504	2789	2791	2794	rBV3	5964	7467	0.17%	0.016%
39	19.563	2794	2801	2810	rBV	3145689	4485911	100.00%	9.516%
40	20.575	2970	2973	2978	rBV3	30595	39494	0.88%	0.084%
41	21.357	3101	3106	3114	rBV	2258396	2916307	65.01%	6.187%
42	23.527	3467	3475	3482	rBV	2236047	4443015	99.04%	9.425%
43	23.674	3493	3500	3512	rVB2	1411596	2885359	64.32%	6.121%




Sum of corrected areas: 47139469

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020168.D
Acq On : 15 Jun 2022 11:03
Operator : CG/JU
Sample : PB145541BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK541

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

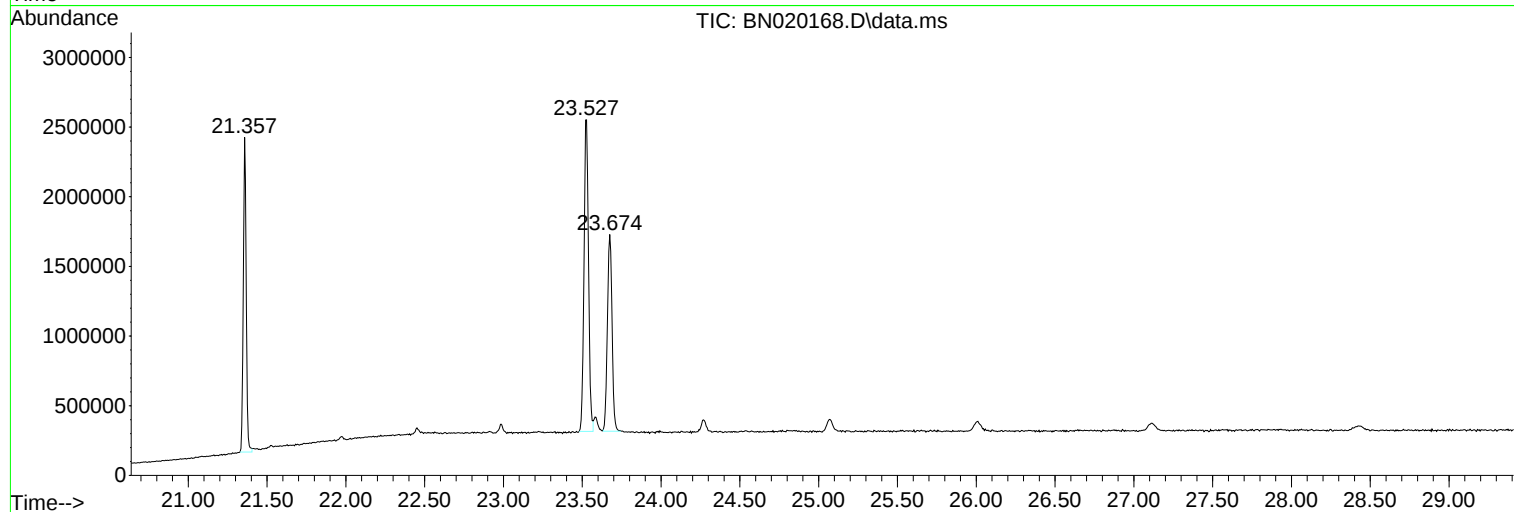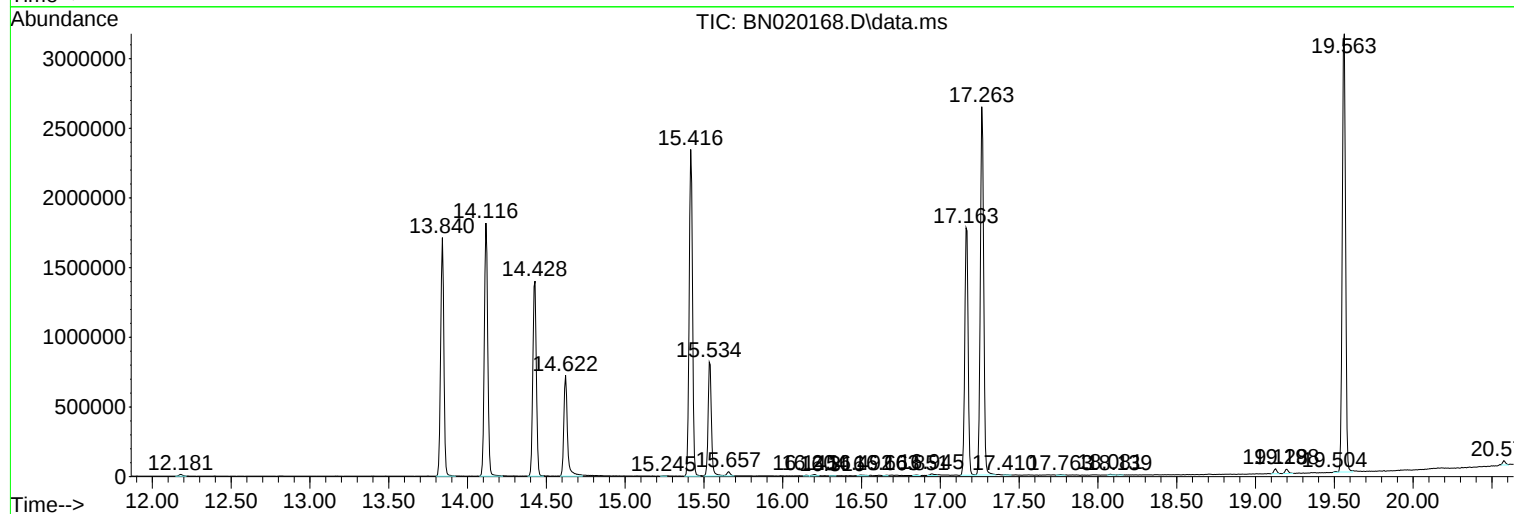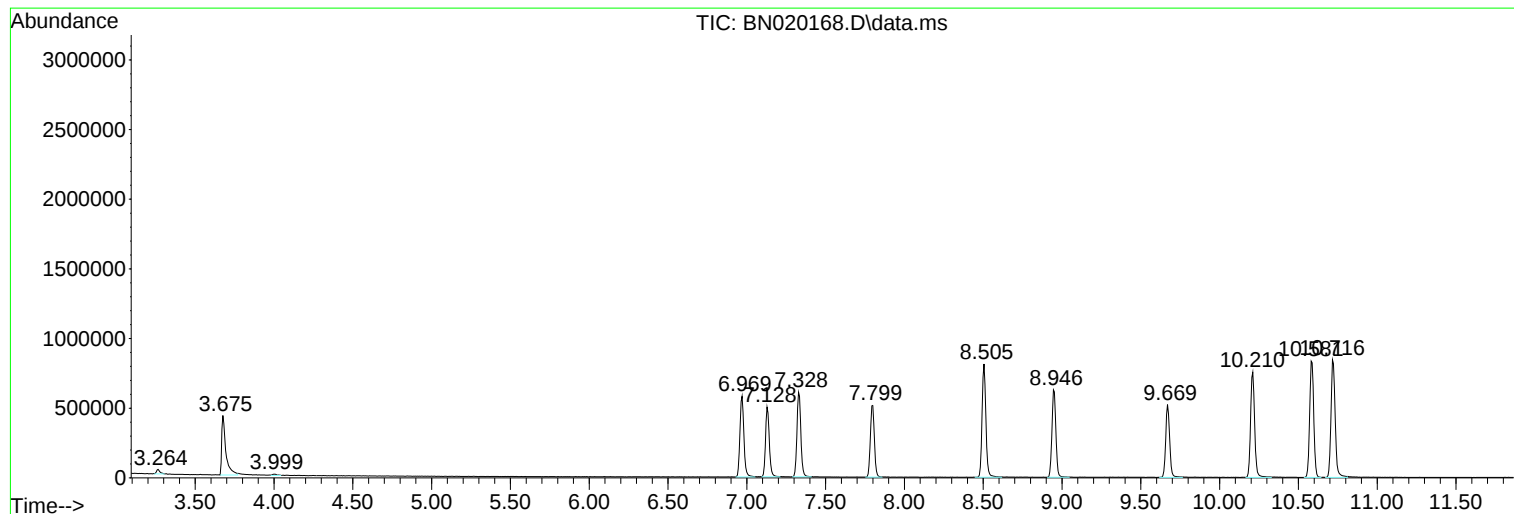

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020168.D
Acq On : 15 Jun 2022 11:03
Operator : CG/JU
Sample : PB145541BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK541

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020168.D
Acq On : 15 Jun 2022 11:03
Operator : CG/JU
Sample : PB145541BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK541

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------