

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020170.D
 Acq On : 15 Jun 2022 12:15
 Operator : CG/JU
 Sample : N3317-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.005	152	156	162	rVB4	4693	8784	0.42%	0.097%
2	7.463	741	744	749	rBV5	1150	2244	0.11%	0.025%
3	7.799	794	801	812	rBV	344575	591358	27.99%	6.533%
4	10.587	1268	1275	1292	rBV	532151	946439	44.79%	10.456%
5	11.946	1503	1506	1509	rBV3	1523	2148	0.10%	0.024%
6	14.428	1921	1928	1941	rBV	967844	1465107	69.34%	16.186%
7	15.440	2094	2100	2106	rBV5	1987	4889	0.23%	0.054%
8	16.151	2216	2221	2224	rBV4	4033	6791	0.32%	0.075%
9	16.181	2224	2226	2233	rVB7	2530	4276	0.20%	0.047%
10	16.322	2246	2250	2254	rVB5	2143	3705	0.18%	0.041%
11	16.363	2254	2257	2259	rBV4	1598	2118	0.10%	0.023%
12	16.498	2275	2280	2283	rBV4	3582	6424	0.30%	0.071%
13	16.557	2288	2290	2294	rVB3	2852	2963	0.14%	0.033%
14	16.610	2297	2299	2304	rVB3	3065	4026	0.19%	0.044%
15	16.663	2304	2308	2310	rBV4	3843	5652	0.27%	0.062%
16	16.692	2311	2313	2317	rVV2	3213	3023	0.14%	0.033%
17	16.728	2317	2319	2323	rVB3	2419	2897	0.14%	0.032%
18	16.945	2351	2356	2361	rBV4	9314	16537	0.78%	0.183%
19	17.163	2387	2393	2405	rBV	1249515	1889202	89.41%	20.871%
20	17.757	2492	2494	2499	rVB6	3084	4023	0.19%	0.044%
21	18.822	2672	2675	2676	rBV3	2431	2810	0.13%	0.031%
22	20.575	2970	2973	2977	rBV4	27644	33378	1.58%	0.369%
23	21.357	3100	3106	3113	rBV	1556980	2112959	100.00%	23.343%
24	23.668	3492	3499	3508	rBV2	942865	1929861	91.33%	21.321%




Sum of corrected areas: 9051614

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020170.D
Acq On : 15 Jun 2022 12:15
Operator : CG/JU
Sample : N3317-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

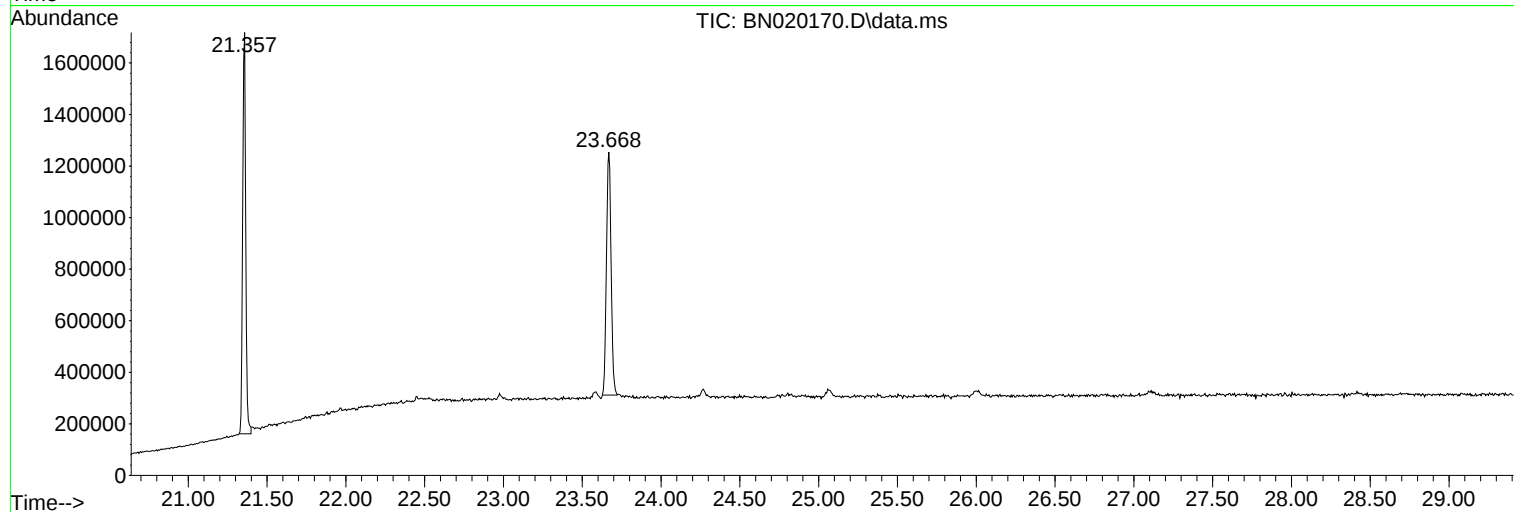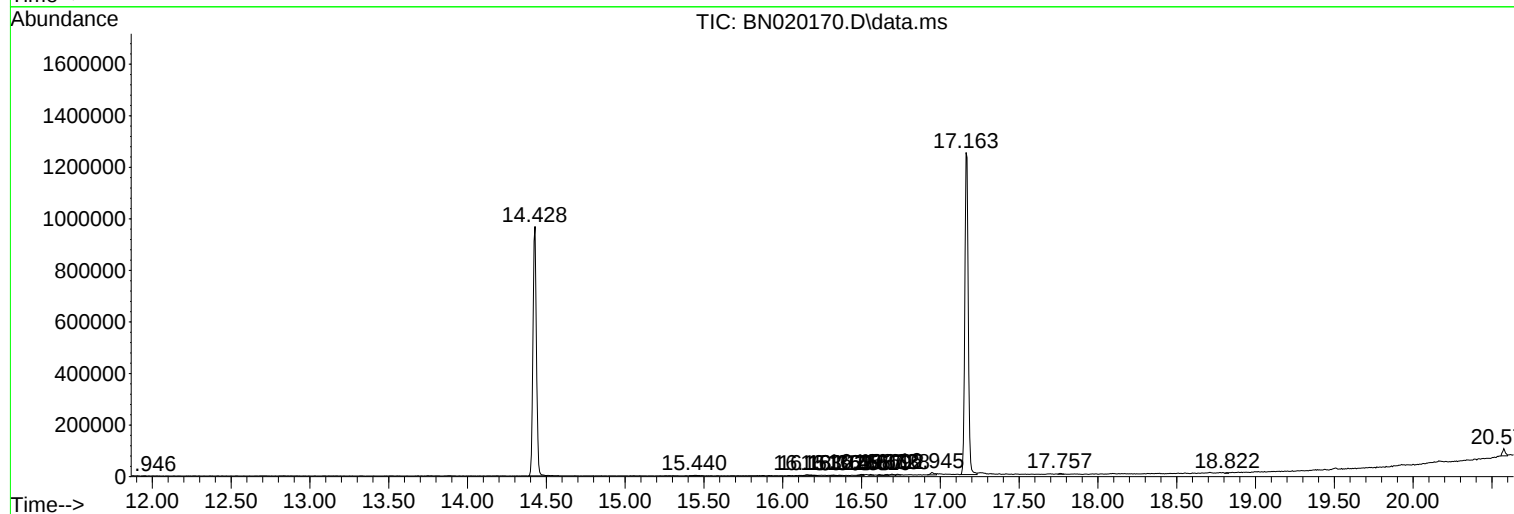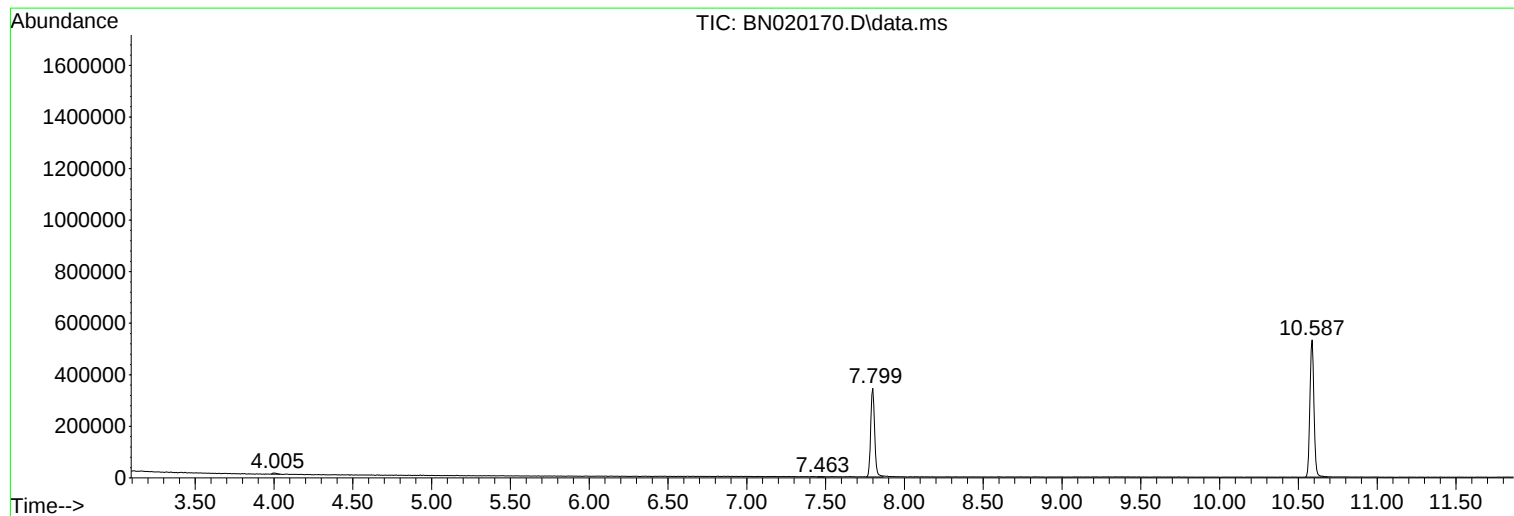

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020170.D
Acq On : 15 Jun 2022 12:15
Operator : CG/JU
Sample : N3317-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020170.D
Acq On : 15 Jun 2022 12:15
Operator : CG/JU
Sample : N3317-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc